

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110424\
 Data File : BP022839.D
 Acq On : 04 Nov 2024 23:04
 Operator : RC/JU
 Sample : P4568-15
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A4EE5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP022839.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.175	30	32	39	rVB2	5152	7128	0.33%	0.046%
2	3.616	104	107	112	rVV2	7819	14522	0.67%	0.094%
3	3.658	112	114	117	rVV4	4318	5930	0.27%	0.038%
4	3.693	117	120	125	rVB4	5022	7314	0.34%	0.047%
5	3.811	135	140	145	rVB8	2334	4459	0.20%	0.029%
6	3.899	151	155	162	rVV2	4860	7996	0.37%	0.052%
7	4.069	178	184	188	rBV8	3285	5236	0.24%	0.034%
8	4.263	215	217	222	rVV6	2481	4071	0.19%	0.026%
9	4.446	244	248	254	rVB6	5855	9595	0.44%	0.062%
10	4.805	300	309	317	rVV4	5445	14161	0.65%	0.092%
11	5.469	418	422	427	rBV3	7364	10537	0.48%	0.068%
12	5.675	452	457	459	rBV6	2823	5282	0.24%	0.034%
13	6.005	507	513	519	rBV	18496	28955	1.33%	0.187%
14	6.046	519	520	526	rVB6	3359	4328	0.20%	0.028%
15	6.228	547	551	553	rBV5	3914	7076	0.32%	0.046%
16	6.446	582	588	592	rBV6	6526	10783	0.49%	0.070%
17	6.499	592	597	604	rVB2	12186	19774	0.91%	0.128%
18	6.581	608	611	619	rVB9	1678	3032	0.14%	0.020%
19	6.775	636	644	645	rBV8	2186	4704	0.22%	0.030%
20	6.828	645	653	670	rVV2	67286	161135	7.39%	1.043%
21	6.975	672	678	686	rVB	55817	89468	4.10%	0.579%
22	7.175	706	712	723	rBV	78484	132492	6.08%	0.857%
23	7.452	754	759	764	rBV5	1739	3113	0.14%	0.020%
24	7.628	781	789	798	rBV	293734	478361	21.94%	3.095%
25	8.269	894	898	903	rVB8	2356	3439	0.16%	0.022%
26	8.340	903	910	922	rBV2	73951	152548	7.00%	0.987%
27	8.446	922	928	937	rVV	77903	135804	6.23%	0.879%
28	8.769	977	983	995	rBV2	70754	129663	5.95%	0.839%
29	9.163	1045	1050	1057	rVB5	5585	8758	0.40%	0.057%
30	9.351	1076	1082	1083	rBV5	2485	3897	0.18%	0.025%
31	9.481	1096	1104	1118	rBV	54105	114411	5.25%	0.740%
32	9.698	1137	1141	1155	rBV4	8820	28483	1.31%	0.184%
33	9.846	1161	1166	1176	rVB2	7250	15810	0.72%	0.102%
34	10.034	1192	1198	1213	rBV2	79273	181588	8.33%	1.175%
35	10.375	1249	1256	1269	rBV	374338	653143	29.95%	4.226%
36	10.545	1278	1285	1298	rBV	27282	69092	3.17%	0.447%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110424\
Data File : BP022839.D
Acq On : 04 Nov 2024 23:04
Operator : RC/JU
Sample : P4568-15
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A4EE5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
Title : SVOA CALIBRATION

37	10.957	1348	1355	1360	rBV10	3858	9724	0.45%	0.063%
38	11.228	1392	1401	1403	rBV6	3787	7561	0.35%	0.049%
39	11.787	1489	1496	1504	rBV7	3238	8339	0.38%	0.054%
40	11.969	1523	1527	1533	rVV7	2776	4634	0.21%	0.030%
41	13.110	1717	1721	1726	rVB7	2171	3223	0.15%	0.021%
42	13.645	1806	1812	1823	rVV	217822	318290	14.60%	2.059%
43	13.928	1854	1860	1870	rBV2	232107	346844	15.90%	2.244%
44	14.063	1881	1883	1889	rVB7	1848	3307	0.15%	0.021%
45	14.245	1902	1914	1920	rBV	700990	1024779	46.99%	6.631%
46	14.304	1920	1924	1931	rVB2	12237	21891	1.00%	0.142%
47	14.539	1957	1964	1973	rBV4	24708	74279	3.41%	0.481%
48	14.663	1981	1985	1988	rBV3	9089	14946	0.69%	0.097%
49	14.881	2017	2022	2026	rBV8	1993	3586	0.16%	0.023%
50	15.263	2079	2087	2093	rBV	313270	488521	22.40%	3.161%
51	15.316	2093	2096	2101	rVB2	20485	27859	1.28%	0.180%
52	15.398	2105	2110	2119	rBV2	35624	65895	3.02%	0.426%
53	15.639	2143	2151	2157	rBV2	65997	89418	4.10%	0.579%
54	15.757	2168	2171	2177	rVB6	5075	8399	0.39%	0.054%
55	15.992	2208	2211	2213	rBV3	3469	4077	0.19%	0.026%
56	16.010	2213	2214	2218	rVV4	3333	3466	0.16%	0.022%
57	16.169	2237	2241	2246	rVB2	9814	15287	0.70%	0.099%
58	16.345	2268	2271	2275	rVB6	4095	5812	0.27%	0.038%
59	16.398	2276	2280	2283	rVB5	2814	3566	0.16%	0.023%
60	16.445	2284	2288	2293	rBV8	2849	5403	0.25%	0.035%
61	16.580	2308	2311	2315	rBV6	2674	3696	0.17%	0.024%
62	16.710	2328	2333	2339	rVB8	5574	9471	0.43%	0.061%
63	16.786	2341	2346	2351	rBV7	6847	12313	0.56%	0.080%
64	16.851	2354	2357	2364	rVB	12606	18291	0.84%	0.118%
65	16.963	2372	2376	2380	rBV7	4496	7969	0.37%	0.052%
66	17.051	2383	2391	2394	rBV	1015113	1379245	63.25%	8.924%
67	17.086	2394	2397	2402	rVB	369262	421637	19.33%	2.728%
68	17.145	2402	2407	2412	rBV2	292264	508231	23.31%	3.288%
69	17.269	2425	2428	2436	rVB6	6281	9982	0.46%	0.065%
70	17.480	2459	2464	2474	rVV	17926	34159	1.57%	0.221%
71	17.586	2478	2482	2487	rVB6	4786	7677	0.35%	0.050%
72	17.733	2505	2507	2513	rVB6	4521	6945	0.32%	0.045%
73	17.857	2522	2528	2536	rBV10	8175	17953	0.82%	0.116%
74	17.951	2540	2544	2546	rBV	24308	33055	1.52%	0.214%
75	17.986	2546	2550	2559	rVB2	122865	205045	9.40%	1.327%
76	18.086	2564	2567	2571	rVV5	11751	21390	0.98%	0.138%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110424\
 Data File : BP022839.D
 Acq On : 04 Nov 2024 23:04
 Operator : RC/JU
 Sample : P4568-15
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A4EE5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
 Title : SVOA CALIBRATION

77	18.151	2572	2578	2582	rVV2	48521	93872	4.30%	0.607%
78	18.192	2582	2585	2593	rVB2	18252	33924	1.56%	0.220%
79	18.469	2629	2632	2637	rBV	22081	33066	1.52%	0.214%
80	18.527	2639	2642	2646	rVV3	15500	20518	0.94%	0.133%
81	18.727	2673	2676	2681	rBV7	7169	9454	0.43%	0.061%
82	18.804	2683	2689	2694	rBV2	23243	44131	2.02%	0.286%
83	18.851	2694	2697	2702	rVB3	15646	21273	0.98%	0.138%
84	18.910	2703	2707	2711	rVV4	9678	14758	0.68%	0.095%
85	19.074	2730	2735	2739	rBV8	21004	42764	1.96%	0.277%
86	19.174	2747	2752	2759	rVB	593487	865050	39.67%	5.597%
87	19.316	2772	2776	2781	rBV3	40866	63343	2.90%	0.410%
88	19.527	2806	2812	2814	rBV	467058	614018	28.16%	3.973%
89	19.557	2814	2817	2828	rVV	287699	416739	19.11%	2.696%
90	19.651	2829	2833	2838	rVB3	19353	29854	1.37%	0.193%
91	19.757	2848	2851	2858	rVB2	26317	34899	1.60%	0.226%
92	20.086	2904	2907	2911	rVB	73103	91163	4.18%	0.590%
93	20.192	2921	2925	2930	rBV	61385	82422	3.78%	0.533%
94	21.057	3069	3072	3076	rBV	37837	53305	2.44%	0.345%
95	21.151	3084	3088	3090	rBV3	34647	53732	2.46%	0.348%
96	21.480	3136	3144	3150	rBV2	1145214	2180769	100.00%	14.110%
97	21.527	3150	3152	3160	rVB	190187	314083	14.40%	2.032%
98	23.698	3516	3521	3529	rBV	165236	462675	21.22%	2.994%
99	24.492	3651	3656	3664	rBV2	128254	311862	14.30%	2.018%
100	24.727	3687	3696	3706	rVB	652721	1775043	81.40%	11.485%

Sum of corrected areas: 15454970




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110424\
Data File : BP022839.D
Acq On : 04 Nov 2024 23:04
Operator : RC/JU
Sample : P4568-15
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A4EE5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L

TIC Integration Parameters: LSCINT.P

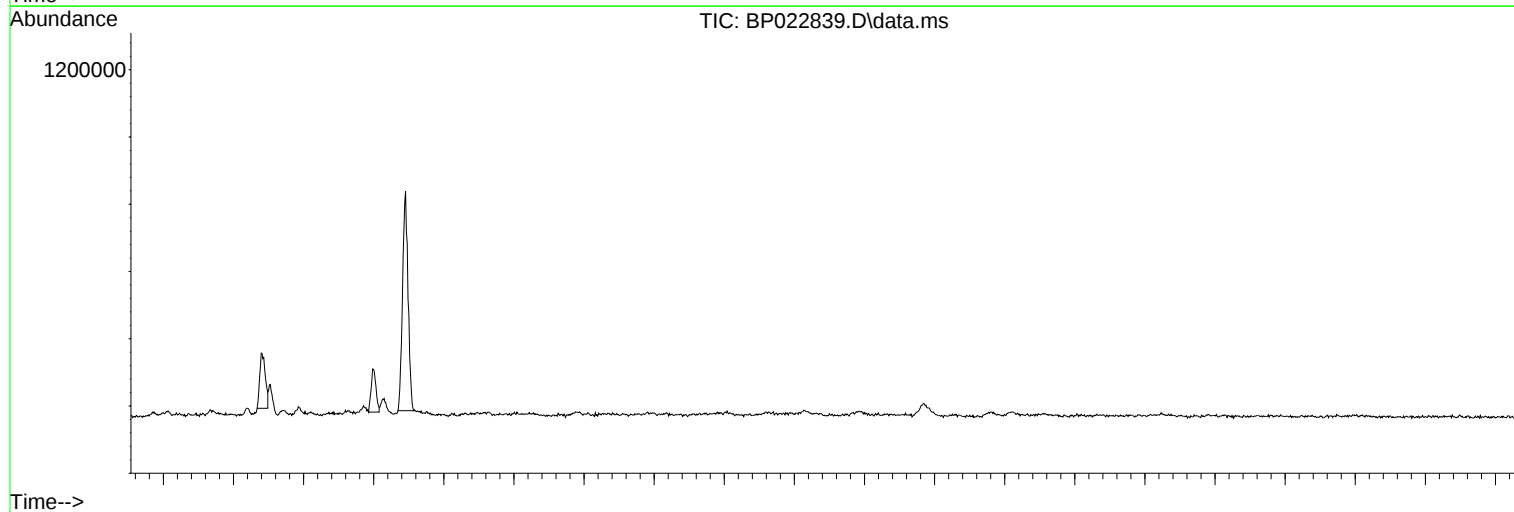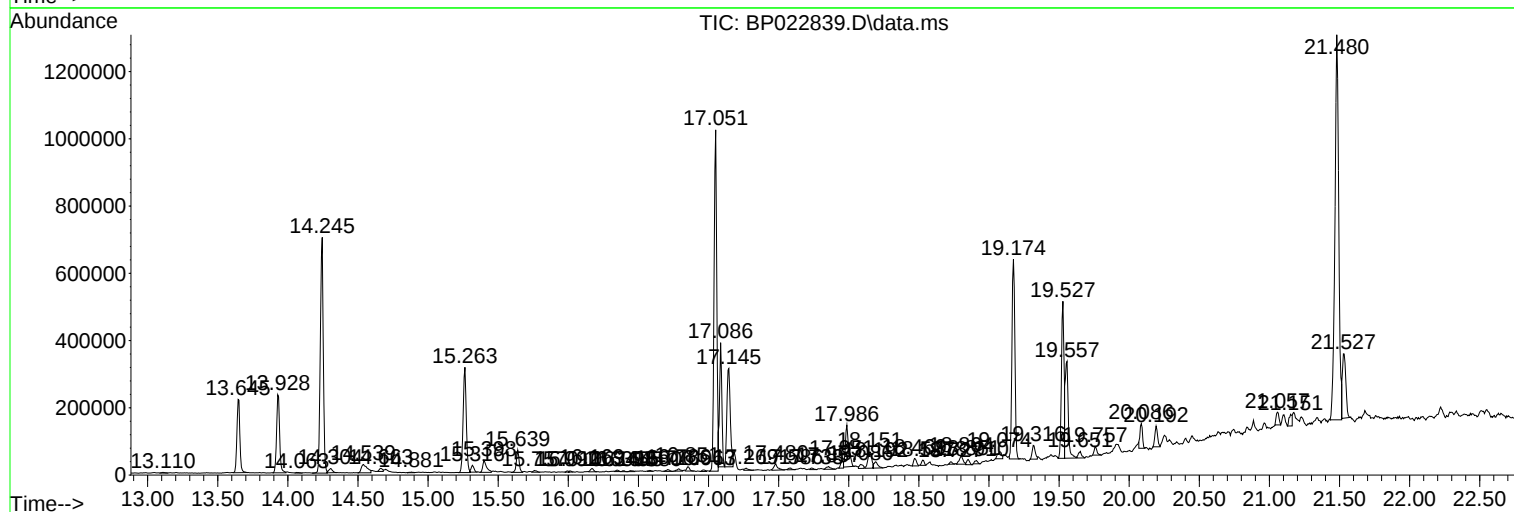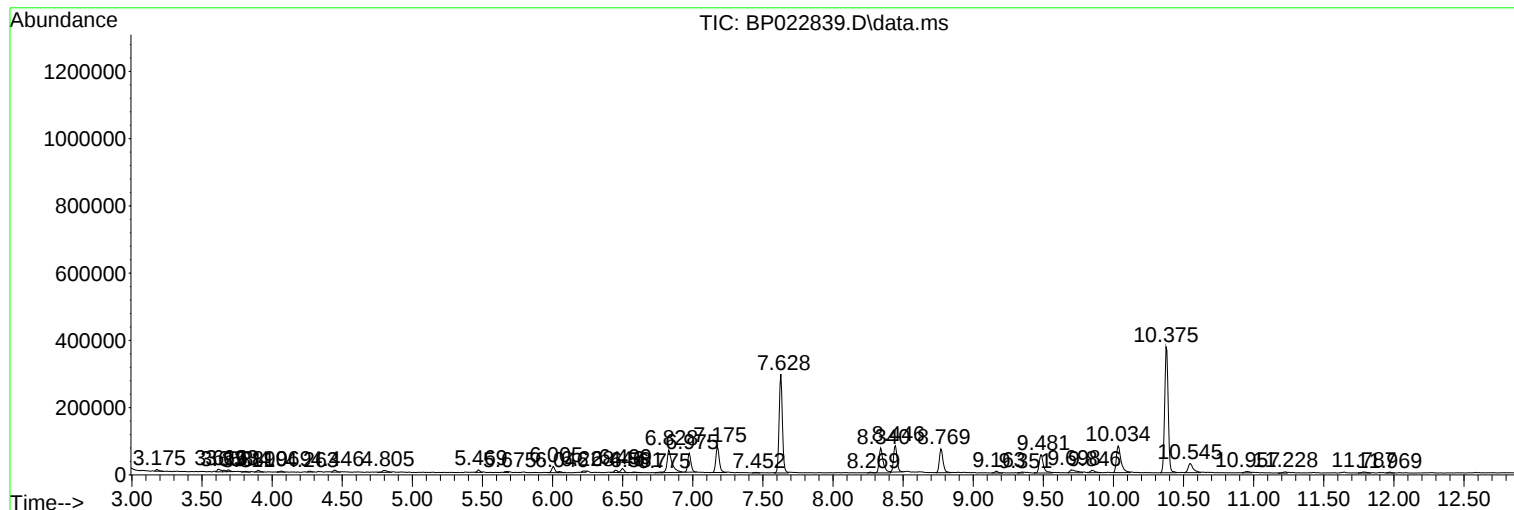

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110424\
Data File : BP022839.D
Acq On : 04 Nov 2024 23:04
Operator : RC/JU
Sample : P4568-15
Misc :
ALS Vial : 18 Sample Multiplier: 1










Instrument :
BNA_P
ClientSampleId :
A4EE5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 n-Hexadecanoic acid Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD		R.T.	
17.986	2.97 ng/ul	205045	Phenanthrene-d10		17.051	
Hit# of 5	Tentative ID		MW	MolForm	CAS#	Qual
1	n-Hexadecanoic acid		256	C16H32O2	000057-10-3	96
2	n-Hexadecanoic acid		256	C16H32O2	000057-10-3	94
3	n-Hexadecanoic acid		256	C16H32O2	000057-10-3	91
4	Tridecanoic acid		214	C13H26O2	000638-53-9	83
5	n-Hexadecanoic acid		256	C16H32O2	000057-10-3	76

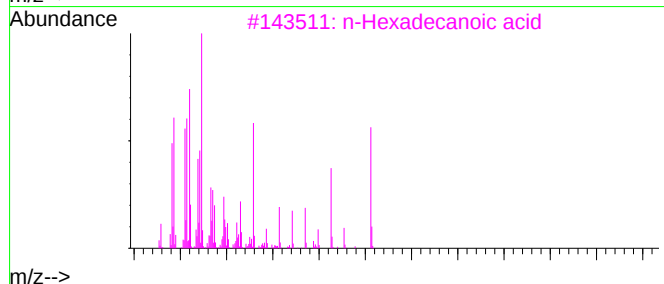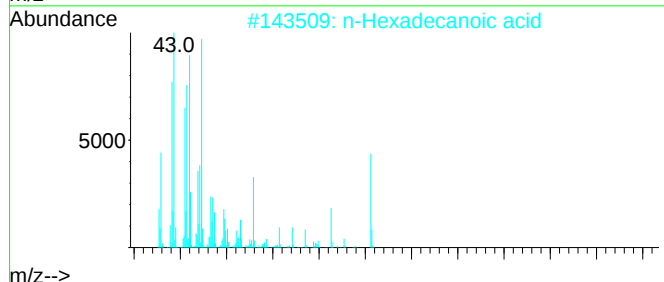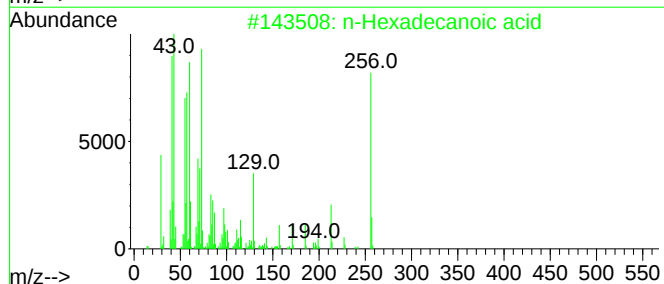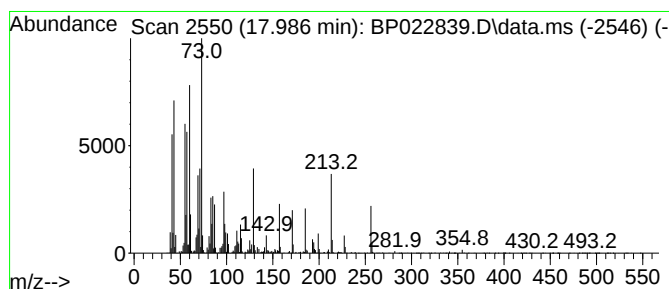

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110424\
Data File : BP022839.D
Acq On : 04 Nov 2024 23:04
Operator : RC/JU
Sample : P4568-15
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A4EE5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
n-Hexadecanoic ...	17.986	3.0	ng/ul	205045	4	17.051	1379250	20.0