

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110424\
 Data File : BP022841.D
 Acq On : 05 Nov 2024 00:25
 Operator : RC/JU
 Sample : P4581-22
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A4EB4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP022841.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.187	30	34	36	rBV4	3642	4176	0.22%	0.036%
2	3.611	103	106	116	rBV2	9854	20757	1.11%	0.180%
3	3.693	116	120	129	rVB2	6096	10737	0.58%	0.093%
4	3.905	152	156	160	rVB4	3834	6198	0.33%	0.054%
5	4.063	179	183	185	rBV4	1247	1922	0.10%	0.017%
6	4.122	190	193	199	rVV8	4436	6318	0.34%	0.055%
7	4.269	215	218	223	rVB7	3028	4416	0.24%	0.038%
8	4.399	235	240	244	rBV	8425	11681	0.63%	0.102%
9	4.522	255	261	266	rBV9	2589	5344	0.29%	0.046%
10	4.799	303	308	313	rBV2	6584	13021	0.70%	0.113%
11	5.475	420	423	427	rBV5	1415	1992	0.11%	0.017%
12	5.675	451	457	458	rBV5	2029	3433	0.18%	0.030%
13	5.999	509	512	517	rVB7	2358	3730	0.20%	0.032%
14	6.310	561	565	566	rBV4	2523	2823	0.15%	0.025%
15	6.452	585	589	593	rBV7	1777	3003	0.16%	0.026%
16	6.493	594	596	603	rVB7	2141	3466	0.19%	0.030%
17	6.763	640	642	646	rBV4	1652	2124	0.11%	0.018%
18	6.828	646	653	669	rVV	57495	135647	7.29%	1.179%
19	6.975	672	678	690	rVV	53302	86917	4.67%	0.756%
20	7.175	706	712	720	rBV	67747	116191	6.24%	1.010%
21	7.252	723	725	730	rVB6	1699	2130	0.11%	0.019%
22	7.622	781	788	799	rBV	284216	478323	25.69%	4.159%
23	8.346	904	911	921	rBV2	46813	103976	5.58%	0.904%
24	8.440	921	927	939	rVB	59399	115694	6.21%	1.006%
25	8.628	957	959	964	rVB5	1886	1967	0.11%	0.017%
26	8.769	976	983	996	rBV	62196	116178	6.24%	1.010%
27	9.163	1045	1050	1055	rVB4	5523	9236	0.50%	0.080%
28	9.357	1078	1083	1084	rBV5	1925	3017	0.16%	0.026%
29	9.481	1096	1104	1116	rBV	49427	98180	5.27%	0.854%
30	9.722	1135	1145	1151	rBV3	6947	20259	1.09%	0.176%
31	9.846	1161	1166	1172	rVB4	5941	10277	0.55%	0.089%
32	10.040	1190	1199	1211	rBV	66914	158944	8.54%	1.382%
33	10.381	1250	1257	1272	rBV	387985	653245	35.09%	5.680%
34	10.540	1278	1284	1297	rBV	45108	100475	5.40%	0.874%
35	11.228	1395	1401	1403	rBV6	2645	4819	0.26%	0.042%
36	11.645	1466	1472	1477	rBV6	3628	6575	0.35%	0.057%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110424\
 Data File : BP022841.D
 Acq On : 05 Nov 2024 00:25
 Operator : RC/JU
 Sample : P4581-22
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A4EB4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
 Title : SVOA CALIBRATION

37	11.975	1526	1528	1536	rVB7	1659	2927	0.16%	0.025%
38	12.839	1672	1675	1678	rBV5	1425	2077	0.11%	0.018%
39	13.334	1757	1759	1767	rVB9	1120	2530	0.14%	0.022%
40	13.645	1806	1812	1826	rBV	206590	287614	15.45%	2.501%
41	13.939	1850	1862	1873	rBV	221062	304534	16.36%	2.648%
42	14.251	1908	1915	1922	rVV	720918	1027781	55.20%	8.937%
43	14.534	1958	1963	1977	rBV4	26827	82978	4.46%	0.722%
44	14.692	1983	1990	1991	rBV6	4336	8718	0.47%	0.076%
45	14.710	1991	1993	1998	rVB6	4258	5539	0.30%	0.048%
46	15.057	2048	2052	2056	rVB7	2148	2683	0.14%	0.023%
47	15.269	2080	2088	2096	rBV	234555	439043	23.58%	3.818%
48	15.410	2106	2112	2122	rBV	44415	71999	3.87%	0.626%
49	15.639	2144	2151	2158	rBV	42641	61733	3.32%	0.537%
50	16.022	2213	2216	2223	rVB8	2911	4373	0.23%	0.038%
51	16.533	2296	2303	2307	rVB9	2717	5547	0.30%	0.048%
52	16.598	2307	2314	2320	rBV7	3823	7835	0.42%	0.068%
53	16.786	2342	2346	2348	rBV5	1515	2614	0.14%	0.023%
54	16.927	2367	2370	2375	rVB6	2281	3507	0.19%	0.030%
55	16.986	2375	2380	2382	rBV6	3257	5168	0.28%	0.045%
56	17.057	2385	2392	2397	rBV	949017	1413692	75.93%	12.292%
57	17.157	2403	2409	2421	rVB2	314866	468399	25.16%	4.073%
58	17.557	2475	2477	2479	rBV3	2316	2169	0.12%	0.019%
59	17.575	2479	2480	2483	rVB3	3045	2436	0.13%	0.021%
60	17.692	2494	2500	2505	rVB9	7707	14610	0.78%	0.127%
61	17.751	2507	2510	2515	rBV7	6127	8644	0.46%	0.075%
62	17.857	2524	2528	2529	rBV4	3920	4550	0.24%	0.040%
63	17.992	2546	2551	2560	rBV2	92537	133276	7.16%	1.159%
64	18.069	2560	2564	2568	rVV7	4554	7807	0.42%	0.068%
65	18.163	2575	2580	2584	rBV7	12028	19343	1.04%	0.168%
66	18.463	2627	2631	2633	rBV5	6559	9381	0.50%	0.082%
67	18.539	2641	2644	2647	rBV5	4820	7951	0.43%	0.069%
68	18.680	2666	2668	2670	rBV3	4082	3415	0.18%	0.030%
69	18.816	2687	2691	2695	rBV	19007	26702	1.43%	0.232%
70	18.863	2696	2699	2704	rVB3	12865	15711	0.84%	0.137%
71	18.939	2709	2712	2719	rVB8	13369	27557	1.48%	0.240%
72	19.192	2751	2755	2760	rVB	71969	96774	5.20%	0.841%
73	19.327	2774	2778	2785	rBV5	36290	55045	2.96%	0.479%
74	19.539	2808	2814	2823	rBV2	311396	490768	26.36%	4.267%
75	20.557	2984	2987	2993	rVB	53871	71142	3.82%	0.619%
76	21.098	3077	3079	3085	rBV6	27759	44198	2.37%	0.384%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110424\
Data File : BP022841.D
Acq On : 05 Nov 2024 00:25
Operator : RC/JU
Sample : P4581-22
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A4EB4

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
Title : SVOA CALIBRATION

77	21.486	3138	3145	3150	rBV	1180885	1810233	97.23%	15.740%
78	24.504	3653	3658	3668	rVB	110852	248734	13.36%	2.163%
79	24.721	3687	3695	3706	rVB	760500	1861754	100.00%	16.188%

Sum of corrected areas: 11500682




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110424\
Data File : BP022841.D
Acq On : 05 Nov 2024 00:25
Operator : RC/JU
Sample : P4581-22
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A4EB4

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L

TIC Integration Parameters: LSCINT.P

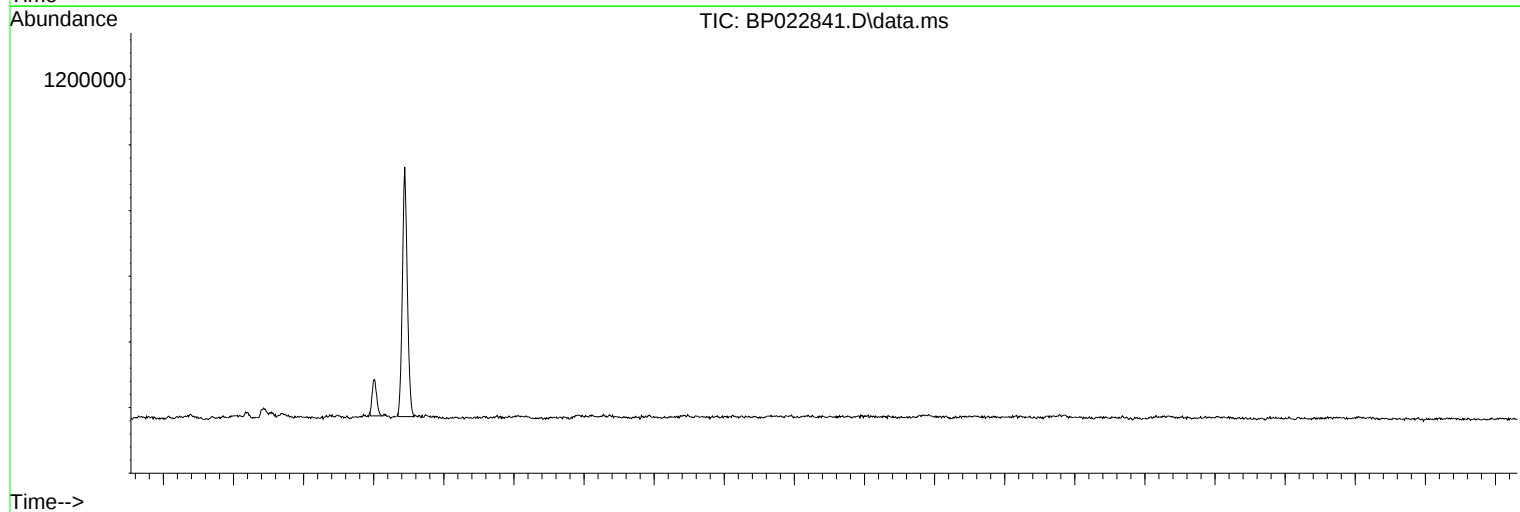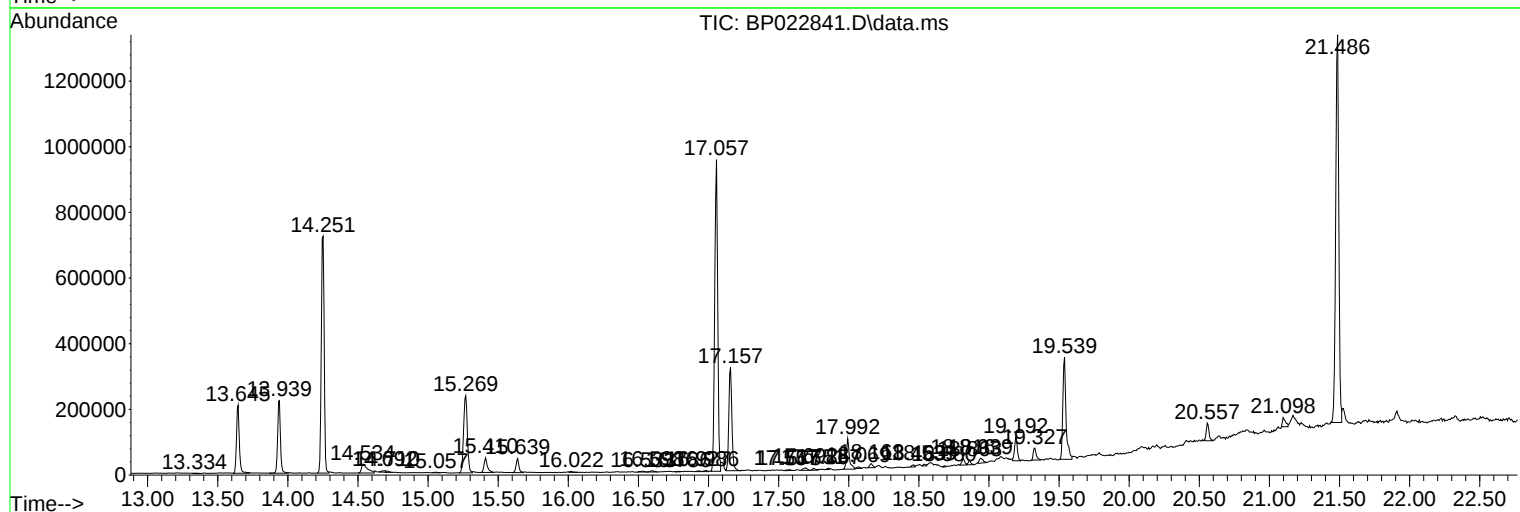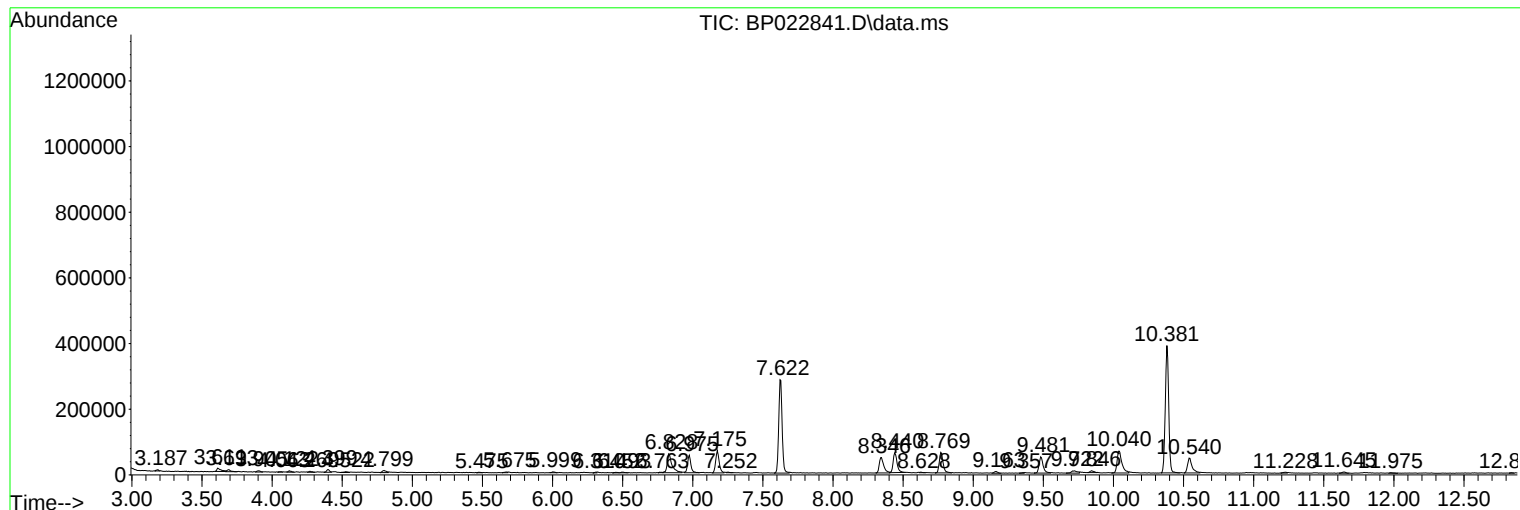

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110424\
Data File : BP022841.D
Acq On : 05 Nov 2024 00:25
Operator : RC/JU
Sample : P4581-22
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A4EB4

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110424\
Data File : BP022841.D
Acq On : 05 Nov 2024 00:25
Operator : RC/JU
Sample : P4581-22
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A4EB4

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc
