

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110424\
 Data File : BP022863.D
 Acq On : 05 Nov 2024 16:50
 Operator : RC/JU
 Sample : P4671-02
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0AB1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP022863.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.175	29	32	38	rBV	13590	18139	0.59%	0.071%
2	3.593	99	103	118	rBV	81183	146039	4.78%	0.568%
3	3.899	151	155	161	rVB	8486	12389	0.41%	0.048%
4	4.264	210	217	220	rBV8	4183	8406	0.28%	0.033%
5	4.399	236	240	246	rVB4	5194	8292	0.27%	0.032%
6	6.311	560	565	572	rBV4	5304	9598	0.31%	0.037%
7	6.828	647	653	669	rVV2	81409	161676	5.29%	0.629%
8	6.969	670	677	692	rVB	227438	361355	11.83%	1.406%
9	7.169	705	711	723	rBV	289398	486495	15.93%	1.893%
10	7.281	727	730	733	rVB5	3080	4264	0.14%	0.017%
11	7.622	781	788	801	rBV	335762	521773	17.09%	2.031%
12	8.334	902	909	925	rBV	254951	466307	15.27%	1.815%
13	8.769	975	983	996	rBV	324361	566035	18.54%	2.203%
14	8.904	1000	1006	1019	rVB2	12648	28591	0.94%	0.111%
15	9.163	1046	1050	1056	rVB5	6120	9423	0.31%	0.037%
16	9.481	1097	1104	1116	rBV	297596	509955	16.70%	1.985%
17	10.022	1187	1196	1212	rBV	398602	790333	25.88%	3.076%
18	10.181	1217	1223	1233	rBV4	12212	37255	1.22%	0.145%
19	10.381	1250	1257	1269	rVB	454973	734217	24.04%	2.858%
20	10.522	1273	1281	1297	rBV	318988	639439	20.94%	2.489%
21	11.646	1464	1472	1479	rBV2	8190	14902	0.49%	0.058%
22	11.987	1523	1530	1535	rBV4	5408	11280	0.37%	0.044%
23	12.828	1670	1673	1678	rBV6	2481	4426	0.14%	0.017%
24	13.198	1728	1736	1738	rBV9	2090	3154	0.10%	0.012%
25	13.651	1806	1813	1827	rBV	743435	1280541	41.93%	4.984%
26	13.934	1848	1861	1877	rBV2	793725	1380022	45.19%	5.371%
27	14.245	1907	1914	1925	rBV	753822	1133187	37.11%	4.410%
28	14.516	1952	1960	1974	rBV3	46402	153517	5.03%	0.597%
29	14.710	1989	1993	2000	rVB10	4870	9734	0.32%	0.038%
30	15.063	2051	2053	2057	rBV2	3982	5669	0.19%	0.022%
31	15.251	2078	2085	2098	rBV	1408987	1924367	63.02%	7.489%
32	15.416	2106	2113	2125	rBV	289226	495998	16.24%	1.930%
33	15.510	2125	2129	2135	rVB5	7178	13058	0.43%	0.051%
34	15.628	2142	2149	2157	rVB	14126	23379	0.77%	0.091%
35	16.010	2210	2214	2219	rVB7	1948	3069	0.10%	0.012%
36	16.186	2242	2244	2254	rVB10	3022	5497	0.18%	0.021%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110424\
 Data File : BP022863.D
 Acq On : 05 Nov 2024 16:50
 Operator : RC/JU
 Sample : P4671-02
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0AB1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
 Title : SVOA CALIBRATION

37	16.534	2298	2303	2307	rBV7	2542	4863	0.16%	0.019%
38	16.833	2349	2354	2363	rVB7	3544	8898	0.29%	0.035%
39	17.051	2383	2391	2400	rBV	1092110	1501145	49.16%	5.842%
40	17.157	2401	2409	2423	rVV	1561763	2391504	78.31%	9.308%
41	17.281	2426	2430	2436	rVV8	7032	13104	0.43%	0.051%
42	17.351	2439	2442	2446	rVB6	4449	6065	0.20%	0.024%
43	17.751	2508	2510	2517	rVB8	4437	5773	0.19%	0.022%
44	17.986	2545	2550	2558	rBV2	27526	52605	1.72%	0.205%
45	18.057	2558	2562	2567	rVB	8201	13869	0.45%	0.054%
46	19.092	2734	2738	2742	rVB3	18275	26302	0.86%	0.102%
47	19.163	2746	2750	2754	rBV	21598	31058	1.02%	0.121%
48	19.322	2774	2777	2782	rVB7	10876	14224	0.47%	0.055%
49	19.539	2808	2814	2823	rBV	2201258	2962605	97.02%	11.530%
50	21.498	3141	3147	3158	rVB2	1023004	1785143	58.46%	6.948%
51	24.527	3652	3662	3675	rVB	1164230	3053741	100.00%	11.885%
52	24.751	3691	3700	3715	rVB	753078	1841612	60.31%	7.167%




Sum of corrected areas: 25694292

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110424\
Data File : BP022863.D
Acq On : 05 Nov 2024 16:50
Operator : RC/JU
Sample : P4671-02
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AB1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

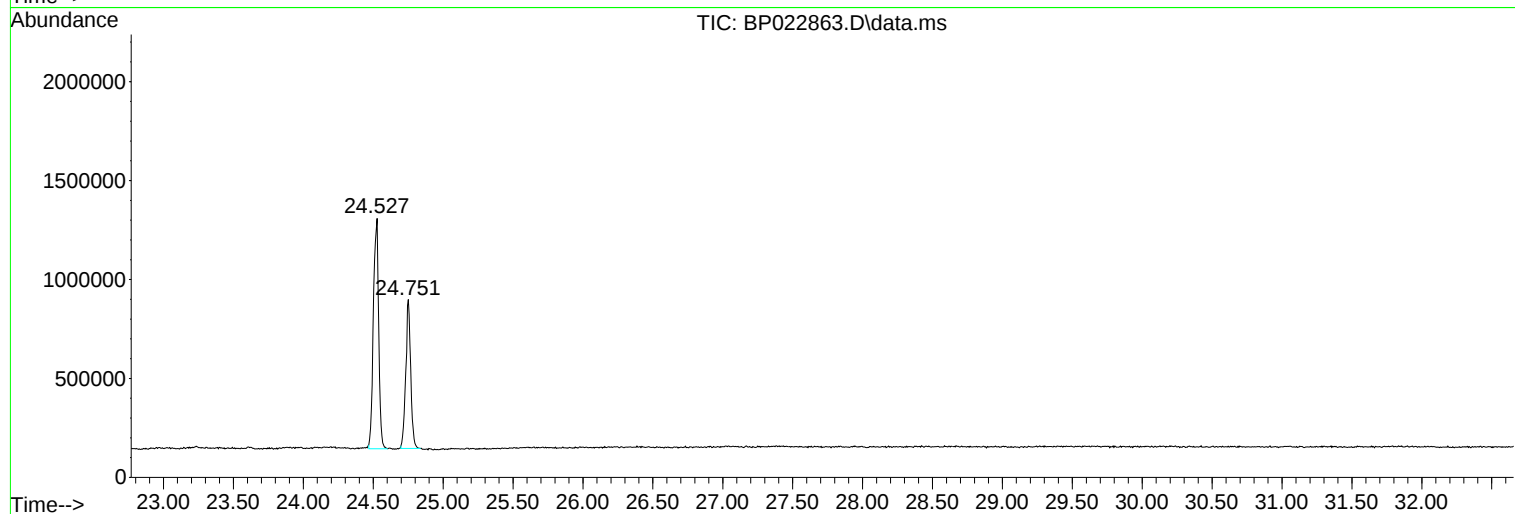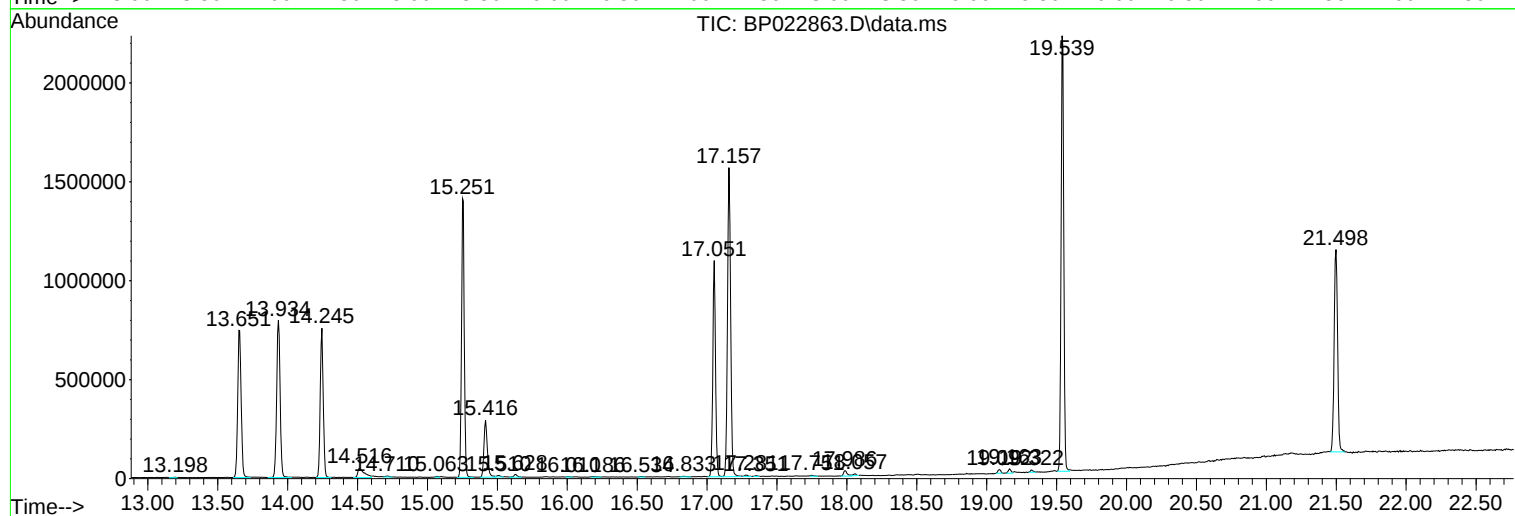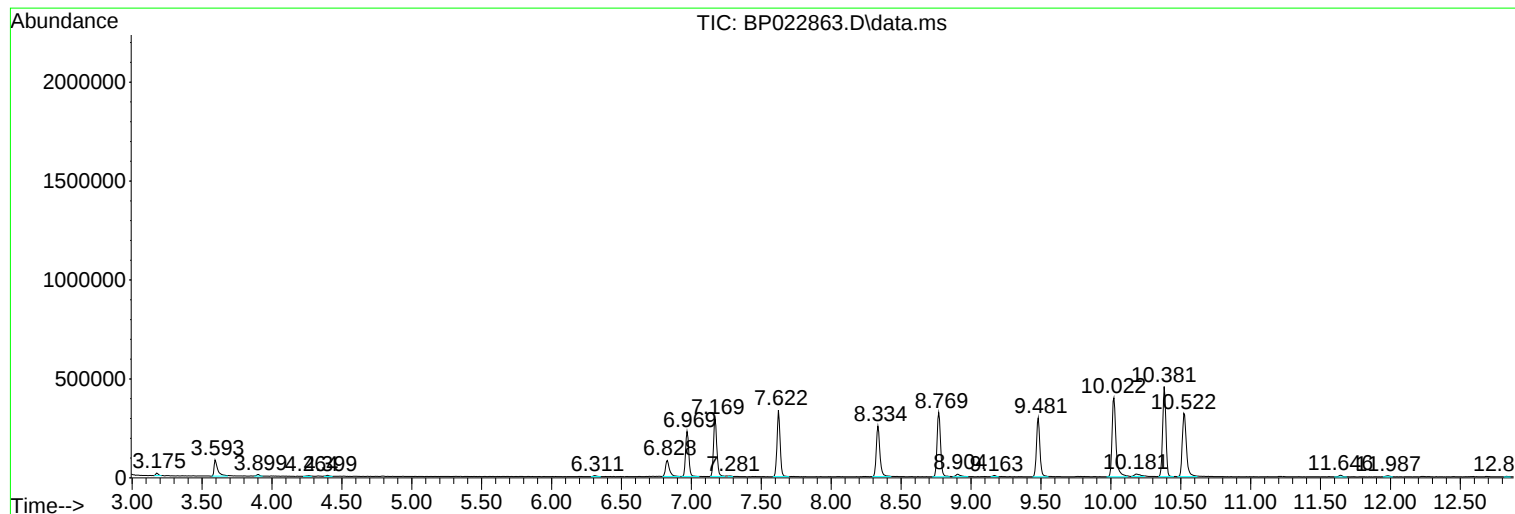

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110424\
Data File : BP022863.D
Acq On : 05 Nov 2024 16:50
Operator : RC/JU
Sample : P4671-02
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AB1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110424\
Data File : BP022863.D
Acq On : 05 Nov 2024 16:50
Operator : RC/JU
Sample : P4671-02
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AB1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc