

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110424\
 Data File : BP022864.D
 Acq On : 05 Nov 2024 17:31
 Operator : RC/JU
 Sample : P4671-03
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0AB2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP022864.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.175	28	32	40	rVB	12638	17762	0.58%	0.080%
2	3.599	100	104	116	rBV	25742	54167	1.77%	0.244%
3	3.893	152	154	161	rVB6	3728	5813	0.19%	0.026%
4	4.258	213	216	221	rBV5	2845	4738	0.15%	0.021%
5	4.340	224	230	231	rBV5	1813	3311	0.11%	0.015%
6	6.316	560	566	571	rBV9	3210	6383	0.21%	0.029%
7	6.828	647	653	670	rVB	66798	134679	4.40%	0.608%
8	6.969	670	677	686	rBV	195663	307865	10.07%	1.390%
9	7.169	705	711	721	rBV	245004	408768	13.37%	1.845%
10	7.622	780	788	801	rBV	233040	378920	12.39%	1.710%
11	8.334	902	909	926	rBV2	198945	388402	12.70%	1.753%
12	8.522	935	941	947	rBV10	1410	3455	0.11%	0.016%
13	8.769	976	983	1000	rBV	268845	458978	15.01%	2.072%
14	8.899	1000	1005	1013	rBV3	9382	19822	0.65%	0.089%
15	9.063	1027	1033	1035	rBV6	2223	4165	0.14%	0.019%
16	9.163	1046	1050	1056	rVB7	4928	6873	0.22%	0.031%
17	9.481	1096	1104	1118	rBV	256524	423371	13.85%	1.911%
18	9.763	1144	1152	1155	rBV8	2170	4338	0.14%	0.020%
19	10.016	1186	1195	1215	rBV	309736	656102	21.46%	2.961%
20	10.193	1218	1225	1238	rVV3	16292	52587	1.72%	0.237%
21	10.375	1249	1256	1266	rVB	289507	516685	16.90%	2.332%
22	10.528	1275	1282	1295	rBV2	138834	301741	9.87%	1.362%
23	11.216	1395	1399	1403	rBV7	2533	4366	0.14%	0.020%
24	11.646	1467	1472	1479	rVB9	2799	5394	0.18%	0.024%
25	11.981	1523	1529	1538	rBV3	5128	9994	0.33%	0.045%
26	12.216	1562	1569	1576	rBV5	5596	12255	0.40%	0.055%
27	13.663	1806	1815	1827	rBV	699152	1141084	37.32%	5.150%
28	13.934	1852	1861	1876	rBV2	628747	1175668	38.45%	5.306%
29	14.245	1907	1914	1925	rVB	465439	824894	26.98%	3.723%
30	14.522	1954	1961	1982	rBV2	50927	164912	5.39%	0.744%
31	14.934	2027	2031	2038	rVB9	1532	3502	0.11%	0.016%
32	15.063	2049	2053	2062	rBV2	4283	8064	0.26%	0.036%
33	15.257	2080	2086	2096	rBV	1336449	1681752	55.00%	7.591%
34	15.410	2105	2112	2126	rBV	302049	518144	16.94%	2.339%
35	15.510	2127	2129	2135	rVB4	6067	9079	0.30%	0.041%
36	15.634	2145	2150	2162	rVB2	27712	42000	1.37%	0.190%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110424\
 Data File : BP022864.D
 Acq On : 05 Nov 2024 17:31
 Operator : RC/JU
 Sample : P4671-03
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0AB2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
 Title : SVOA CALIBRATION

37	15.851	2182	2187	2192	rBV10	2842	5305	0.17%	0.024%
38	15.998	2209	2212	2217	rVV7	3475	6066	0.20%	0.027%
39	16.057	2220	2222	2227	rVB6	3221	3815	0.12%	0.017%
40	16.469	2287	2292	2294	rVB5	2245	3148	0.10%	0.014%
41	16.528	2299	2302	2305	rVB5	2682	3750	0.12%	0.017%
42	16.716	2331	2334	2339	rVB7	2565	4480	0.15%	0.020%
43	17.051	2384	2391	2397	rBV	903336	1137729	37.21%	5.135%
44	17.145	2400	2407	2423	rBV2	1301966	2186979	71.52%	9.871%
45	17.357	2438	2443	2446	rBV6	4241	6557	0.21%	0.030%
46	17.980	2545	2549	2556	rBV2	50690	78595	2.57%	0.355%
47	18.057	2558	2562	2565	rVB2	8510	11204	0.37%	0.051%
48	18.510	2635	2639	2641	rBV5	4190	5958	0.19%	0.027%
49	19.086	2733	2737	2741	rBV3	20508	27851	0.91%	0.126%
50	19.157	2746	2749	2753	rBV	21506	24987	0.82%	0.113%
51	19.327	2774	2778	2785	rBV2	34855	49914	1.63%	0.225%
52	19.539	2807	2814	2821	rBV	2110113	2835898	92.74%	12.800%
53	21.498	3141	3147	3157	rBV2	863897	1440742	47.12%	6.503%
54	24.533	3653	3663	3678	rVB	1153979	3057814	100.00%	13.801%
55	24.757	3692	3701	3716	rVB	577102	1504934	49.22%	6.793%




Sum of corrected areas: 22155759

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110424\
Data File : BP022864.D
Acq On : 05 Nov 2024 17:31
Operator : RC/JU
Sample : P4671-03
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AB2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

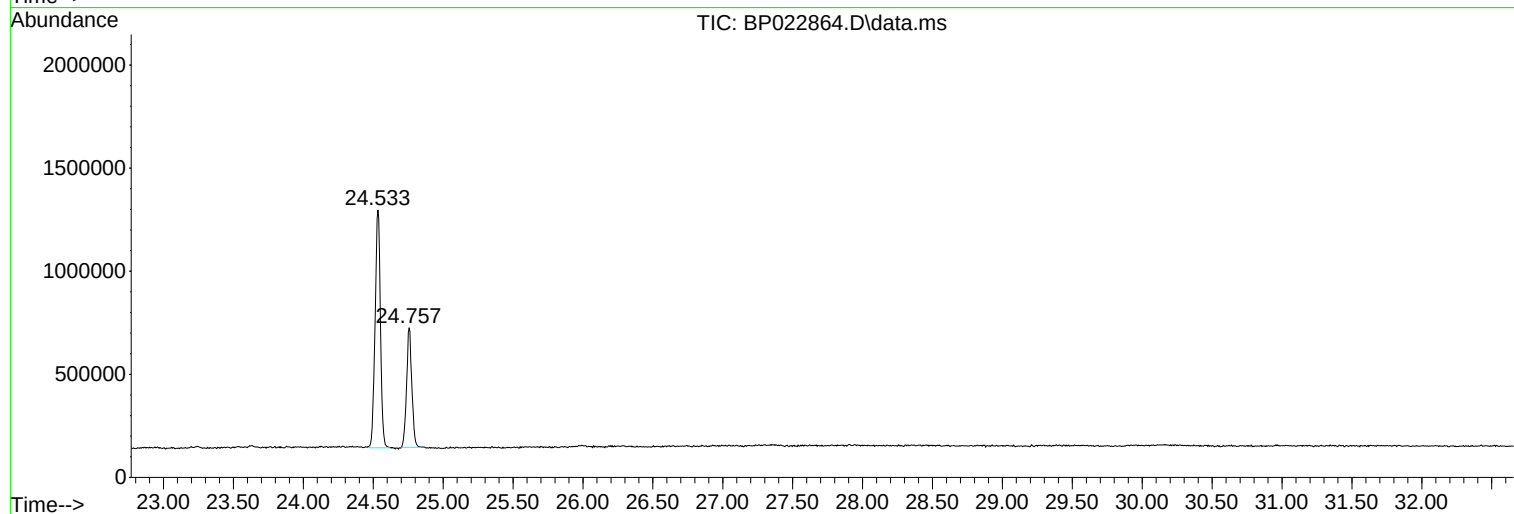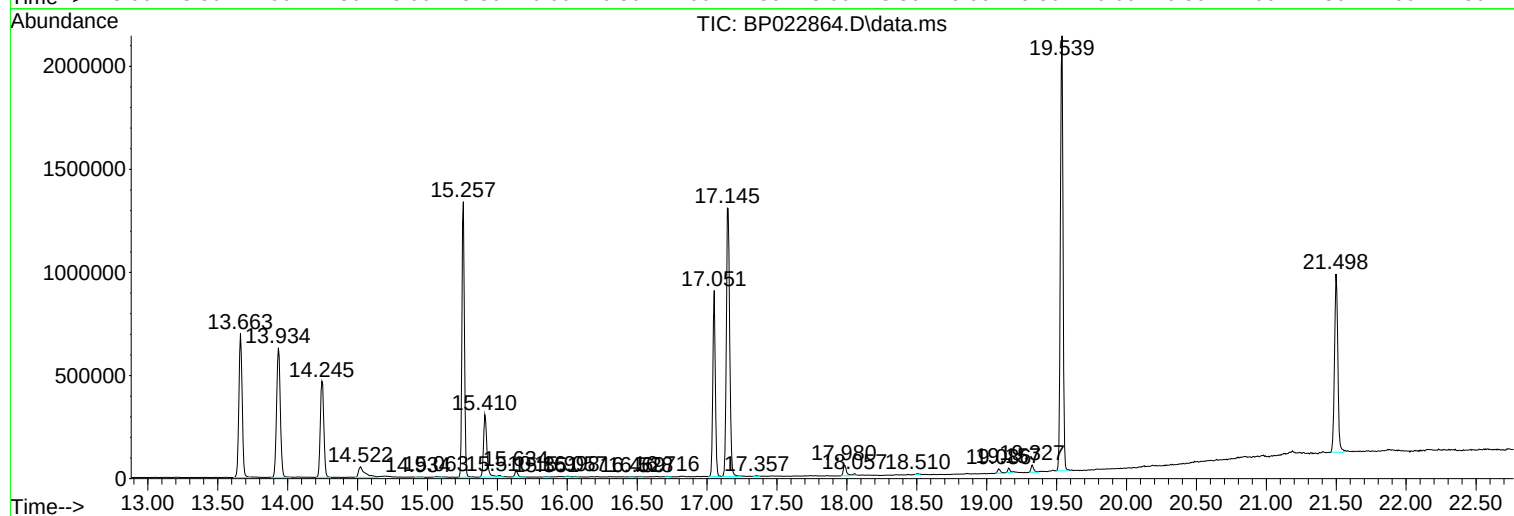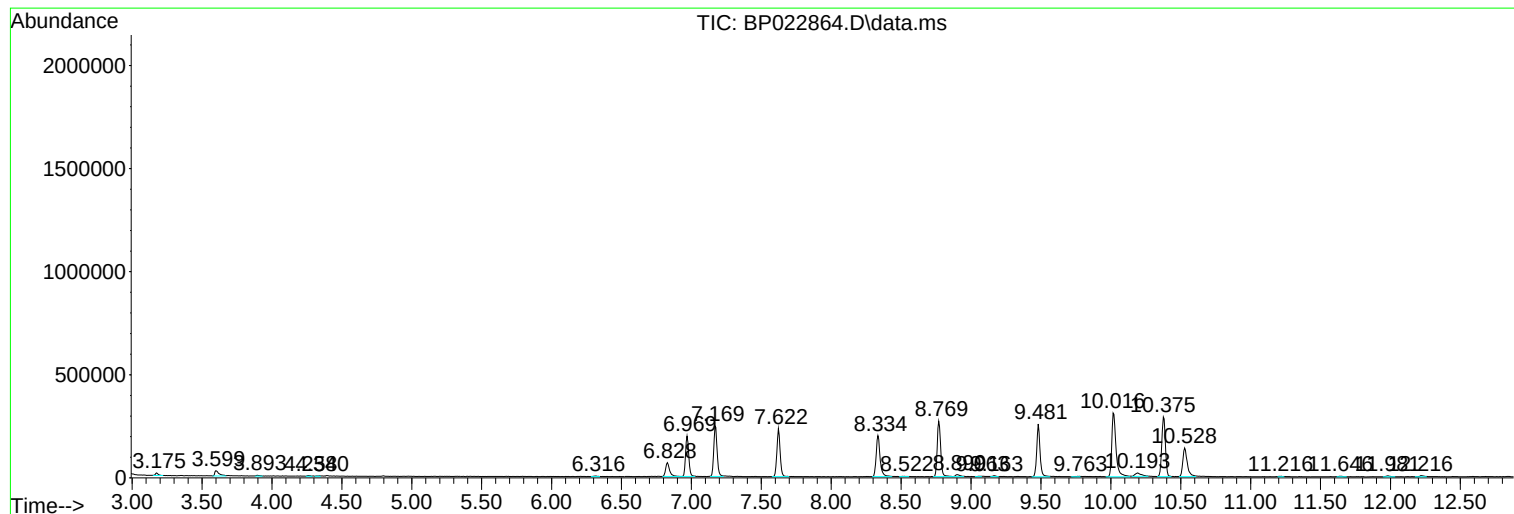

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110424\
Data File : BP022864.D
Acq On : 05 Nov 2024 17:31
Operator : RC/JU
Sample : P4671-03
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AB2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110424\
Data File : BP022864.D
Acq On : 05 Nov 2024 17:31
Operator : RC/JU
Sample : P4671-03
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AB2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc