

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110424\
 Data File : BP022867.D
 Acq On : 05 Nov 2024 19:33
 Operator : RC/JU
 Sample : P4670-03
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0SY4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP022867.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.175	28	32	38	rBV	14407	16938	0.57%	0.076%
2	3.599	100	104	114	rBV	36534	68766	2.31%	0.310%
3	3.899	151	155	159	rBV2	5646	7281	0.24%	0.033%
4	4.399	235	240	244	rVB7	2411	3943	0.13%	0.018%
5	5.728	459	466	472	rBV7	1183	3027	0.10%	0.014%
6	6.822	646	652	665	rBV	79049	153682	5.15%	0.692%
7	6.969	671	677	690	rVB	198282	314387	10.54%	1.416%
8	7.169	703	711	723	rBV	259965	439046	14.72%	1.977%
9	7.516	763	770	776	rBV4	4513	7990	0.27%	0.036%
10	7.622	780	788	802	rBV	235777	399124	13.38%	1.797%
11	7.975	843	848	852	rBV7	2629	5133	0.17%	0.023%
12	8.334	901	909	927	rBV	229487	428580	14.37%	1.930%
13	8.763	975	982	987	rBV	271033	480740	16.12%	2.165%
14	8.804	987	989	998	rVV2	33166	54817	1.84%	0.247%
15	8.910	1000	1007	1014	rVB9	3942	9277	0.31%	0.042%
16	9.169	1049	1051	1054	rVV4	3107	2986	0.10%	0.013%
17	9.216	1055	1059	1065	rVB8	2414	4382	0.15%	0.020%
18	9.475	1096	1103	1119	rBV	243907	441992	14.82%	1.990%
19	10.022	1189	1196	1218	rBV	344842	690876	23.16%	3.111%
20	10.186	1218	1224	1225	rBV5	6552	8464	0.28%	0.038%
21	10.245	1230	1234	1243	rVB2	19483	36888	1.24%	0.166%
22	10.375	1249	1256	1267	rVB	331778	555397	18.62%	2.501%
23	10.539	1277	1284	1297	rBV2	14454	37486	1.26%	0.169%
24	10.763	1316	1322	1328	rVB2	14761	27154	0.91%	0.122%
25	10.998	1356	1362	1377	rBV2	23238	53785	1.80%	0.242%
26	11.210	1391	1398	1402	rBV9	5863	13513	0.45%	0.061%
27	11.645	1467	1472	1478	rVB2	12573	18426	0.62%	0.083%
28	11.710	1478	1483	1488	rVB8	3105	4581	0.15%	0.021%
29	11.986	1524	1530	1538	rVB3	5117	9723	0.33%	0.044%
30	12.228	1564	1571	1577	rBV3	2870	8214	0.28%	0.037%
31	12.392	1591	1599	1603	rBV5	9471	18613	0.62%	0.084%
32	12.675	1642	1647	1653	rBV10	4211	10213	0.34%	0.046%
33	12.839	1667	1675	1680	rBV10	2077	4737	0.16%	0.021%
34	13.045	1703	1710	1718	rBV8	10070	24530	0.82%	0.110%
35	13.251	1741	1745	1753	rVB2	4213	7044	0.24%	0.032%
36	13.333	1754	1759	1767	rVB2	2251	4950	0.17%	0.022%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110424\
 Data File : BP022867.D
 Acq On : 05 Nov 2024 19:33
 Operator : RC/JU
 Sample : P4670-03
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 COSY4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
 Title : SVOA CALIBRATION

37	13.651	1807	1813	1825	rBV	789088	1066034	35.74%	4.801%
38	13.733	1825	1827	1832	rVV6	4063	7250	0.24%	0.033%
39	13.939	1855	1862	1869	rBV2	784314	1139750	38.21%	5.133%
40	14.063	1880	1883	1888	rVB4	3909	6026	0.20%	0.027%
41	14.245	1908	1914	1927	rBV	567935	860268	28.84%	3.874%
42	14.357	1930	1933	1939	rVV7	2959	5075	0.17%	0.023%
43	14.533	1954	1963	1984	rBV4	46629	179110	6.00%	0.807%
44	14.680	1986	1988	1992	rVB5	3809	5143	0.17%	0.023%
45	14.763	1998	2002	2012	rVB5	3753	8048	0.27%	0.036%
46	14.922	2025	2029	2033	rBV7	2777	5077	0.17%	0.023%
47	15.016	2043	2045	2049	rBV3	2602	3150	0.11%	0.014%
48	15.269	2080	2088	2097	rBV	949223	1616735	54.20%	7.281%
49	15.333	2097	2099	2106	rVV8	6561	14038	0.47%	0.063%
50	15.404	2106	2111	2123	rVV	387002	513199	17.21%	2.311%
51	15.498	2123	2127	2136	rVB9	6875	17625	0.59%	0.079%
52	15.645	2146	2152	2158	rBV	22796	38432	1.29%	0.173%
53	16.004	2207	2213	2221	rBV4	8276	16535	0.55%	0.074%
54	16.286	2256	2261	2264	rBV7	8560	13408	0.45%	0.060%
55	16.639	2316	2321	2322	rBV4	4139	6262	0.21%	0.028%
56	16.733	2333	2337	2341	rVB7	2540	4196	0.14%	0.019%
57	16.827	2348	2353	2357	rVB5	2293	4519	0.15%	0.020%
58	17.063	2386	2393	2400	rBV	831504	1174471	39.38%	5.289%
59	17.157	2403	2409	2421	rVV	1621359	2112192	70.81%	9.512%
60	17.257	2424	2426	2430	rVB4	3674	5100	0.17%	0.023%
61	17.368	2442	2445	2450	rVB5	3753	5531	0.19%	0.025%
62	17.427	2450	2455	2457	rBV6	2597	4365	0.15%	0.020%
63	17.763	2508	2512	2516	rVB3	11269	15156	0.51%	0.068%
64	18.004	2548	2553	2561	rBV2	58778	97198	3.26%	0.438%
65	18.074	2562	2565	2569	rVV	6947	9470	0.32%	0.043%
66	18.492	2631	2636	2643	rBV2	78704	100879	3.38%	0.454%
67	18.792	2685	2687	2689	rBV2	2965	3211	0.11%	0.014%
68	19.092	2734	2738	2741	rBV2	15970	22755	0.76%	0.102%
69	19.133	2742	2745	2748	rVB5	7920	8570	0.29%	0.039%
70	19.174	2748	2752	2756	rBV2	18692	24781	0.83%	0.112%
71	19.339	2776	2780	2786	rBV2	57880	82724	2.77%	0.373%
72	19.551	2810	2816	2827	rBV	1896483	2650286	88.85%	11.935%
73	21.498	3142	3147	3154	rBV	1040729	1450527	48.63%	6.532%
74	24.539	3655	3664	3675	rVB	1195882	2982775	100.00%	13.433%
75	24.750	3691	3700	3716	rVB	587953	1548873	51.93%	6.975%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110424\
Data File : BP022867.D
Acq On : 05 Nov 2024 19:33
Operator : RC/JU
Sample : P4670-03
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0SY4

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
Title : SVOA CALIBRATION




Sum of corrected areas: 22205429

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110424\
Data File : BP022867.D
Acq On : 05 Nov 2024 19:33
Operator : RC/JU
Sample : P4670-03
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0SY4

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

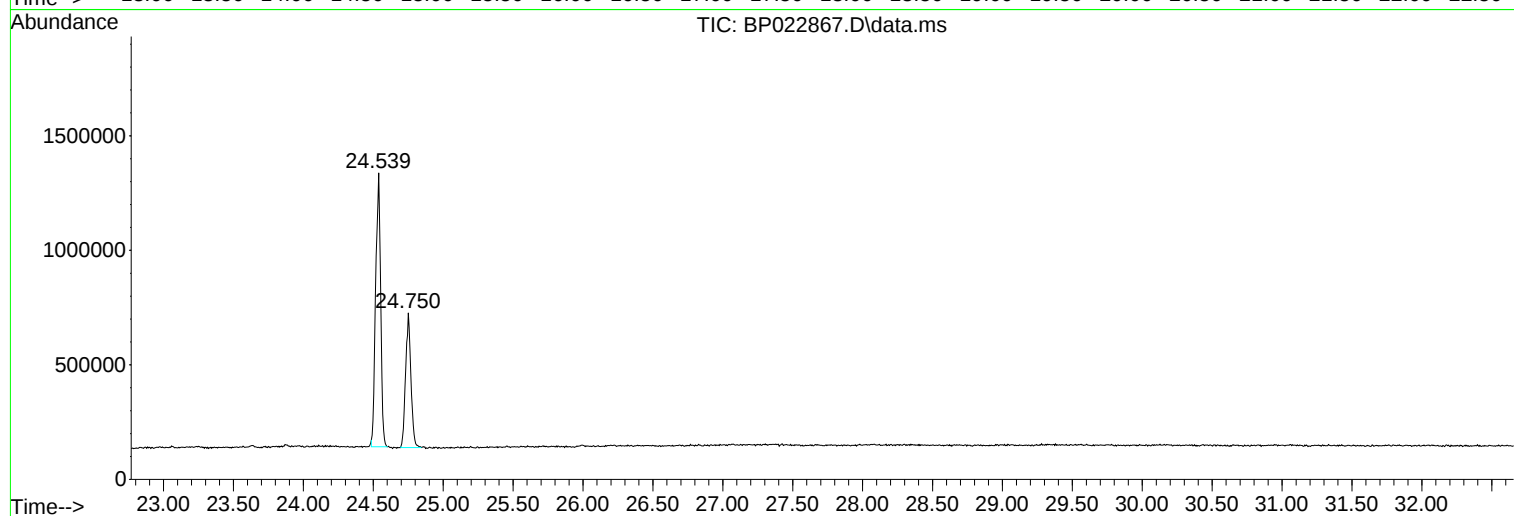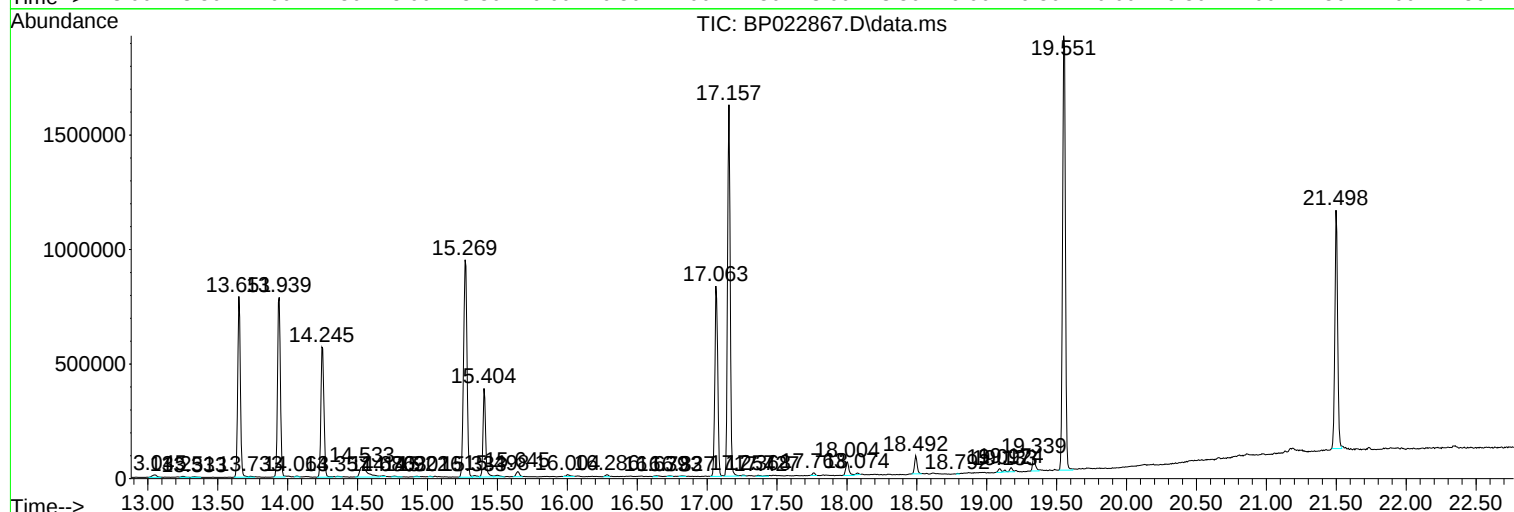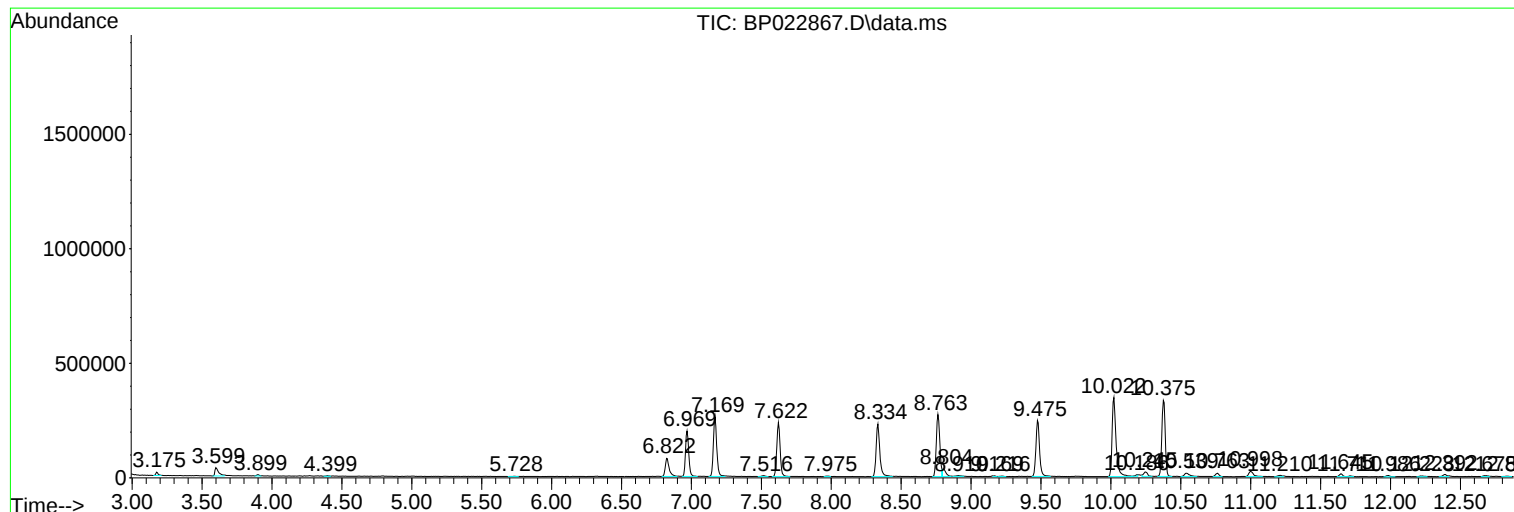

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110424\
Data File : BP022867.D
Acq On : 05 Nov 2024 19:33
Operator : RC/JU
Sample : P4670-03
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0SY4

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110424\
Data File : BP022867.D
Acq On : 05 Nov 2024 19:33
Operator : RC/JU
Sample : P4670-03
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0SY4

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------