

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110424\
 Data File : BP022882.D
 Acq On : 06 Nov 2024 06:22
 Operator : RC/JU
 Sample : P4644-13
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0CC0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP022882.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.175	28	32	42	rVB	17868	26993	0.76%	0.091%
2	3.599	101	104	116	rBV	30574	59444	1.68%	0.199%
3	3.905	150	156	163	rBV5	5362	10437	0.29%	0.035%
4	4.264	213	217	222	rVB7	5242	8419	0.24%	0.028%
5	4.417	237	243	252	rVB2	36889	58922	1.66%	0.198%
6	6.311	561	565	571	rVB8	2867	4780	0.13%	0.016%
7	6.699	624	631	634	rBV8	3481	6723	0.19%	0.023%
8	6.828	647	653	668	rBV	111597	223891	6.32%	0.751%
9	6.969	670	677	689	rBV	282822	468239	13.22%	1.571%
10	7.169	704	711	721	rBV	375612	622455	17.58%	2.088%
11	7.622	782	788	798	rBV	373010	608032	17.17%	2.040%
12	8.240	887	893	899	rVB9	3693	7769	0.22%	0.026%
13	8.334	901	909	923	rBV	334847	584822	16.52%	1.962%
14	8.769	975	983	997	rBV	401466	707810	19.99%	2.374%
15	8.905	1001	1006	1019	rVB	23113	45543	1.29%	0.153%
16	9.334	1074	1079	1084	rBV8	4961	8626	0.24%	0.029%
17	9.481	1095	1104	1119	rBV	362300	646285	18.25%	2.168%
18	9.757	1148	1151	1161	rVB	3101	5298	0.15%	0.018%
19	10.022	1186	1196	1213	rBV	504860	1010925	28.55%	3.391%
20	10.181	1218	1223	1234	rVB4	11450	34981	0.99%	0.117%
21	10.375	1248	1256	1264	rBV	525416	850457	24.02%	2.853%
22	10.528	1274	1282	1298	rBV	161288	347028	9.80%	1.164%
23	11.204	1389	1397	1400	rBV9	3736	7706	0.22%	0.026%
24	11.334	1414	1419	1426	rVB10	1957	4446	0.13%	0.015%
25	11.969	1522	1527	1533	rBV2	7007	12548	0.35%	0.042%
26	12.216	1563	1569	1575	rBV9	4213	8560	0.24%	0.029%
27	12.440	1601	1607	1608	rBV5	3285	4421	0.12%	0.015%
28	12.687	1641	1649	1654	rBV5	2322	3858	0.11%	0.013%
29	13.645	1805	1812	1822	rBV	1049219	1506147	42.54%	5.052%
30	13.928	1849	1860	1872	rBV2	1075674	1679312	47.43%	5.633%
31	14.234	1905	1912	1924	rBV	863503	1294380	36.56%	4.342%
32	14.510	1954	1959	1981	rBV	66457	196926	5.56%	0.661%
33	15.051	2041	2051	2053	rBV10	4076	7334	0.21%	0.025%
34	15.245	2077	2084	2093	rBV	1651612	2287055	64.59%	7.672%
35	15.310	2093	2095	2103	rVB9	3007	5479	0.15%	0.018%
36	15.398	2103	2110	2122	rBV	318830	524329	14.81%	1.759%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110424\
 Data File : BP022882.D
 Acq On : 06 Nov 2024 06:22
 Operator : RC/JU
 Sample : P4644-13
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0CC0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
 Title : SVOA CALIBRATION

37	15.492	2123	2126	2132	rVB2	9673	14811	0.42%	0.050%
38	15.616	2142	2147	2156	rBV	63539	103563	2.92%	0.347%
39	15.839	2180	2185	2188	rBV7	2676	5006	0.14%	0.017%
40	16.175	2236	2242	2244	rBV7	2600	5072	0.14%	0.017%
41	16.198	2244	2246	2251	rVB6	3165	4538	0.13%	0.015%
42	16.451	2285	2289	2292	rBV5	2649	3941	0.11%	0.013%
43	16.828	2346	2353	2357	rBV8	3616	7393	0.21%	0.025%
44	17.033	2381	2388	2400	rBV	1167734	1725129	48.72%	5.787%
45	17.151	2400	2408	2420	rBV	1723963	2822545	79.71%	9.468%
46	17.345	2438	2441	2443	rBV4	2828	4139	0.12%	0.014%
47	17.980	2544	2549	2557	rBV	76596	124333	3.51%	0.417%
48	18.345	2607	2611	2616	rBV8	5155	9651	0.27%	0.032%
49	18.492	2632	2636	2641	rBV7	6105	11004	0.31%	0.037%
50	19.080	2732	2736	2741	rBV3	27808	38902	1.10%	0.130%
51	19.151	2744	2748	2752	rBV	25771	34467	0.97%	0.116%
52	19.316	2772	2776	2781	rBV5	30468	45045	1.27%	0.151%
53	19.533	2807	2813	2826	rVB	2421538	3386721	95.65%	11.361%
54	21.480	3139	3144	3155	rVB2	1146415	1997738	56.42%	6.701%
55	24.521	3651	3661	3671	rVB	1505444	3540891	100.00%	11.878%
56	24.745	3690	3699	3711	rVB3	664611	2035165	57.48%	6.827%




Sum of corrected areas: 29810434

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110424\
Data File : BP022882.D
Acq On : 06 Nov 2024 06:22
Operator : RC/JU
Sample : P4644-13
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0CC0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

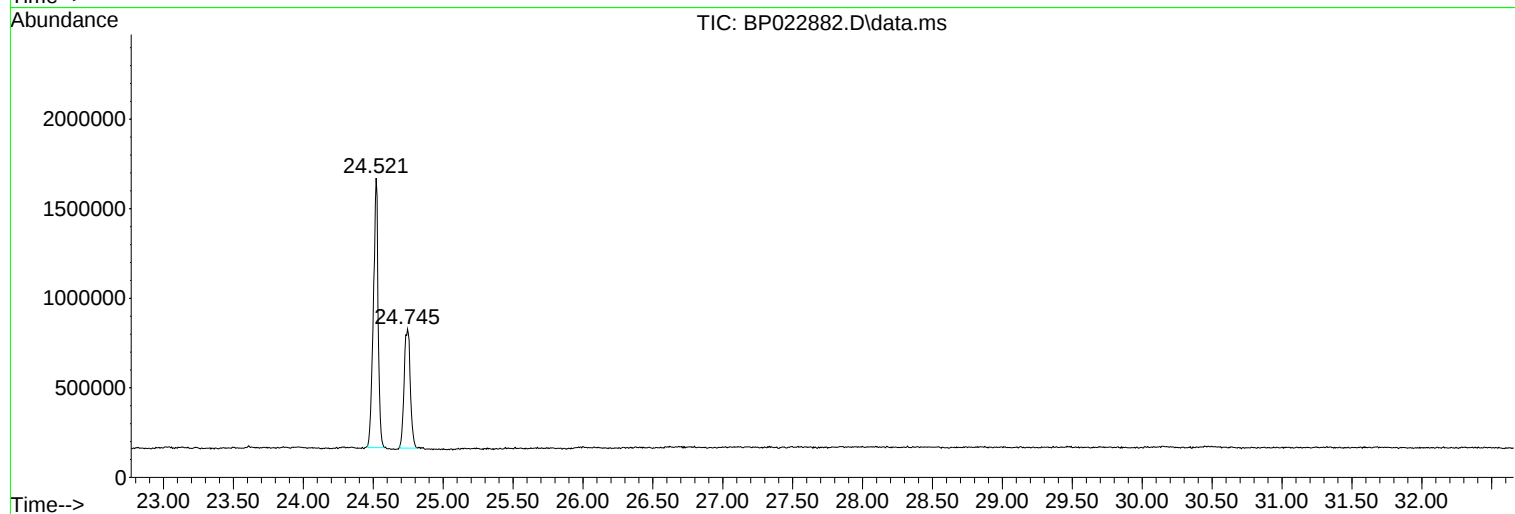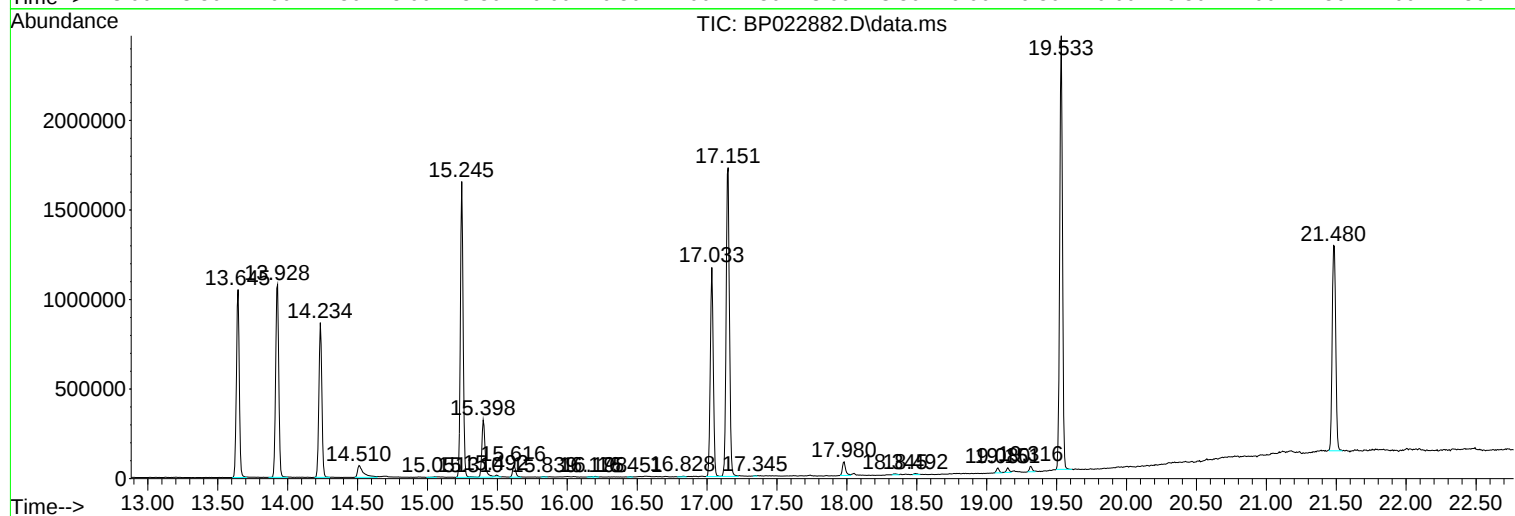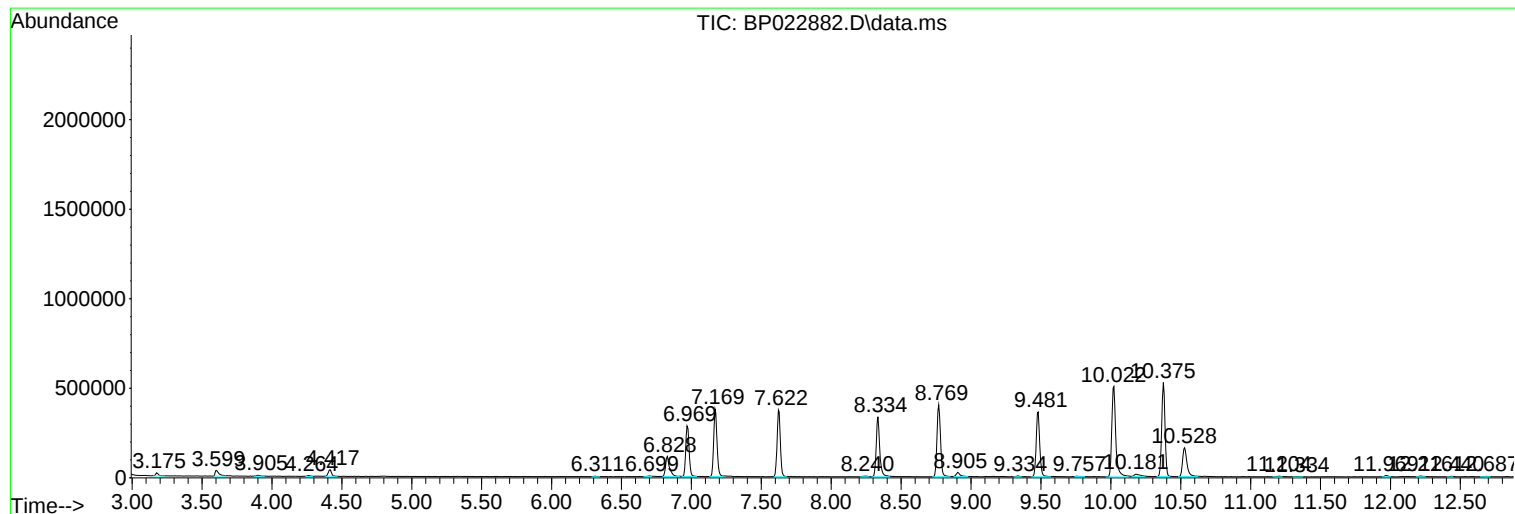

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110424\
Data File : BP022882.D
Acq On : 06 Nov 2024 06:22
Operator : RC/JU
Sample : P4644-13
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0CC0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110424\
Data File : BP022882.D
Acq On : 06 Nov 2024 06:22
Operator : RC/JU
Sample : P4644-13
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0CC0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
