

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110424\
 Data File : BP022885.D
 Acq On : 06 Nov 2024 09:05
 Operator : RC/JU
 Sample : PB164574BL
 Misc :
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK574

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP022885.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.175	28	32	40	rVB	21551	28989	1.02%	0.111%
2	3.587	98	102	122	rBV	265733	452177	15.92%	1.725%
3	3.899	151	155	159	rVB	4318	5554	0.20%	0.021%
4	6.822	645	652	671	rVV	335199	629571	22.16%	2.402%
5	6.969	671	677	688	rVB	270755	419877	14.78%	1.602%
6	7.163	704	710	726	rBV	381426	623740	21.96%	2.380%
7	7.622	781	788	800	rBV	301530	480574	16.92%	1.833%
8	8.328	901	908	931	rBV	430376	795556	28.01%	3.035%
9	8.769	975	983	995	rBV	364725	632794	22.28%	2.414%
10	9.163	1045	1050	1056	rVB6	5196	8444	0.30%	0.032%
11	9.475	1096	1103	1117	rBV	332564	567125	19.96%	2.164%
12	10.016	1188	1195	1221	rBV	430697	895478	31.52%	3.416%
13	10.381	1248	1257	1266	rBV	381469	656584	23.11%	2.505%
14	10.522	1273	1281	1296	rBV	398744	799808	28.16%	3.051%
15	11.634	1464	1470	1479	rVB5	4535	8685	0.31%	0.033%
16	11.975	1519	1528	1537	rBV4	6839	15811	0.56%	0.060%
17	13.645	1803	1812	1828	rBV	770997	1298238	45.70%	4.953%
18	13.934	1854	1861	1877	rBV	1047224	1520094	53.51%	5.799%
19	14.245	1907	1914	1923	rBV	655651	1001394	35.25%	3.820%
20	14.504	1952	1958	1980	rBV	223256	600469	21.14%	2.291%
21	14.940	2028	2032	2036	rBV7	1923	2973	0.10%	0.011%
22	15.257	2078	2086	2097	rBV	1307975	1971271	69.39%	7.520%
23	15.404	2104	2111	2124	rBV	215367	424937	14.96%	1.621%
24	15.504	2124	2128	2135	rVB6	6337	13559	0.48%	0.052%
25	16.528	2298	2302	2305	rBV6	2586	4413	0.16%	0.017%
26	16.710	2330	2333	2338	rBV6	2310	3664	0.13%	0.014%
27	16.834	2350	2354	2359	rVB7	2718	4521	0.16%	0.017%
28	17.045	2383	2390	2400	rBV	833543	1311417	46.17%	5.003%
29	17.145	2400	2407	2422	rVV2	1513027	2249620	79.19%	8.582%
30	17.292	2430	2432	2437	rBV6	1499	2904	0.10%	0.011%
31	17.628	2486	2489	2493	rVB6	2276	3311	0.12%	0.013%
32	19.086	2733	2737	2741	rBV4	18905	24968	0.88%	0.095%
33	19.163	2746	2750	2755	rBV	20832	29282	1.03%	0.112%
34	19.539	2807	2814	2822	rBV	1945274	2768492	97.46%	10.562%
35	21.492	3139	3146	3157	rBV2	913604	1596191	56.19%	6.089%
36	24.515	3652	3660	3677	rVB	1042710	2840690	100.00%	10.837%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110424\
Data File : BP022885.D
Acq On : 06 Nov 2024 09:05
Operator : RC/JU
Sample : PB164574BL
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK574

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
Title : SVOA CALIBRATION

37	24.739	3690	3698	3710	rVB	552642	1519384	53.49%	5.796%
----	--------	------	------	------	-----	--------	---------	--------	--------




Sum of corrected areas: 26212559

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110424\
Data File : BP022885.D
Acq On : 06 Nov 2024 09:05
Operator : RC/JU
Sample : PB164574BL
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK574

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

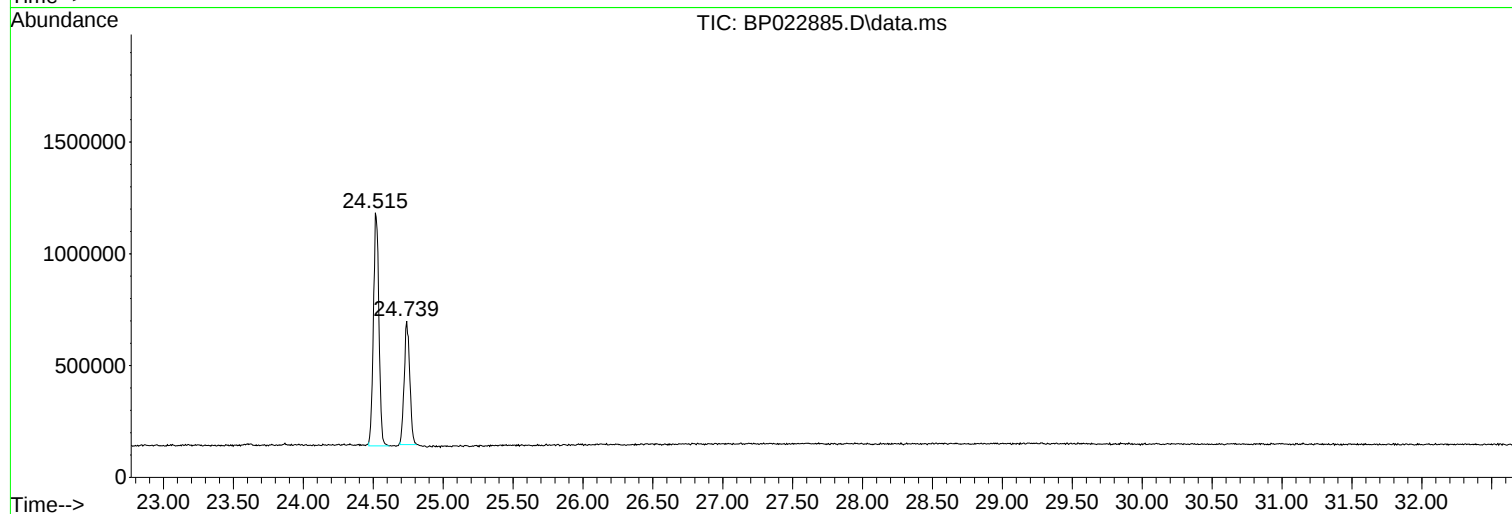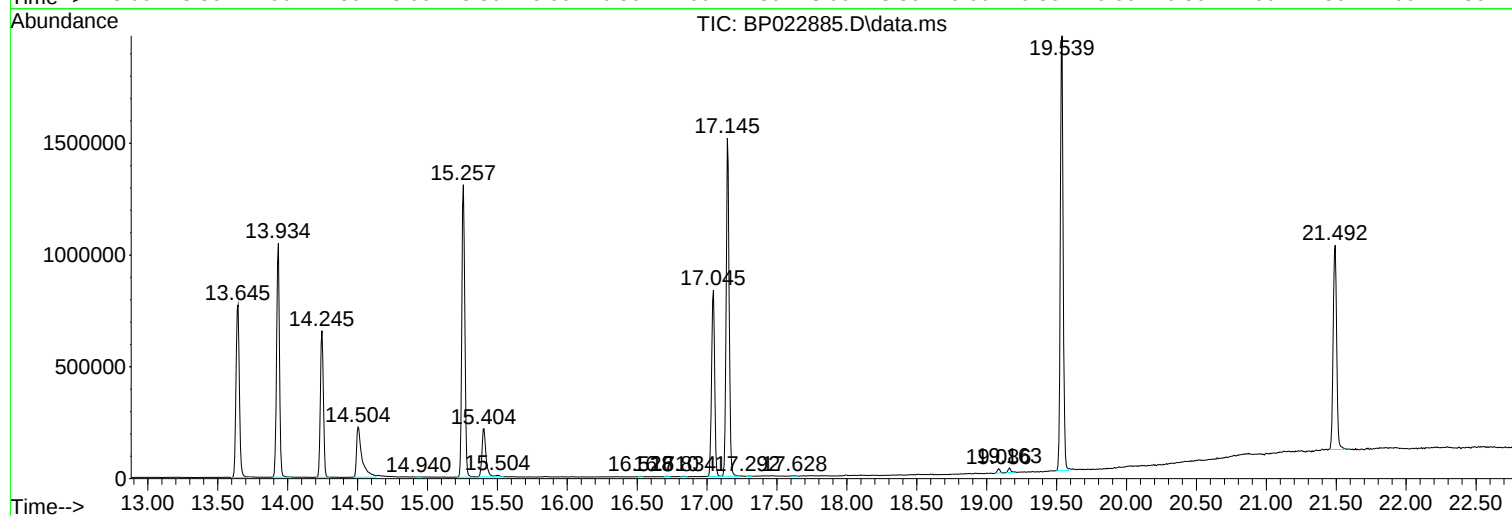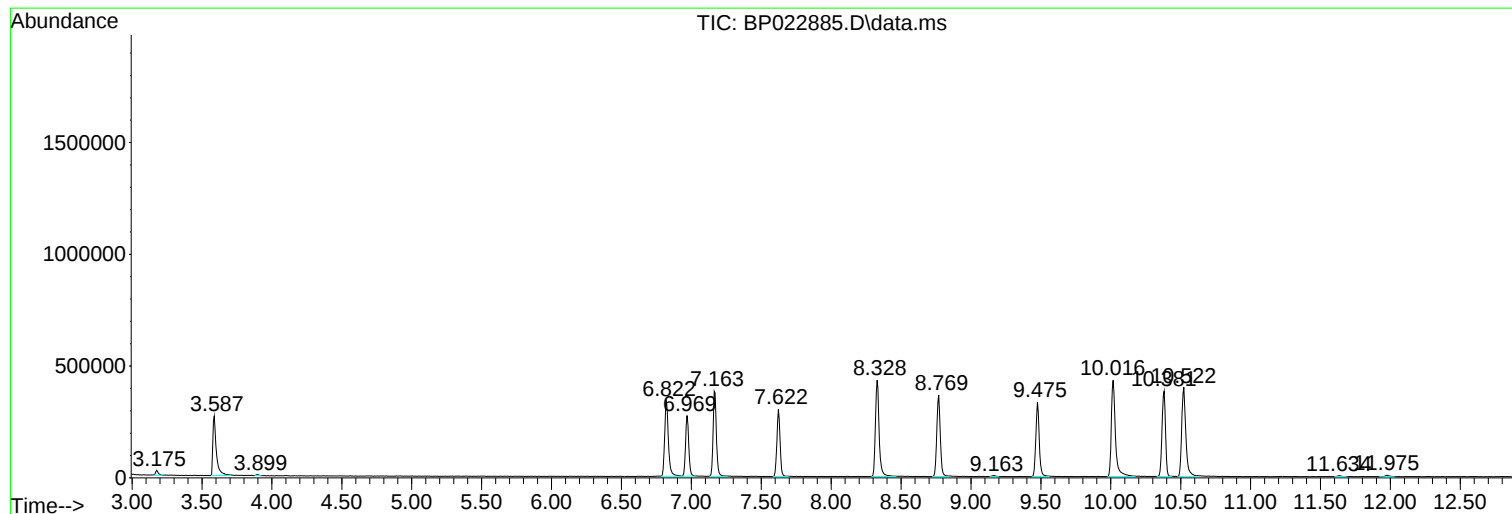

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110424\
Data File : BP022885.D
Acq On : 06 Nov 2024 09:05
Operator : RC/JU
Sample : PB164574BL
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK574

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110424\
Data File : BP022885.D
Acq On : 06 Nov 2024 09:05
Operator : RC/JU
Sample : PB164574BL
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK574

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------