

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110424\
 Data File : BP022908.D
 Acq On : 07 Nov 2024 00:43
 Operator : RC/JU
 Sample : P4622-09
 Misc :
 ALS Vial : 55 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BH6N5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP022908.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.175	29	32	36	rBV	7488	9046	0.48%	0.049%
2	3.681	115	118	123	rBV2	4871	7546	0.40%	0.041%
3	3.758	126	131	134	rVB7	1584	2885	0.15%	0.016%
4	3.893	149	154	155	rBV5	3101	4064	0.21%	0.022%
5	4.399	237	240	245	rVB6	1807	2410	0.13%	0.013%
6	6.040	516	519	523	rVB6	1555	2116	0.11%	0.011%
7	6.822	645	652	669	rBV	169156	321731	16.98%	1.731%
8	6.969	671	677	687	rVB	131404	210438	11.11%	1.132%
9	7.164	701	710	720	rBV	180903	313054	16.52%	1.684%
10	7.616	778	787	800	rBV	313421	535827	28.28%	2.883%
11	8.334	902	909	927	rBV	195768	401822	21.21%	2.162%
12	8.587	948	952	955	rBV6	1317	1907	0.10%	0.010%
13	8.769	974	983	993	rBV	184297	325339	17.17%	1.750%
14	8.928	1006	1010	1015	rVB7	1507	2158	0.11%	0.012%
15	9.158	1046	1049	1054	rVB5	3958	6408	0.34%	0.034%
16	9.481	1095	1104	1116	rBV	151764	269862	14.24%	1.452%
17	9.581	1119	1121	1126	rVB6	1513	2291	0.12%	0.012%
18	10.028	1189	1197	1215	rBV	206783	472560	24.94%	2.542%
19	10.205	1225	1227	1233	rVB7	1258	1903	0.10%	0.010%
20	10.381	1247	1257	1266	rBV	455006	745891	39.37%	4.013%
21	10.528	1275	1282	1307	rBV	162647	335737	17.72%	1.806%
22	11.804	1494	1499	1501	rBV6	1508	1993	0.11%	0.011%
23	11.981	1524	1529	1533	rBV6	3345	5411	0.29%	0.029%
24	12.840	1670	1675	1679	rBV8	1362	2479	0.13%	0.013%
25	13.046	1707	1710	1715	rBV6	3200	5099	0.27%	0.027%
26	13.651	1807	1813	1823	rBV	375051	538776	28.44%	2.899%
27	13.940	1855	1862	1874	rBV	576132	868828	45.86%	4.674%
28	14.157	1896	1899	1902	rVB4	2632	2996	0.16%	0.016%
29	14.251	1906	1915	1923	rVV	836831	1135679	59.95%	6.110%
30	14.304	1923	1924	1931	rVV7	4229	6737	0.36%	0.036%
31	14.351	1931	1932	1938	rVB6	1323	1988	0.10%	0.011%
32	14.522	1954	1961	1978	rBV2	71386	238273	12.58%	1.282%
33	14.698	1989	1991	1995	rVB4	3514	4574	0.24%	0.025%
34	14.857	2014	2018	2021	rBV5	1562	2477	0.13%	0.013%
35	15.263	2080	2087	2101	rBV	734376	1154395	60.94%	6.211%
36	15.410	2107	2112	2124	rBV3	28970	66148	3.49%	0.356%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110424\
 Data File : BP022908.D
 Acq On : 07 Nov 2024 00:43
 Operator : RC/JU
 Sample : P4622-09
 Misc :
 ALS Vial : 55 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BH6N5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
 Title : SVOA CALIBRATION

37	15.504	2124	2128	2131	rVV6	3914	6454	0.34%	0.035%
38	15.640	2145	2151	2158	rBV	225401	249578	13.17%	1.343%
39	15.769	2170	2173	2179	rVB7	1703	2899	0.15%	0.016%
40	15.951	2201	2204	2207	rBV5	1620	2882	0.15%	0.016%
41	15.992	2209	2211	2215	rVV5	2063	2897	0.15%	0.016%
42	16.057	2220	2222	2226	rVB4	2731	2842	0.15%	0.015%
43	16.175	2239	2242	2243	rVV3	2069	1919	0.10%	0.010%
44	16.210	2245	2248	2253	rVB6	3041	4711	0.25%	0.025%
45	16.598	2310	2314	2321	rBV8	3168	6783	0.36%	0.036%
46	16.722	2330	2335	2339	rVB8	2883	5509	0.29%	0.030%
47	16.757	2339	2341	2343	rBV3	1568	1909	0.10%	0.010%
48	16.828	2349	2353	2354	rBV4	2017	2061	0.11%	0.011%
49	16.975	2376	2378	2380	rBV3	2050	2168	0.11%	0.012%
50	17.057	2386	2392	2397	rBV	1106401	1514107	79.92%	8.146%
51	17.151	2403	2408	2424	rVB	871801	1288370	68.01%	6.931%
52	17.263	2424	2427	2428	rBV3	2285	2317	0.12%	0.012%
53	17.287	2428	2431	2436	rVB7	2642	4386	0.23%	0.024%
54	17.363	2441	2444	2447	rBV5	2389	3051	0.16%	0.016%
55	17.575	2476	2480	2481	rBV4	2663	3553	0.19%	0.019%
56	17.745	2505	2509	2516	rVB8	2892	5486	0.29%	0.030%
57	17.992	2547	2551	2562	rBV4	33212	49685	2.62%	0.267%
58	18.169	2577	2581	2584	rBV5	7534	11234	0.59%	0.060%
59	18.292	2598	2602	2606	rBV7	6192	9489	0.50%	0.051%
60	18.345	2608	2611	2614	rVV5	5117	7493	0.40%	0.040%
61	18.439	2623	2627	2629	rBV5	7688	9081	0.48%	0.049%
62	18.869	2695	2700	2705	rBV5	10546	20794	1.10%	0.112%
63	19.086	2734	2737	2742	rVB6	12161	17863	0.94%	0.096%
64	19.169	2747	2751	2752	rBV4	11012	13420	0.71%	0.072%
65	19.204	2752	2757	2761	rVB	41567	64734	3.42%	0.348%
66	19.333	2777	2779	2785	rVB7	8601	12195	0.64%	0.066%
67	19.545	2809	2815	2825	rBV	1078779	1704674	89.98%	9.171%
68	21.492	3140	3146	3161	rVB2	1203988	1873605	98.90%	10.080%
69	24.521	3653	3661	3680	rVB	692358	1774234	93.65%	9.545%
70	24.745	3691	3699	3710	rVB	704130	1894444	100.00%	10.192%




Sum of corrected areas: 18587675

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110424\
Data File : BP022908.D
Acq On : 07 Nov 2024 00:43
Operator : RC/JU
Sample : P4622-09
Misc :
ALS Vial : 55 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH6N5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

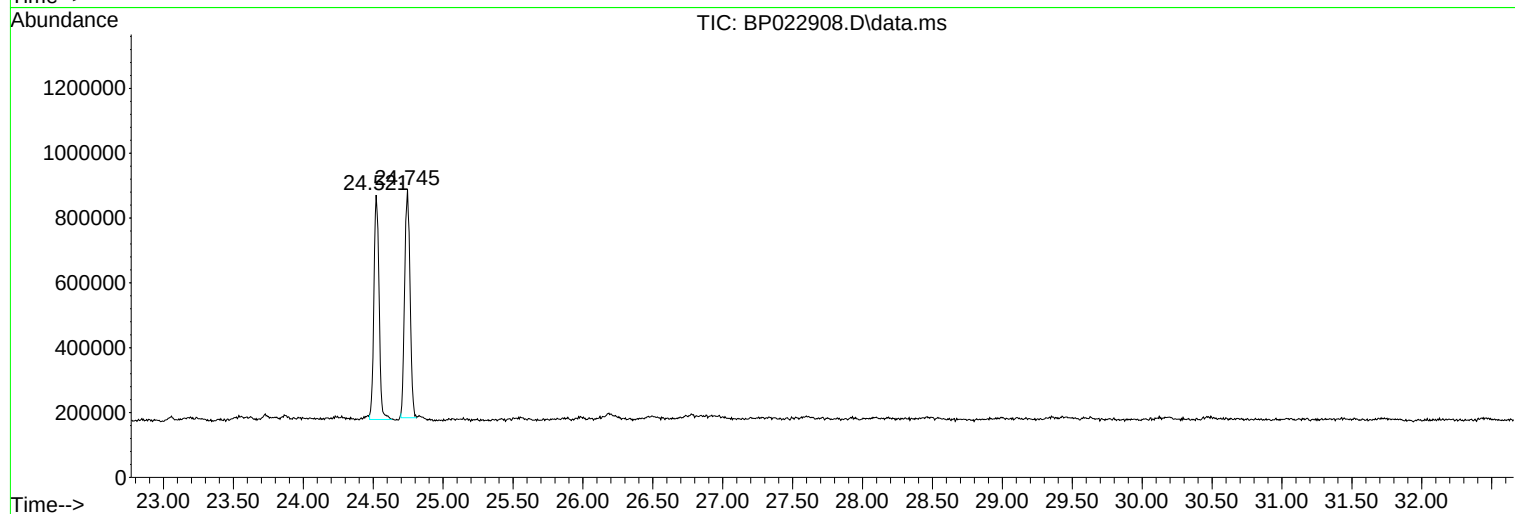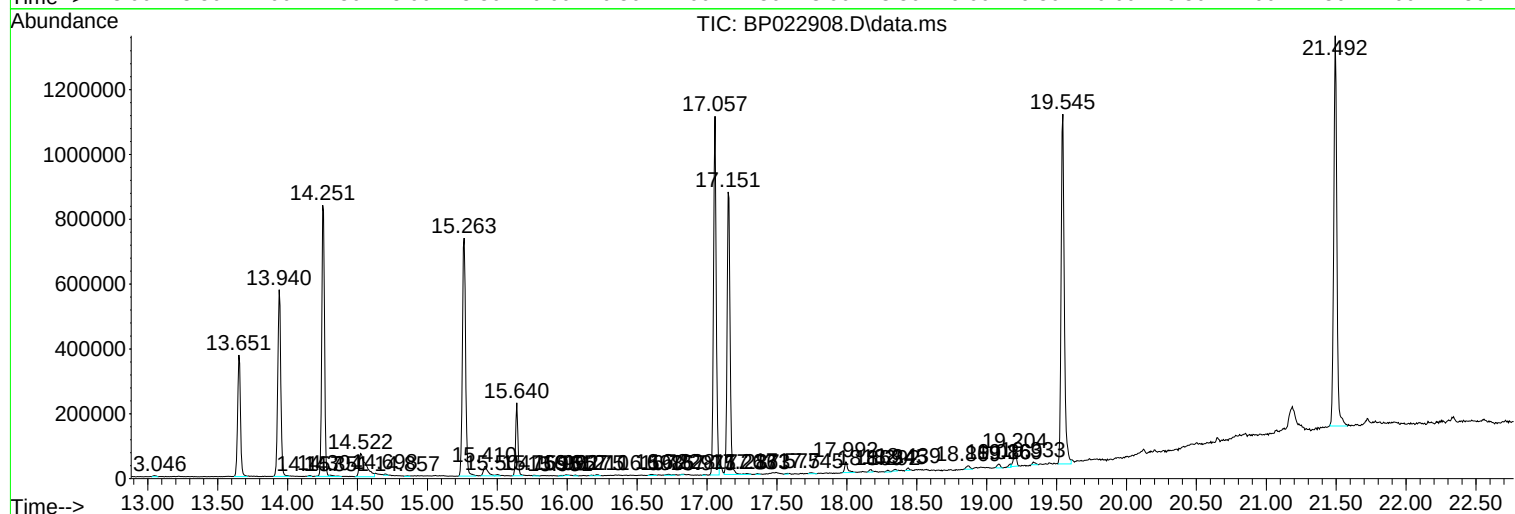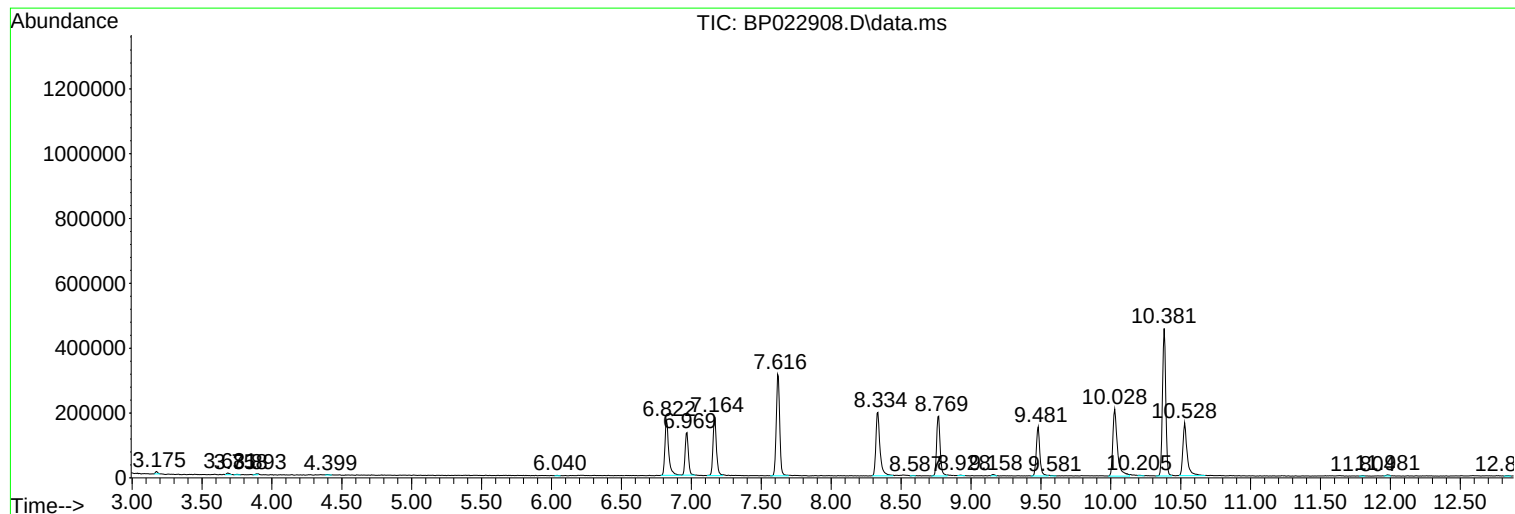

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110424\
Data File : BP022908.D
Acq On : 07 Nov 2024 00:43
Operator : RC/JU
Sample : P4622-09
Misc :
ALS Vial : 55 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH6N5










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Benzophenone Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
15.640	4.40 ng/ul	249578	Acenaphthene-d10	14.257

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Benzophenone	182	C13H10O	000119-61-9	97
2			Benzophenone	182	C13H10O	000119-61-9	96
3			Benzophenone	182	C13H10O	000119-61-9	95
4			Benzophenone	182	C13H10O	000119-61-9	91
5			Benzophenone	182	C13H10O	000119-61-9	72

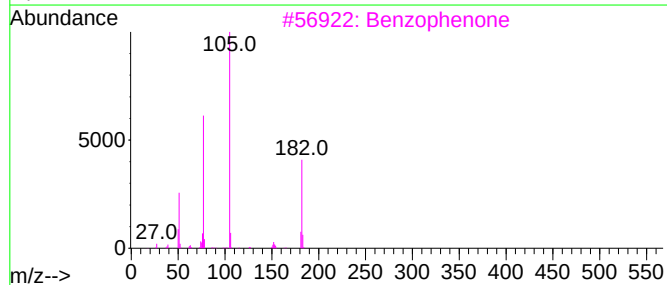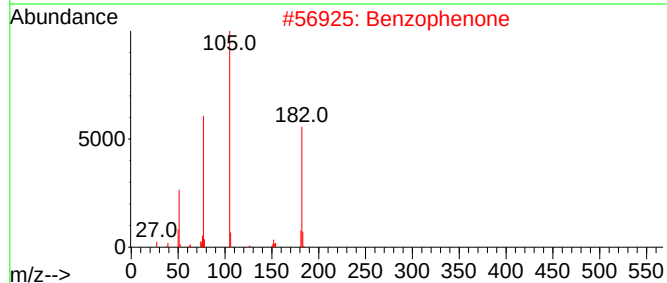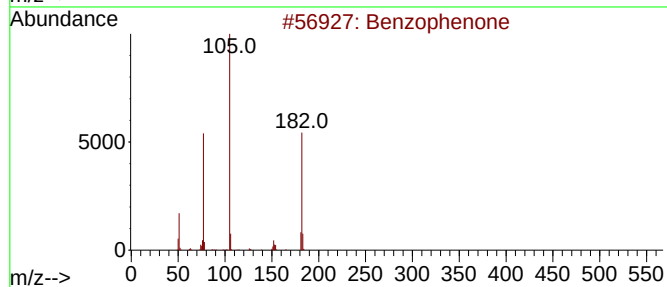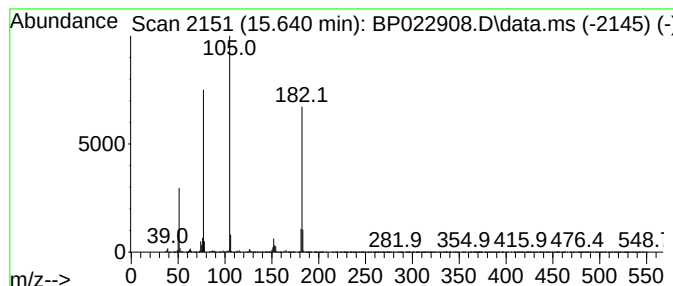

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110424\
Data File : BP022908.D
Acq On : 07 Nov 2024 00:43
Operator : RC/JU
Sample : P4622-09
Misc :
ALS Vial : 55 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH6N5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Benzophenone	15.640	4.4	ng/u1	249578	3	14.257	1135680	20.0