

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110424\
 Data File : BP022909.D
 Acq On : 07 Nov 2024 01:24
 Operator : RC/JU
 Sample : P4622-10
 Misc :
 ALS Vial : 56 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BH6N6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP022909.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.175	29	32	41	rVB	12061	18962	0.87%	0.089%
2	3.611	103	106	114	rBV	11312	21036	0.97%	0.099%
3	3.893	152	154	160	rVB4	5300	7383	0.34%	0.035%
4	4.393	236	239	245	rBV8	3488	5248	0.24%	0.025%
5	6.199	542	546	548	rBV4	1723	2388	0.11%	0.011%
6	6.552	600	606	610	rBV8	1395	2365	0.11%	0.011%
7	6.822	645	652	670	rBV	204655	407831	18.79%	1.913%
8	6.969	670	677	692	rVB	165760	271083	12.49%	1.271%
9	7.169	704	711	733	rVB	241360	395204	18.21%	1.853%
10	7.622	780	788	804	rBV	377356	608146	28.02%	2.852%
11	8.334	902	909	928	rBV	275358	521509	24.03%	2.446%
12	8.516	937	940	942	rBV4	2265	2875	0.13%	0.013%
13	8.769	975	983	994	rBV	233893	413293	19.04%	1.938%
14	8.928	1006	1010	1013	rBV6	1630	2218	0.10%	0.010%
15	9.163	1043	1050	1055	rVB6	5578	10886	0.50%	0.051%
16	9.481	1095	1104	1118	rBV	190952	351862	16.21%	1.650%
17	10.022	1189	1196	1213	rBV	280708	593175	27.33%	2.782%
18	10.381	1249	1257	1269	rBV	484322	841629	38.77%	3.947%
19	10.522	1274	1281	1296	rBV	241214	490166	22.58%	2.299%
20	11.628	1462	1469	1476	rBB	1503	2919	0.13%	0.014%
21	11.793	1493	1497	1502	rBV7	1645	2690	0.12%	0.013%
22	11.975	1522	1528	1534	rVV6	4559	8752	0.40%	0.041%
23	13.046	1707	1710	1719	rVB7	4373	7773	0.36%	0.036%
24	13.193	1731	1735	1743	rVB10	1295	3081	0.14%	0.014%
25	13.651	1805	1813	1829	rBV	561803	861226	39.68%	4.039%
26	13.928	1853	1860	1872	rBV	706060	1108523	51.07%	5.199%
27	14.146	1892	1897	1901	rVB5	3933	4902	0.23%	0.023%
28	14.240	1906	1913	1922	rBV	835144	1247982	57.50%	5.853%
29	14.510	1953	1959	1979	rBV2	113297	337616	15.55%	1.583%
30	14.710	1988	1993	1998	rVB7	5259	10221	0.47%	0.048%
31	14.851	2014	2017	2021	rVB6	1491	2229	0.10%	0.010%
32	15.116	2056	2062	2066	rBV9	2209	3977	0.18%	0.019%
33	15.251	2079	2085	2101	rBV	1020075	1493459	68.81%	7.004%
34	15.422	2107	2114	2123	rBV	56542	117551	5.42%	0.551%
35	15.510	2125	2129	2136	rVB6	6747	12546	0.58%	0.059%
36	15.628	2143	2149	2156	rBV	194324	268769	12.38%	1.260%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110424\
 Data File : BP022909.D
 Acq On : 07 Nov 2024 01:24
 Operator : RC/JU
 Sample : P4622-10
 Misc :
 ALS Vial : 56 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BH6N6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
 Title : SVOA CALIBRATION

37	15.840	2182	2185	2186	rBV3	1925	2176	0.10%	0.010%
38	16.210	2245	2248	2253	rVB3	6100	8804	0.41%	0.041%
39	16.251	2253	2255	2259	rVB5	1896	2332	0.11%	0.011%
40	16.510	2296	2299	2300	rBV3	2594	2343	0.11%	0.011%
41	16.528	2300	2302	2307	rVV6	2513	4927	0.23%	0.023%
42	16.587	2310	2312	2316	rVV4	3673	4505	0.21%	0.021%
43	16.645	2318	2322	2326	rVB7	2348	4243	0.20%	0.020%
44	16.851	2353	2357	2361	rBV4	1663	2959	0.14%	0.014%
45	17.045	2383	2390	2403	rBV	973433	1652489	76.13%	7.750%
46	17.163	2403	2410	2422	rVV2	980476	1638206	75.47%	7.683%
47	17.269	2426	2428	2433	rVB6	8417	11586	0.53%	0.054%
48	17.981	2544	2549	2559	rBV2	55002	93895	4.33%	0.440%
49	18.292	2599	2602	2605	rBV3	8190	10681	0.49%	0.050%
50	18.345	2607	2611	2617	rVV6	9030	17247	0.79%	0.081%
51	18.434	2623	2626	2632	rVB7	9862	15587	0.72%	0.073%
52	18.722	2673	2675	2680	rBV6	3993	5195	0.24%	0.024%
53	18.851	2695	2697	2698	rBV2	5417	4472	0.21%	0.021%
54	19.081	2732	2736	2740	rBV4	16359	22119	1.02%	0.104%
55	19.157	2745	2749	2751	rVV2	14894	23095	1.06%	0.108%
56	19.192	2751	2755	2766	rVB	33641	59912	2.76%	0.281%
57	19.328	2774	2778	2785	rBV5	15936	27370	1.26%	0.128%
58	19.539	2808	2814	2826	rBV	1411775	2114883	97.44%	9.919%
59	21.498	3141	3147	3159	rVB2	1149514	1916892	88.31%	8.990%
60	24.533	3654	3663	3678	rVB	861315	2170552	100.00%	10.180%
61	24.751	3692	3700	3701	rBV	631724	1044524	48.12%	4.899%




Sum of corrected areas: 21322469

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110424\
Data File : BP022909.D
Acq On : 07 Nov 2024 01:24
Operator : RC/JU
Sample : P4622-10
Misc :
ALS Vial : 56 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH6N6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

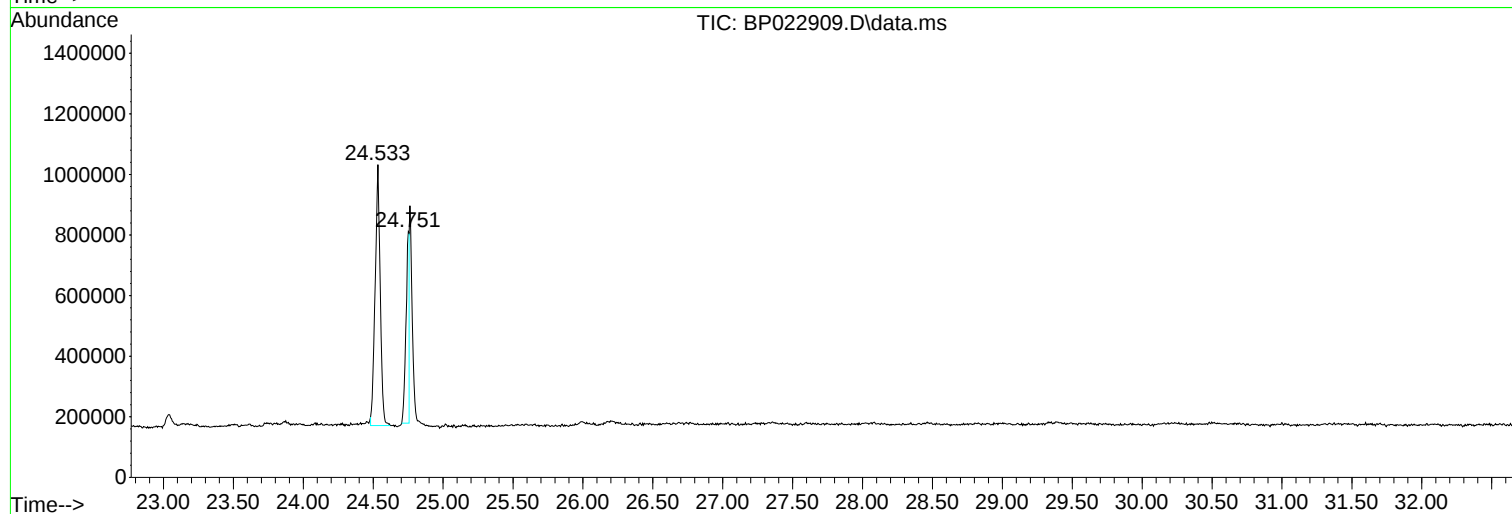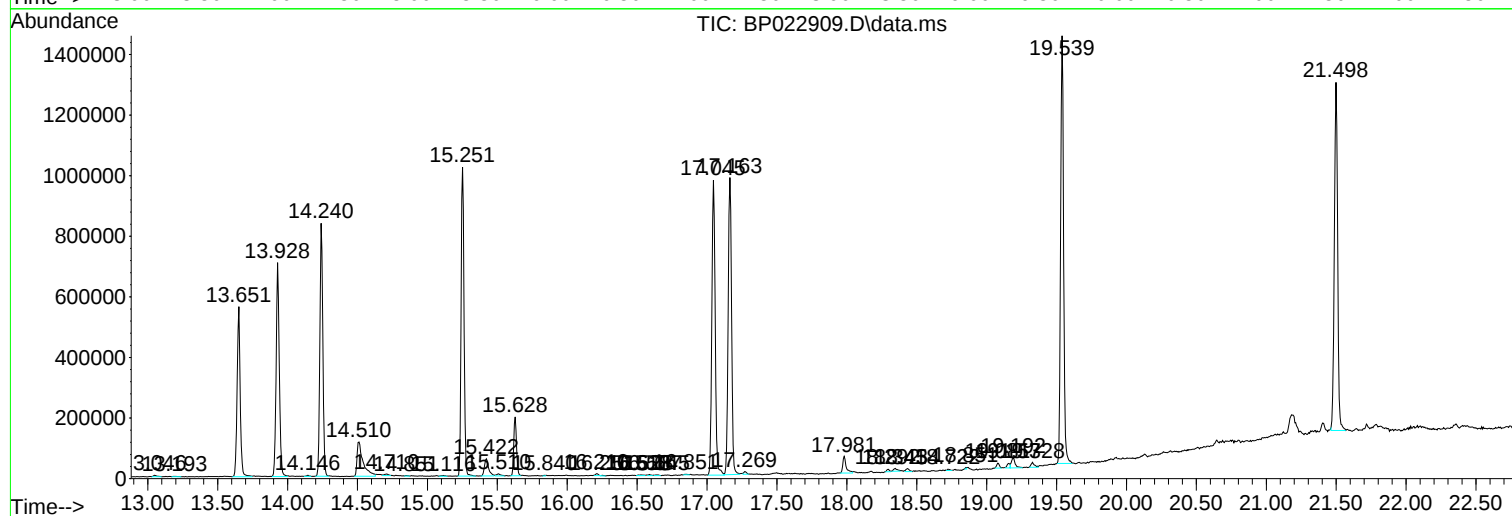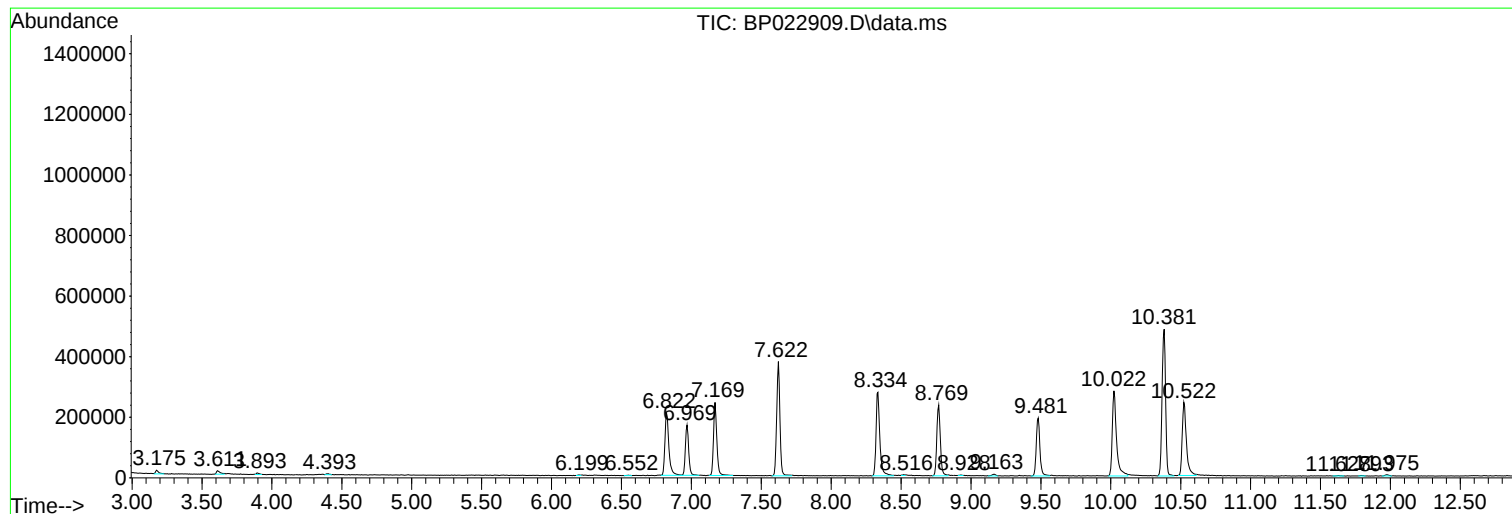

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110424\
Data File : BP022909.D
Acq On : 07 Nov 2024 01:24
Operator : RC/JU
Sample : P4622-10
Misc :
ALS Vial : 56 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH6N6










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Benzophenone Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
15.628	4.31 ng/ul	268769	Acenaphthene-d10	14.240

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Benzophenone	182	C13H10O	000119-61-9	97
2			Benzophenone	182	C13H10O	000119-61-9	96
3			Benzophenone	182	C13H10O	000119-61-9	94
4			Benzophenone	182	C13H10O	000119-61-9	91
5			Azobenzene, (E)-	182	C12H10N2	017082-12-1	59

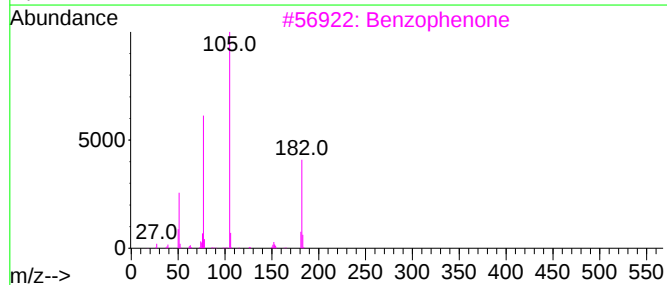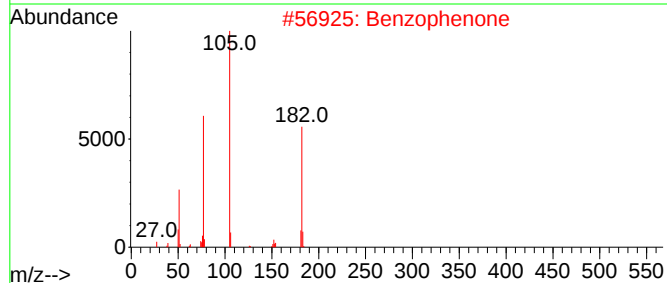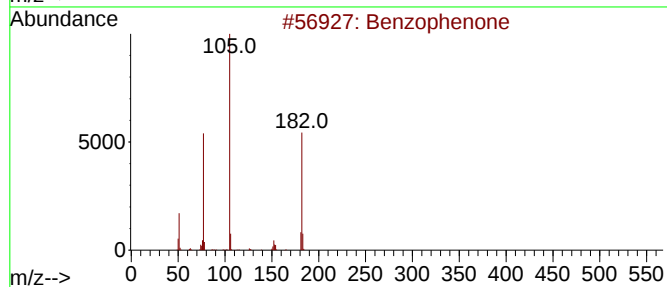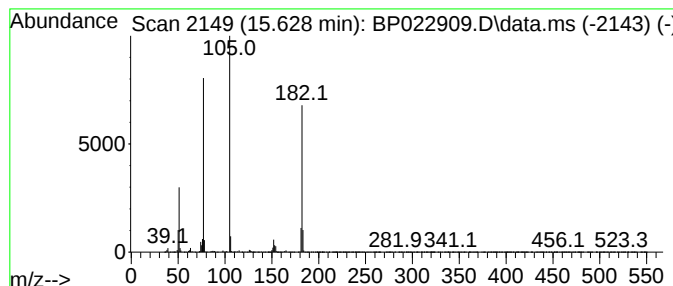

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110424\
Data File : BP022909.D
Acq On : 07 Nov 2024 01:24
Operator : RC/JU
Sample : P4622-10
Misc :
ALS Vial : 56 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH6N6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Benzophenone	15.628	4.3	ng/u1	268769	3	14.240	1247980	20.0