

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110425\
Data File : BP026070.D
Acq On : 04 Nov 2025 14:11
Operator : RC/JU
Sample : PB170372BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB170372BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP102925.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP026070.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.308	396	403	415	rBV	8014418	11630957	49.67%	10.749%
2	6.866	658	668	678	rBV	7169279	11388119	48.63%	10.525%
3	7.690	798	808	818	rBV	1515859	2358527	10.07%	2.180%
4	8.825	993	1001	1015	rBV	4672041	7409687	31.64%	6.848%
5	10.454	1270	1278	1291	rVB	1817306	3136061	13.39%	2.898%
6	12.937	1691	1700	1714	rBV	10593709	16657806	71.14%	15.395%
7	14.325	1928	1936	1952	rBV	2504953	3992149	17.05%	3.689%
8	15.842	2185	2194	2215	rBV	8156854	12174892	51.99%	11.252%
9	17.131	2406	2413	2426	rBV	3325357	4599905	19.64%	4.251%
10	19.878	2874	2880	2886	rBV	17069628	23415914	100.00%	21.640%
11	21.589	3164	3171	3181	rVB	3109678	5461681	23.32%	5.048%
12	24.924	3730	3738	3749	rVB	2190302	5979259	25.54%	5.526%




Sum of corrected areas: 108204957

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110425\
Data File : BP026070.D
Acq On : 04 Nov 2025 14:11
Operator : RC/JU
Sample : PB170372BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB170372BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP102925.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

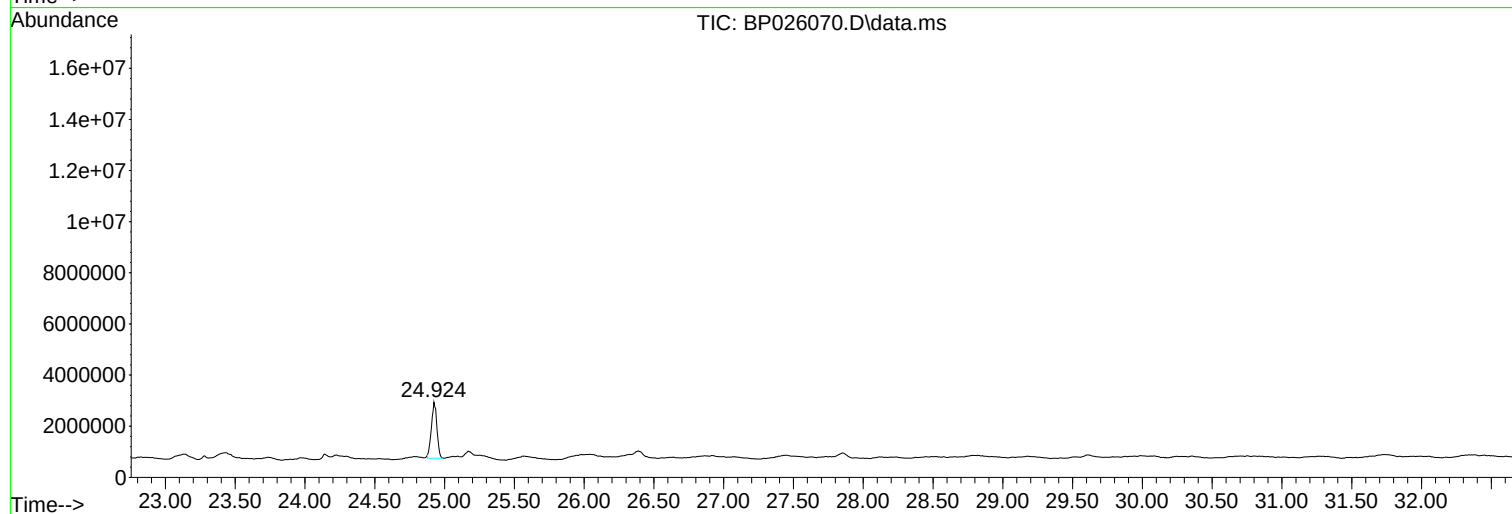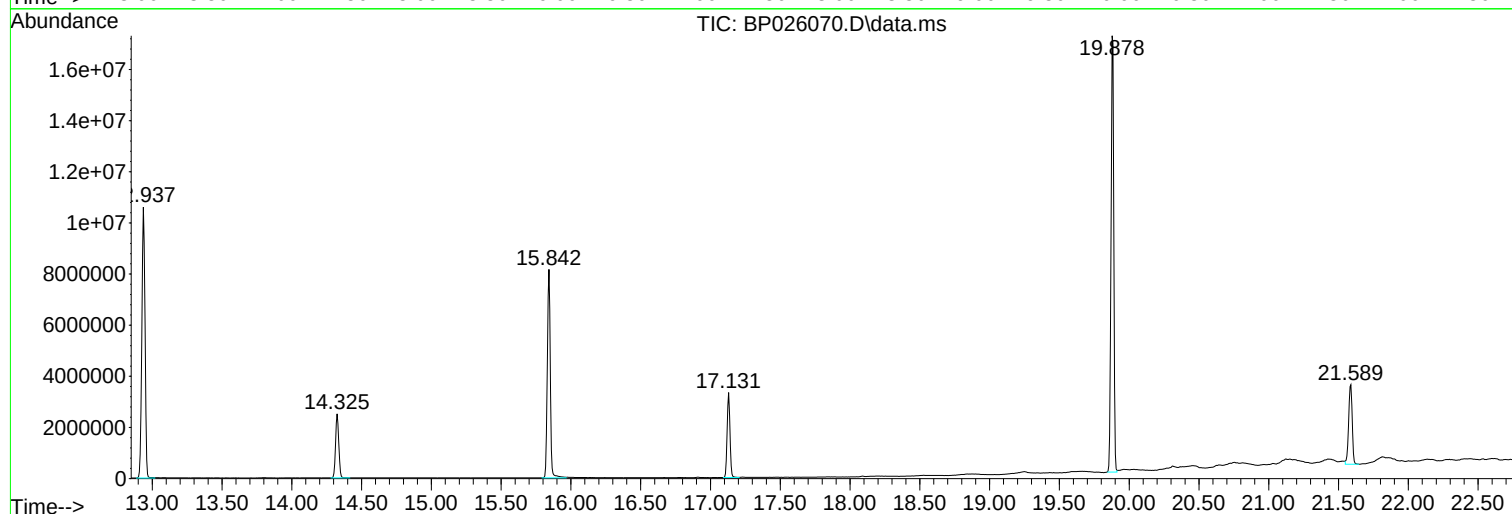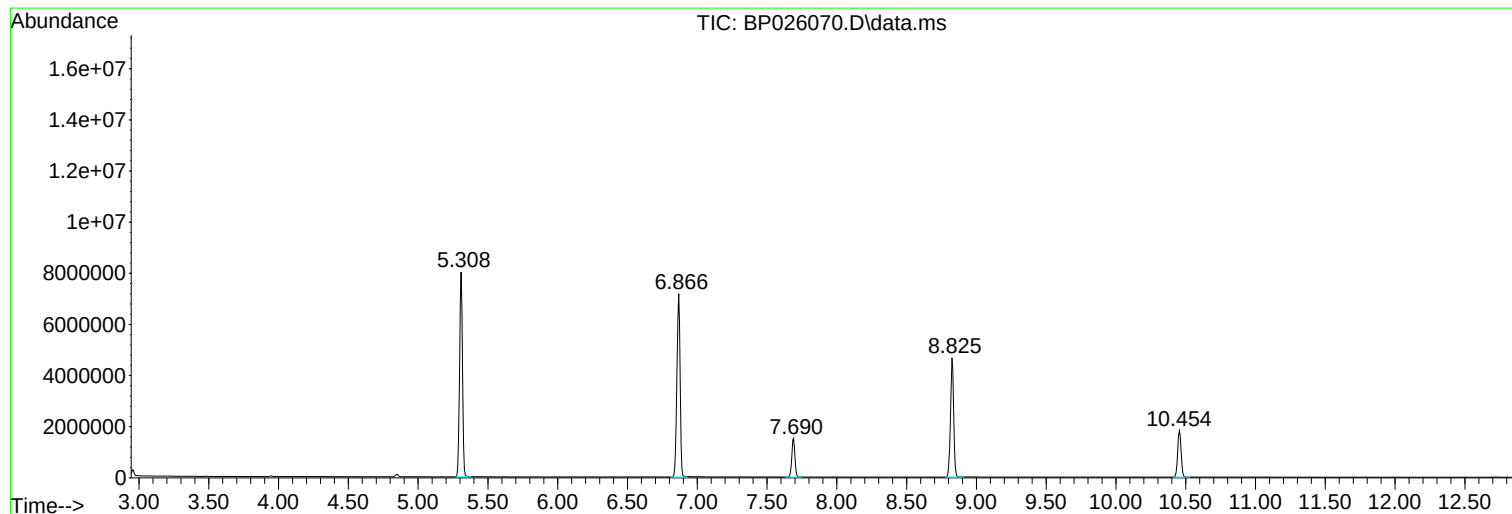

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110425\
Data File : BP026070.D
Acq On : 04 Nov 2025 14:11
Operator : RC/JU
Sample : PB170372BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB170372BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP102925.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110425\
Data File : BP026070.D
Acq On : 04 Nov 2025 14:11
Operator : RC/JU
Sample : PB170372BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB170372BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP102925.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------