
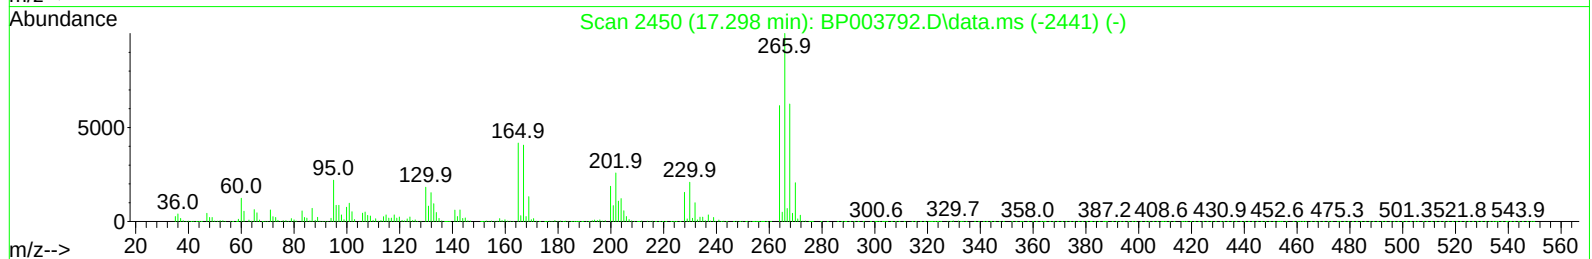
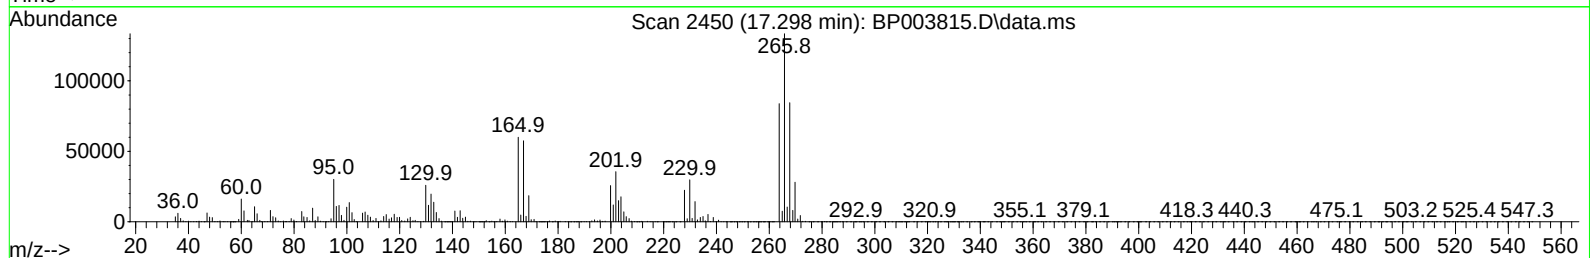


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110520\
Data File : BP003815.D
Acq On : 05 Nov 2020 09:35
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 06 03:34:08 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP110320.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 05 14:31:45 2020
Response via : Initial Calibration

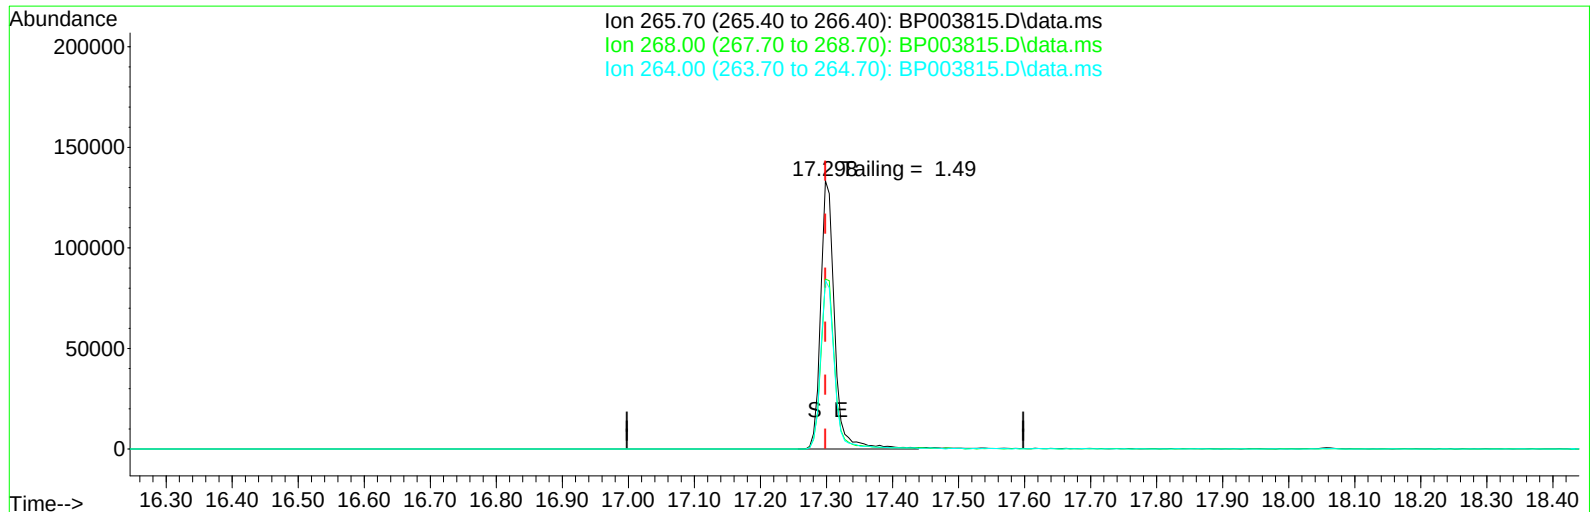

TIC: BP003815.D\data.ms

(70) Pentachlorophenol (C)




17.298min (+ 0.000) 2046350.84 ng

response 196033

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.90	63.35
264.00	63.30	62.81
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110520\
Data File : BP003815.D
Acq On : 05 Nov 2020 09:35
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 06 03:34:08 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP110320.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 05 14:31:45 2020
Response via : Initial Calibration

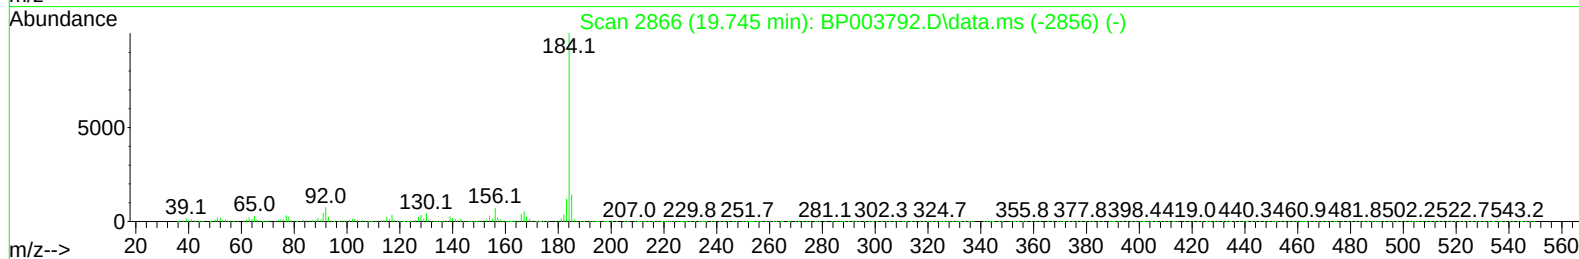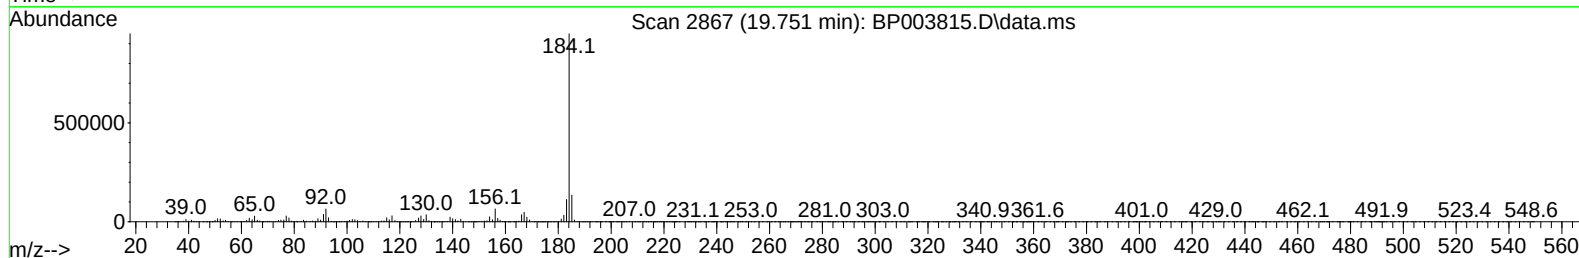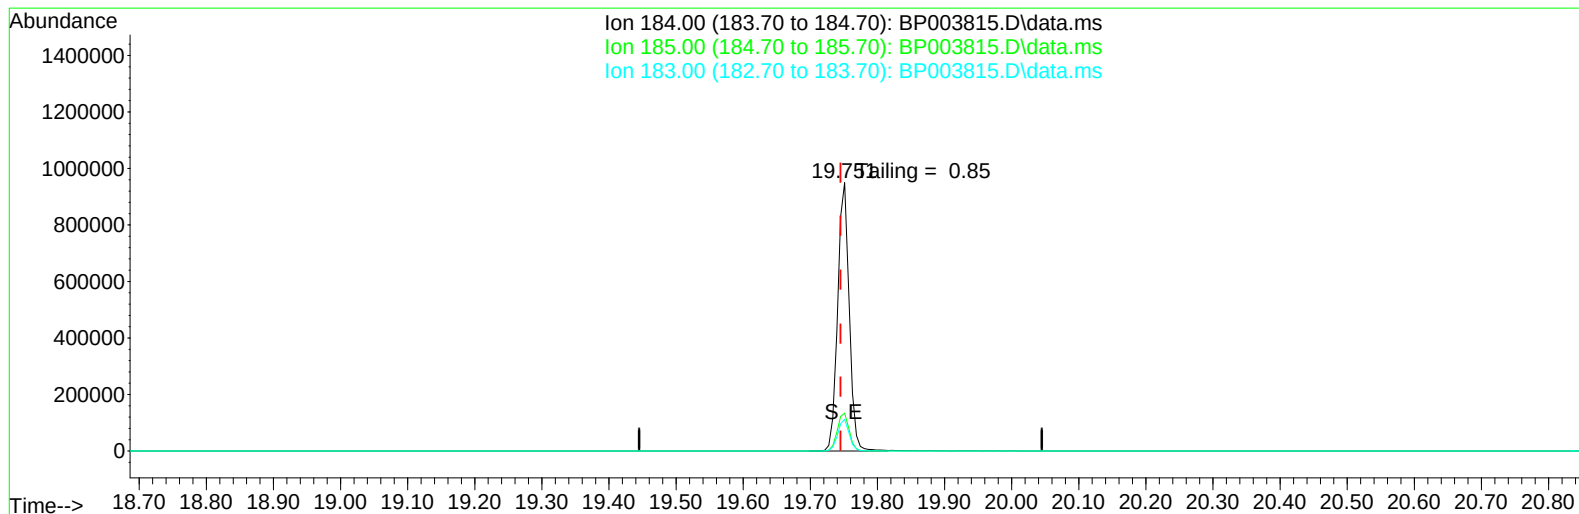

TIC: BP003815.D\data.ms

(77) Benzidine

19.751min (+ 0.006) 1053952.62 ng

response 1143569

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	14.15
183.00	12.00	11.82
0.00	0.00	0.00