

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110520\
 Data File : BP003821.D
 Acq On : 05 Nov 2020 15:18
 Operator : CG/JU
 Sample : L4625-12
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 CONTAINER-002-A-B-COMP

Manual Integrations
 APPROVED

mohammad
 11/6/2020 10:32:42 AM

Quant Time: Nov 05 16:35:17 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP110320.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Nov 05 14:31:45 2020
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.299	152	161187	20.00	ng	0.00
21) Naphthalene-d8	11.128	136	608194	20.00	ng	# 0.00
39) Acenaphthene-d10	14.910	164	357233	20.00	ng	0.00
64) Phenanthrene-d10	17.633	188	702983	20.00	ng	# 0.00
76) Chrysene-d12	21.657	240	673837	20.00	ng	0.00
86) Perylene-d12	24.127	264	731014	20.00	ng	0.02
System Monitoring Compounds						
5) 2-Fluorophenol	5.816	112	1067359	110.52	ng	0.00
7) Phenol-d6	7.458	99	1334960	96.29	ng	0.00
23) Nitrobenzene-d5	9.457	82	842745	67.86	ng	0.00
42) 2,4,6-Tribromophenol	16.386	330	474272	106.15	ng	0.00
45) 2-Fluorobiphenyl	13.540	172	1682277	65.84	ng	0.00
79) Terphenyl-d14	20.127	244	1972815	56.56	ng	0.00
Target Compounds						Qvalue
50) Dimethylphthalate	14.334	163	209616	7.51	ng	99
71) Phenanthrene	17.675	178	219703	5.57	ng	99
75) Fluoranthene	19.604	202	884272	19.42	ng	98
78) Pyrene	19.951	202	814012	17.80	ng	97
81) Benzo(a)anthracene	21.639	228	547551	12.32	ng	98
83) Chrysene	21.692	228	489837	11.47	ng	96
87) Indeno(1,2,3-cd)pyrene	26.662	276	142475	2.70	ng	95
88) Benzo(b)fluoranthene	23.380	252	489023m	10.22	ng	
89) Benzo(k)fluoranthene	23.416	252	185314m	3.92	ng	
90) Benzo(a)pyrene	24.015	252	294057	6.64	ng	98
92) Benzo(g,h,i)perylene	27.451	276	121549	2.86	ng	96

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110520\
Data File : BP003821.D
Acq On : 05 Nov 2020 15:18
Operator : CG/JU
Sample : L4625-12
Misc :
ALS Vial : 7 Sample Multiplier: 1


Instrument :
BNA_P
ClientSampleId :
CONTAINER-002-A-B-COMP

Manual Integrations
APPROVED

mohammad
11/6/2020 10:32:42 AM


Quant Time: Nov 05 16:35:17 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP110320.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 05 14:31:45 2020
Response via : Initial Calibration

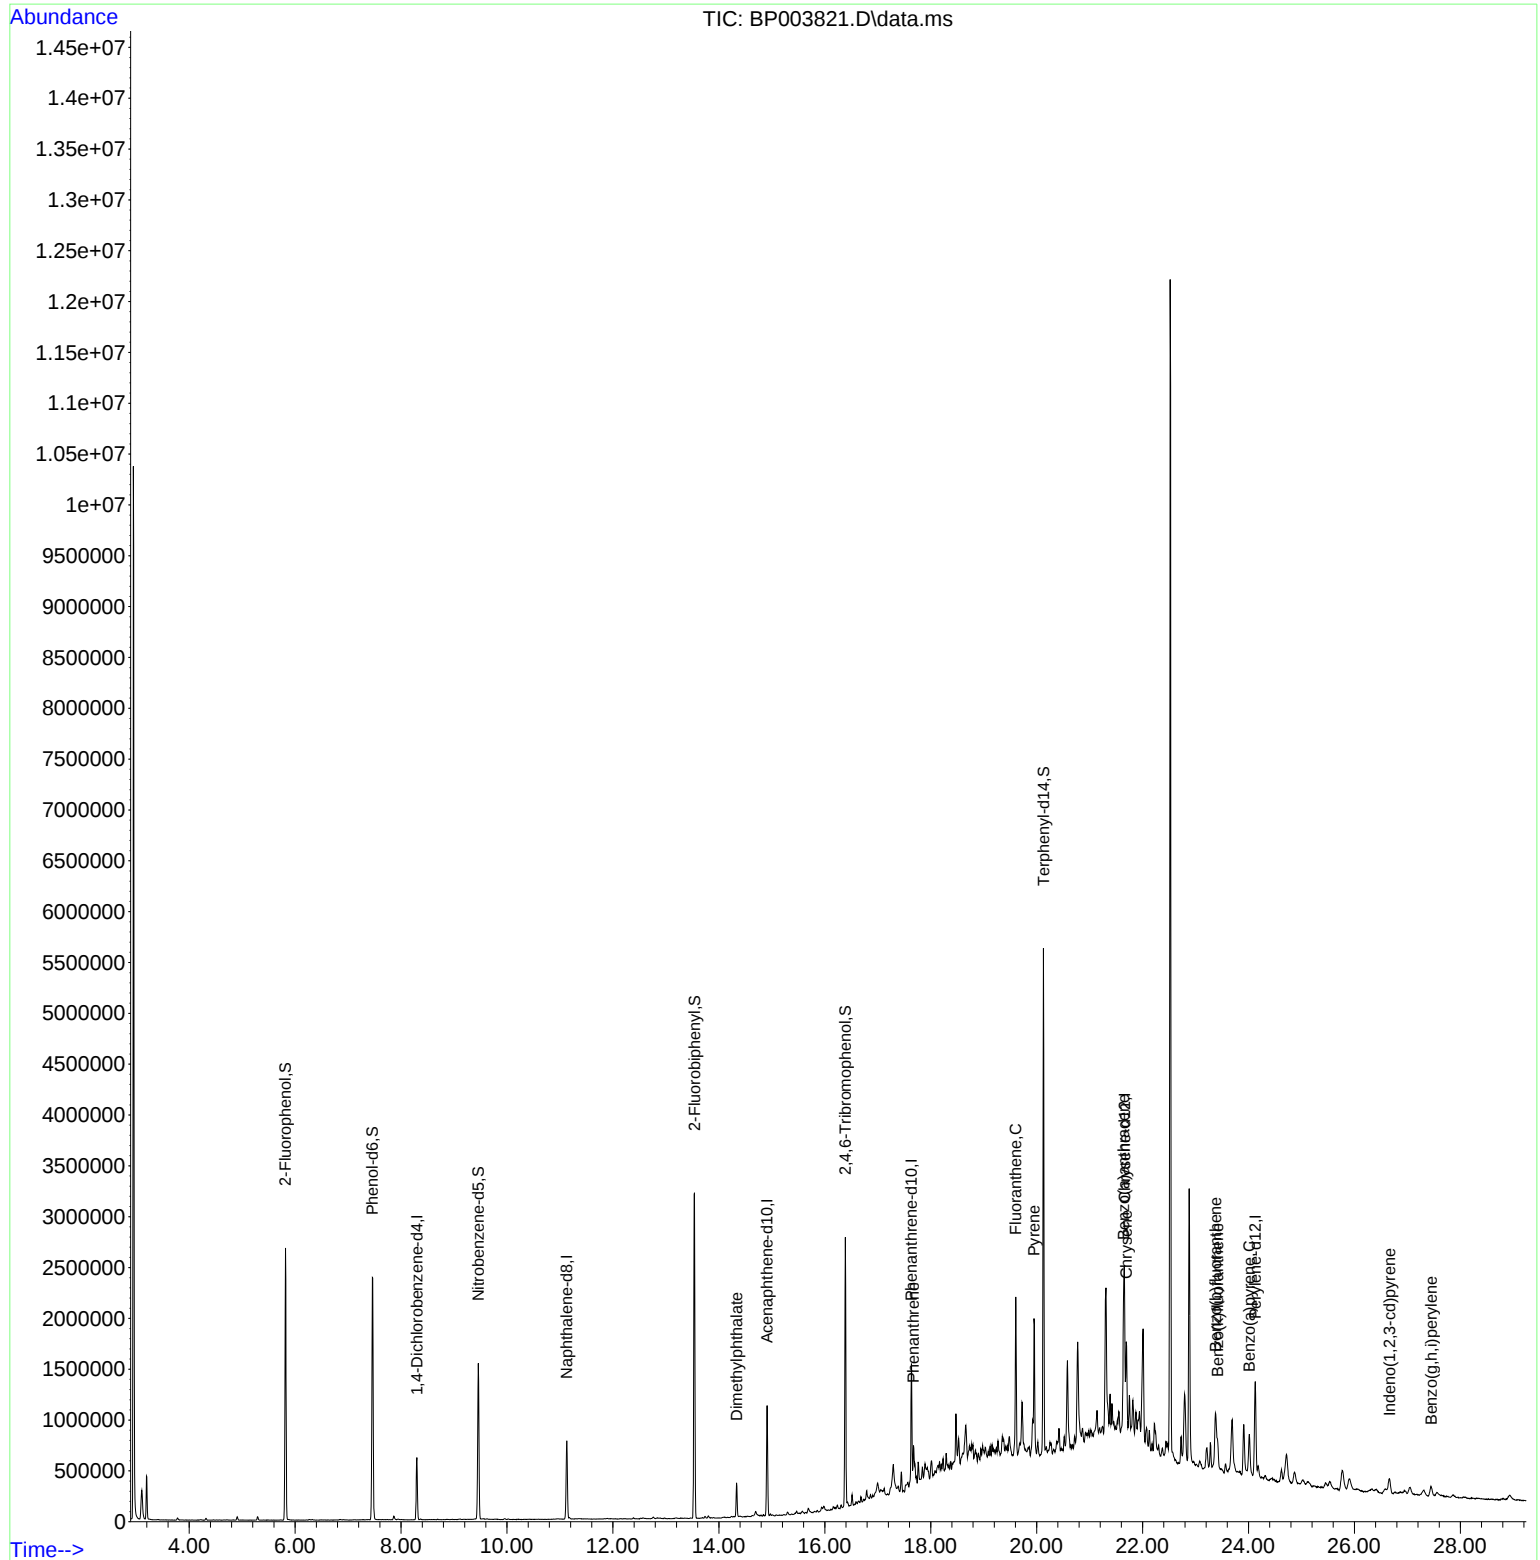



#1
1,4-Dichlorobenzene-d4
Concen: 20.00 ng
RT: 8.299 min Scan# 920
Delta R.T. 0.006 min
Lab File: BP003821.D
Acq: 05 Nov 2020 15:18




Instrument :
BNA_P
ClientSampleId :
CONTAINER-002-A-B-COMP




Tgt Ion:152 Resp: 161187
Ion Ratio Lower Upper
152 100
150 154.7 123.8 185.6
115 60.0 43.8 65.6

Manual Integrations
APPROVED



mohammad
11/6/2020 10:32:42 AM

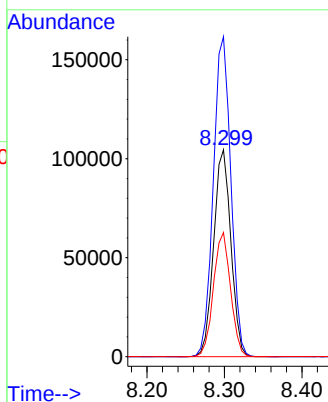


#5
2-Fluorophenol
Concen: 110.52 ng
RT: 5.816 min Scan# 498
Delta R.T. 0.005 min
Lab File: BP003821.D
Acq: 05 Nov 2020 15:18




Tgt Ion:112 Resp: 1067359
Ion Ratio Lower Upper
112 100
64 63.3 32.8 49.2#
63 32.8 17.0 25.4#

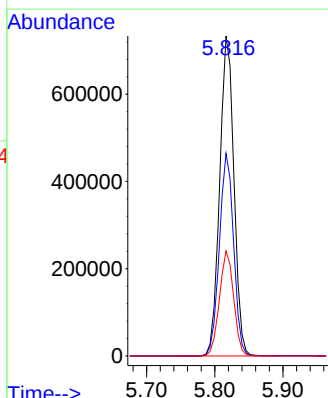



#7
Phenol-d6
Concen: 96.29 ng
RT: 7.458 min Scan# 777
Delta R.T. -0.000 min
Lab File: BP003821.D
Acq: 05 Nov 2020 15:18




Instrument :
BNA_P
ClientSampleId :
CONTAINER-002-A-B-COMP




Tgt Ion: 99 Resp: 1334960
Ion Ratio Lower Upper
99 100
42 19.1 8.6 13.0#
71 36.0 23.4 35.2#

Manual Integrations
APPROVED



mohammad
11/6/2020 10:32:42 AM

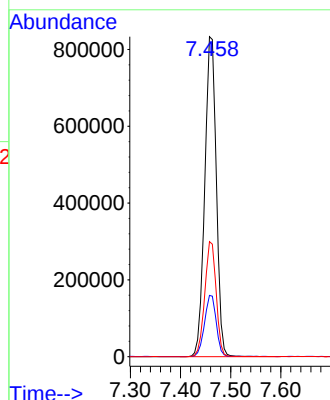


#21
Naphthalene-d8
Concen: 20.00 ng
RT: 11.128 min Scan# 1401
Delta R.T. -0.000 min
Lab File: BP003821.D
Acq: 05 Nov 2020 15:18



Tgt Ion: 136 Resp: 608194
Ion Ratio Lower Upper
136 100
137 11.1 8.6 13.0
54 9.5 3.6 5.4#
68 5.9 3.3 4.9#

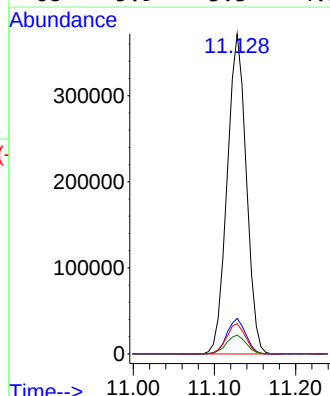







#23
Nitrobenzene-d5
Concen: 67.86 ng
RT: 9.457 min Scan# 1117
Delta R.T. -0.001 min
Lab File: BP003821.D
Acq: 05 Nov 2020 15:18

Tgt Ion: 82 Resp: 842745
Ion Ratio Lower Upper
82 100
128 41.6 45.6 68.4#
54 54.1 30.1 45.1#

Instrument :
BNA_P
ClientSampleId :
CONTAINER-002-A-B-COMP




Manual Integrations
APPROVED


mohammad
11/6/2020 10:32:42 AM

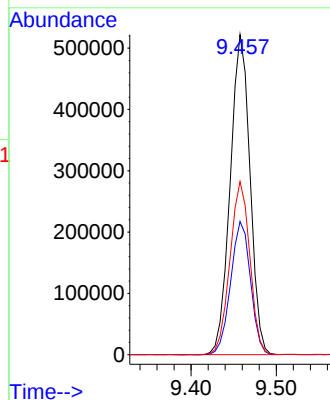

#39
Acenaphthene-d10
Concen: 20.00 ng
RT: 14.910 min Scan# 2044
Delta R.T. 0.000 min
Lab File: BP003821.D
Acq: 05 Nov 2020 15:18


Tgt Ion: 164 Resp: 357233
Ion Ratio Lower Upper
164 100
162 97.8 79.4 119.2
160 42.5 36.1 54.1

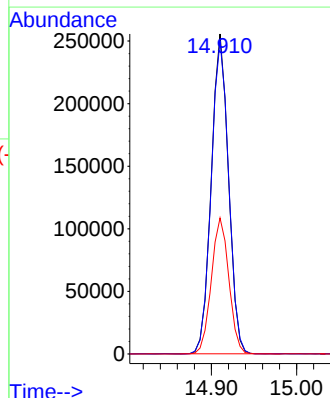



#42
2,4,6-Tribromophenol
Concen: 106.15 ng
RT: 16.386 min Scan# 2295
Delta R.T. -0.001 min
Lab File: BP003821.D
Acq: 05 Nov 2020 15:18




Instrument :
BNA_P
ClientSampleId :
CONTAINER-002-A-B-COMP

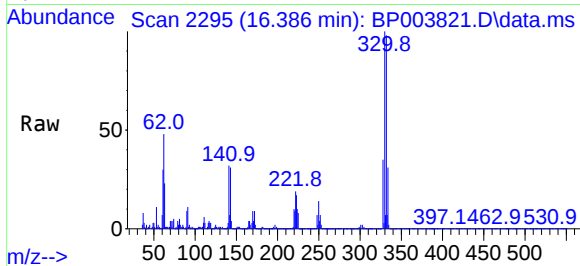


Tgt Ion:330 Resp: 474272
Ion Ratio Lower Upper
330 100
332 98.2 77.1 115.7
141 32.3 23.4 35.2

Manual Integrations
APPROVED



mohammad
11/6/2020 10:32:42 AM

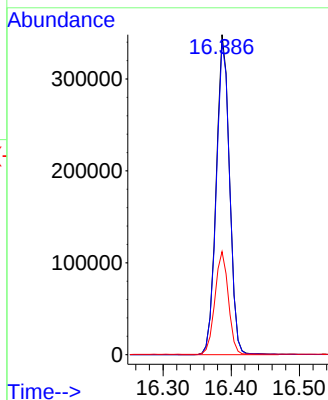


#45
2-Fluorobiphenyl
Concen: 65.84 ng
RT: 13.540 min Scan# 1811
Delta R.T. 0.006 min
Lab File: BP003821.D
Acq: 05 Nov 2020 15:18

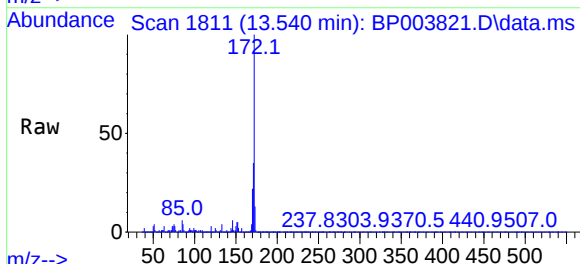


Tgt Ion:172 Resp: 1682277
Ion Ratio Lower Upper
172 100
171 34.8 28.5 42.7
170 22.4 19.2 28.8

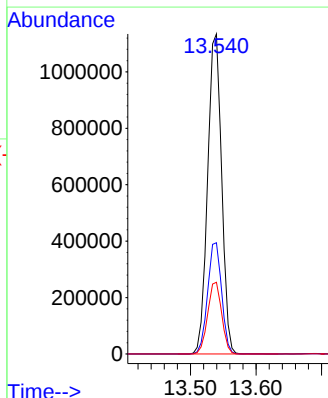



#50
Dimethylphthalate
Concen: 7.51 ng
RT: 14.334 min Scan# 1946
Delta R.T. -0.006 min
Lab File: BP003821.D
Acq: 05 Nov 2020 15:18




Instrument :
BNA_P
ClientSampleId :
CONTAINER-002-A-B-COMP

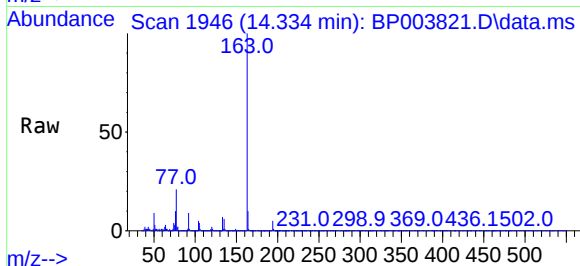

Tgt Ion:163 Resp: 209616
Ion Ratio Lower Upper
163 100
194 4.7 3.3 4.9
164 10.4 8.2 12.2




Manual Integrations
APPROVED


mohammad
11/6/2020 10:32:42 AM

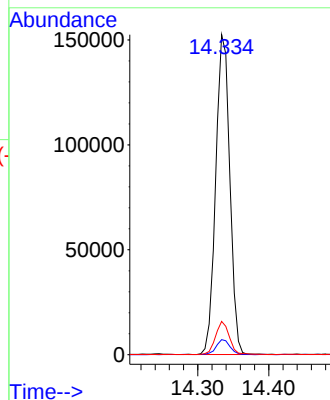

#64
Phenanthrene-d10
Concen: 20.00 ng
RT: 17.633 min Scan# 2507
Delta R.T. -0.001 min
Lab File: BP003821.D
Acq: 05 Nov 2020 15:18

Tgt Ion:188 Resp: 702983
Ion Ratio Lower Upper
188 100
94 8.6 6.2 9.2
80 9.8 6.2 9.2#

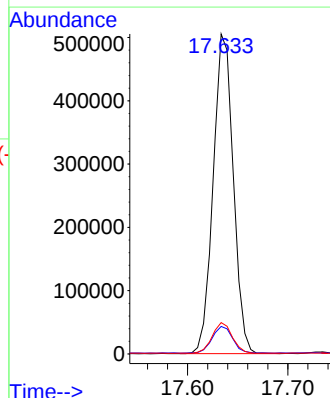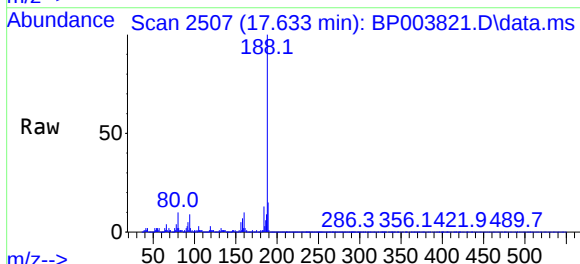







#71
Phenanthrene
Concen: 5.57 ng
RT: 17.675 min Scan# 2514
Delta R.T. -0.000 min
Lab File: BP003821.D
Acq: 05 Nov 2020 15:18

Tgt Ion:178 Resp: 219703
Ion Ratio Lower Upper
178 100
176 19.4 15.3 22.9
179 16.3 12.5 18.7

Instrument :
BNA_P
ClientSampleId :
CONTAINER-002-A-B-COMP




Manual Integrations
APPROVED


mohammad
11/6/2020 10:32:42 AM

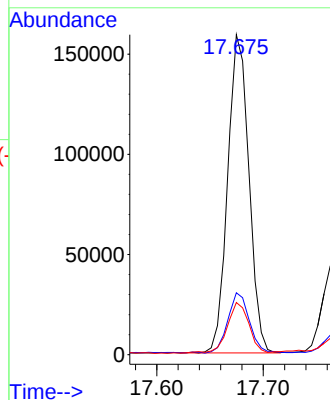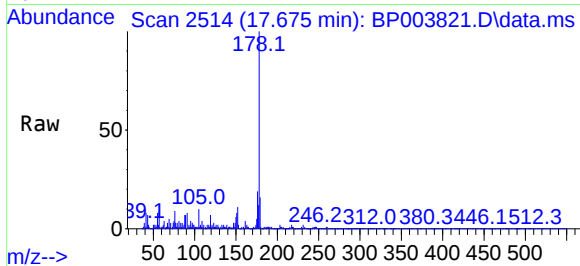

#75
Fluoranthene
Concen: 19.42 ng
RT: 19.604 min Scan# 2842
Delta R.T. 0.006 min
Lab File: BP003821.D
Acq: 05 Nov 2020 15:18

Tgt Ion:202 Resp: 884272
Ion Ratio Lower Upper
202 100
101 10.1 0.0 29.4
203 19.0 0.0 37.8

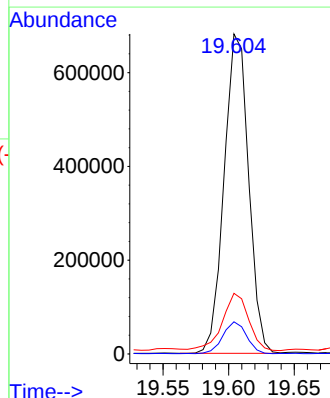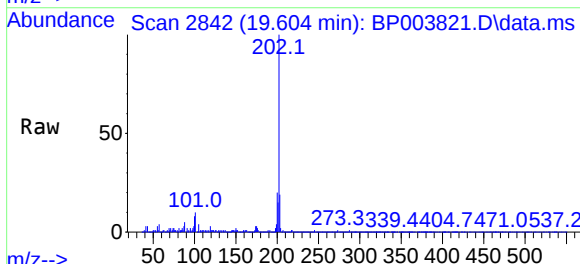







#76
Chrysene-d12
Concen: 20.00 ng
RT: 21.657 min Scan# 3191
Delta R.T. 0.006 min
Lab File: BP003821.D
Acq: 05 Nov 2020 15:18

Tgt Ion:240 Resp: 673837
Ion Ratio Lower Upper
240 100
120 9.5 7.8 11.6
236 24.9 20.8 31.2

Instrument :
BNA_P
ClientSampleId :
CONTAINER-002-A-B-COMP




Manual Integrations
APPROVED


mohammad
11/6/2020 10:32:42 AM

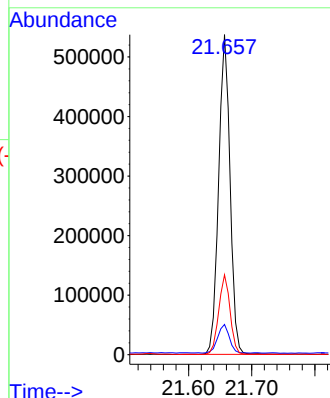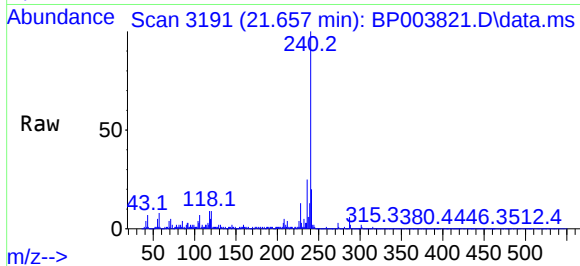

#78
Pyrene
Concen: 17.80 ng
RT: 19.951 min Scan# 2901
Delta R.T. -0.000 min
Lab File: BP003821.D
Acq: 05 Nov 2020 15:18

Tgt Ion:202 Resp: 814012
Ion Ratio Lower Upper
202 100
200 20.4 17.1 25.7
203 19.2 14.2 21.2

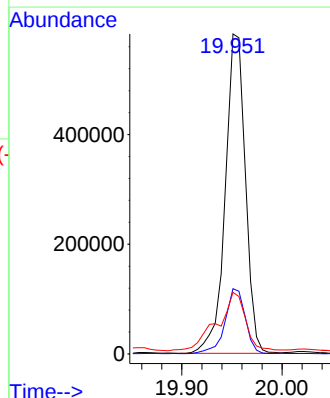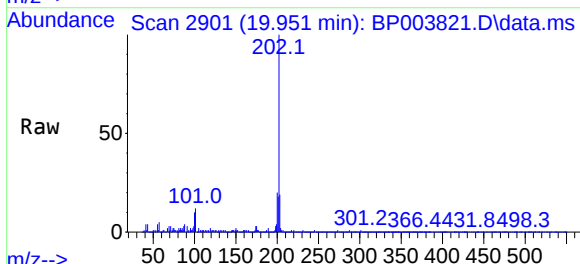



#79
Terphenyl-d14
Concen: 56.56 ng
RT: 20.127 min Scan# 2931
Delta R.T. 0.005 min
Lab File: BP003821.D
Acq: 05 Nov 2020 15:18





Tgt Ion:244 Resp: 1972815

Ion	Ratio	Lower	Upper
244	100		
212	7.2	5.8	8.6
122	9.1	7.8	11.8

Instrument :
BNA_P
ClientSampleId :
CONTAINER-002-A-B-COMP

Manual Integrations
APPROVED




mohammad
11/6/2020 10:32:42 AM

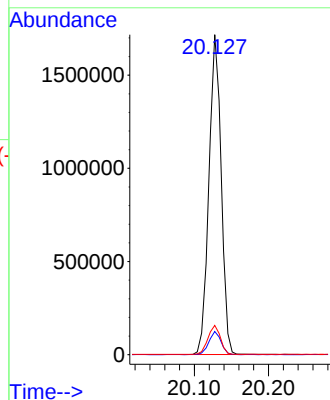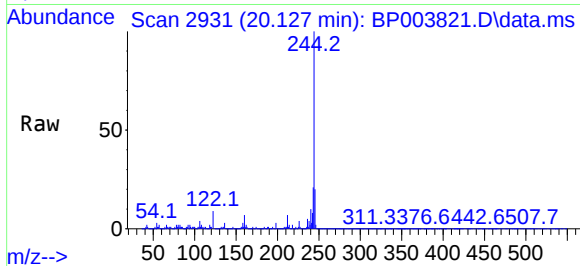


#81
Benzo(a)anthracene
Concen: 12.32 ng
RT: 21.639 min Scan# 3188
Delta R.T. 0.006 min
Lab File: BP003821.D
Acq: 05 Nov 2020 15:18


Tgt Ion:228 Resp: 547551

Ion	Ratio	Lower	Upper
228	100		
226	26.7	22.1	33.1
229	21.5	15.9	23.9

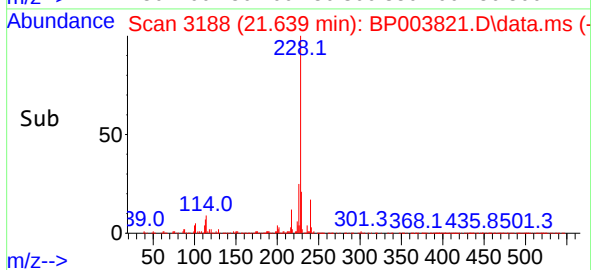
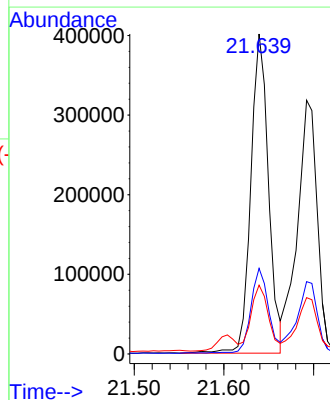
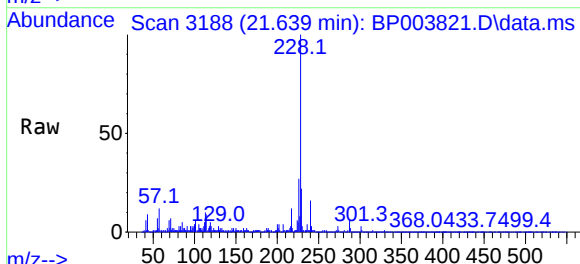





#83
Chrysene
Concen: 11.47 ng
RT: 21.692 min Scan# 3197
Delta R.T. 0.006 min
Lab File: BP003821.D
Acq: 05 Nov 2020 15:18





Tgt Ion:228 Resp: 489837
Ion Ratio Lower Upper
228 100
226 28.5 24.4 36.6
229 22.2 15.8 23.6

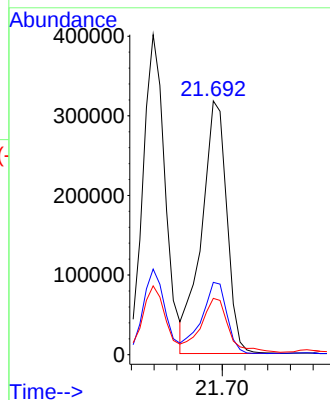

#86
Perylene-d12
Concen: 20.00 ng
RT: 24.127 min Scan# 3611
Delta R.T. 0.018 min
Lab File: BP003821.D
Acq: 05 Nov 2020 15:18




Tgt Ion:264 Resp: 731014
Ion Ratio Lower Upper
264 100
260 23.0 18.8 28.2
265 21.6 17.4 26.2

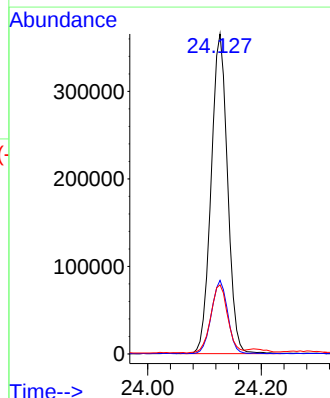

Instrument :
BNA_P
ClientSampleId :
CONTAINER-002-A-B-COMP


Manual Integrations
APPROVED

mohammad
11/6/2020 10:32:42 AM



#87
 Indeno(1,2,3-cd)pyrene
 Concen: 2.70 ng
 RT: 26.662 min Scan# 4042
 Delta R.T. 0.012 min
 Lab File: BP003821.D
 Acq: 05 Nov 2020 15:18




Instrument :
 BNA_P
 ClientSampleId :
 CONTAINER-002-A-B-COMP

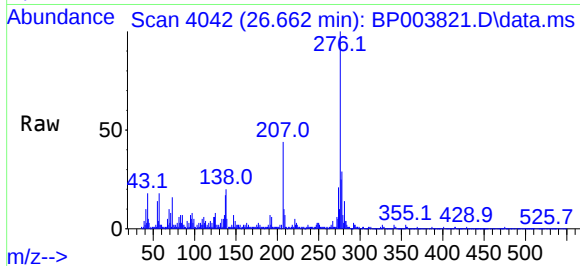


Tgt Ion: 276 Resp: 142475
 Ion Ratio Lower Upper
 276 100
 138 19.5 18.7 28.1
 277 24.3 20.4 30.6

Manual Integrations
 APPROVED



mohammad
 11/6/2020 10:32:42 AM

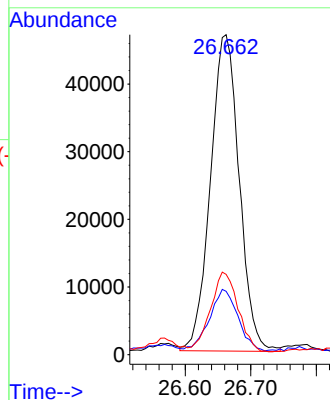


#88
 Benzo(b)fluoranthene
 Concen: 10.22 ng m
 RT: 23.380 min Scan# 3484
 Delta R.T. 0.023 min
 Lab File: BP003821.D
 Acq: 05 Nov 2020 15:18

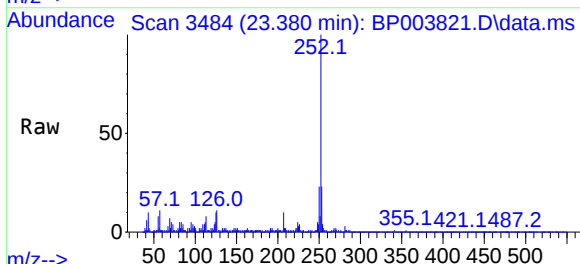

Tgt Ion: 252 Resp: 489023
 Ion Ratio Lower Upper
 252 100
 253 23.3 17.6 26.4
 125 10.4 7.3 10.9

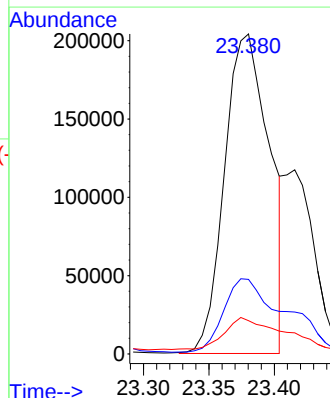







#89
Benzo(k)fluoranthene
Concen: 3.92 ng m
RT: 23.416 min Scan# 3490
Delta R.T. 0.006 min
Lab File: BP003821.D
Acq: 05 Nov 2020 15:18

Tgt Ion:252 Resp: 185314
Ion Ratio Lower Upper
252 100
253 22.7 17.8 26.8
125 11.5 7.4 11.2#

Instrument :
BNA_P
ClientSampleId :
CONTAINER-002-A-B-COMP




Manual Integrations
APPROVED


mohammad
11/6/2020 10:32:42 AM

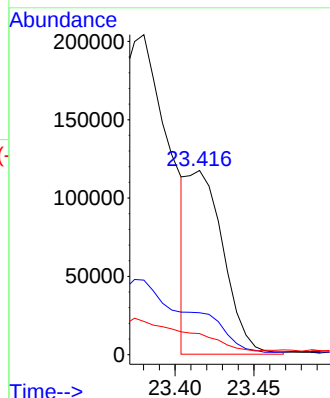

#90
Benzo(a)pyrene
Concen: 6.64 ng
RT: 24.015 min Scan# 3592
Delta R.T. 0.018 min
Lab File: BP003821.D
Acq: 05 Nov 2020 15:18


Tgt Ion:252 Resp: 294057
Ion Ratio Lower Upper
252 100
253 22.5 17.4 26.0
125 11.1 8.2 12.4

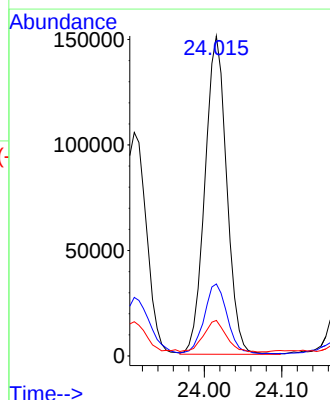



#92
Benzo(g,h,i)perylene
Concen: 2.86 ng
RT: 27.451 min Scan# 4176
Delta R.T. 0.018 min
Lab File: BP003821.D
Acq: 05 Nov 2020 15:18

Instrument :
BNA_P
ClientSampleId :
CONTAINER-002-A-B-COMP



Tgt Ion: 276 Resp: 121549
Ion Ratio Lower Upper
276 100
277 25.5 19.0 28.6
138 18.5 16.6 24.8

Manual Integrations
APPROVED

mohammad
11/6/2020 10:32:42 AM

