
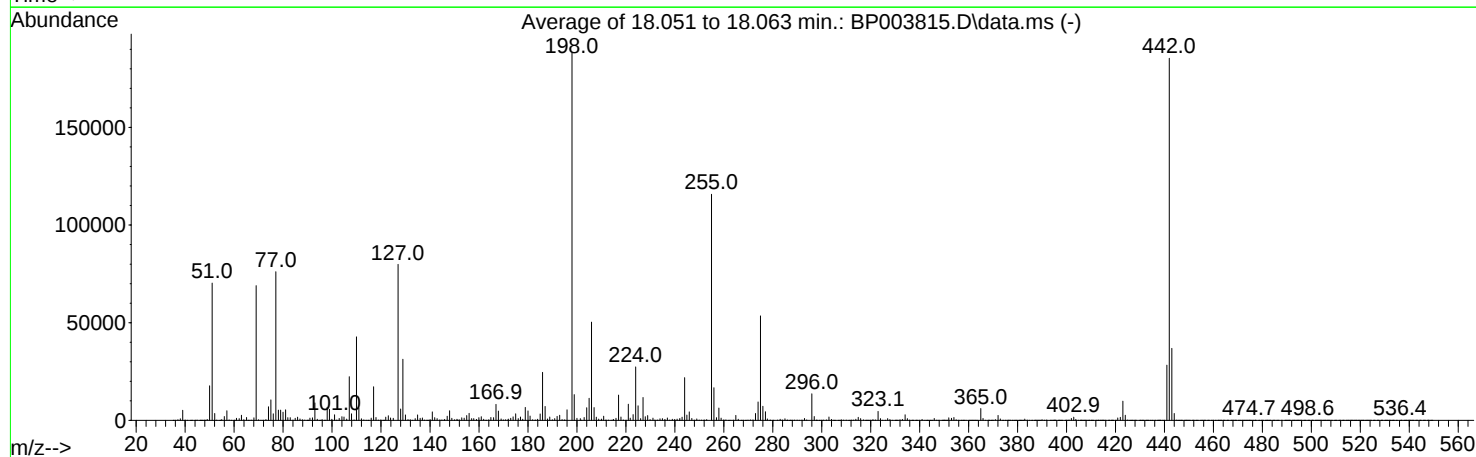


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110520\
Data File : BP003815.D
Acq On : 05 Nov 2020 09:35
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP110320.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue Nov 10 13:41:24 2020

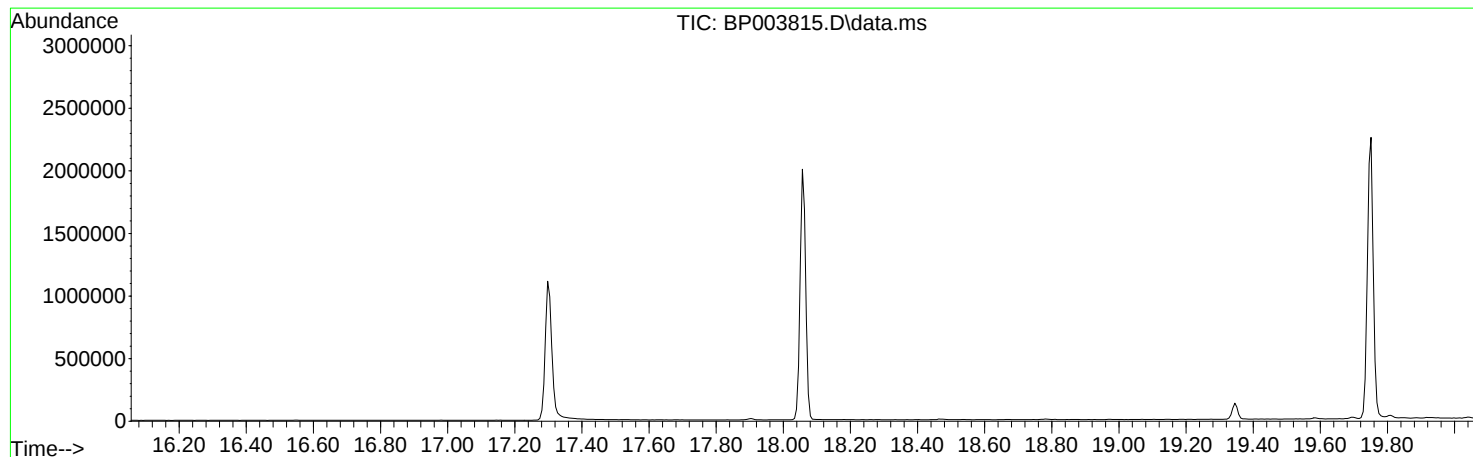

AutoFind: Scans 2578, 2579, 2580; Background Corrected with Scan 2571

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	37.3	70284	PASS
68	69	0.00	2	1.9	1334	PASS
69	198	0.00	100	36.6	68968	PASS
70	69	0.00	2	0.5	372	PASS
127	198	10	80	42.4	79862	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	188355	PASS
199	198	5	9	7.0	13175	PASS
275	198	10	60	28.4	53490	PASS
365	198	1	100	3.2	6051	PASS
441	198	0.01	100	15.0	28298	PASS
442	198	50	100	98.4	185427	PASS
443	442	15	24	19.9	36857	PASS