
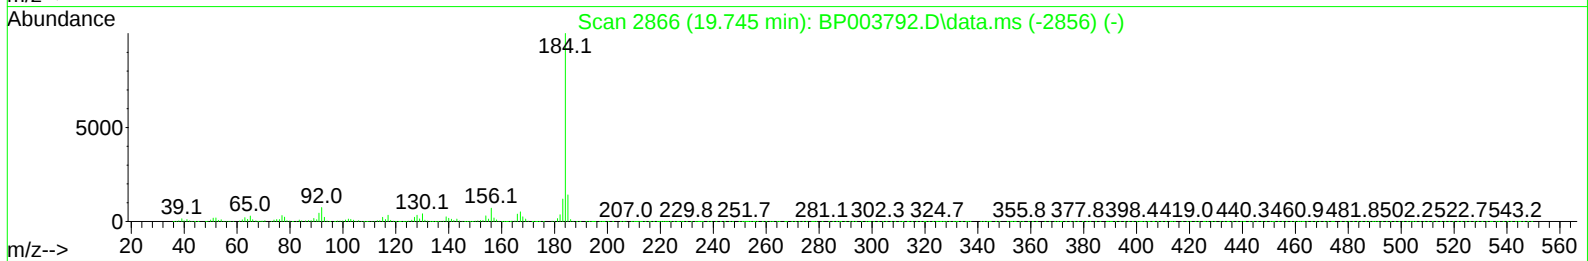
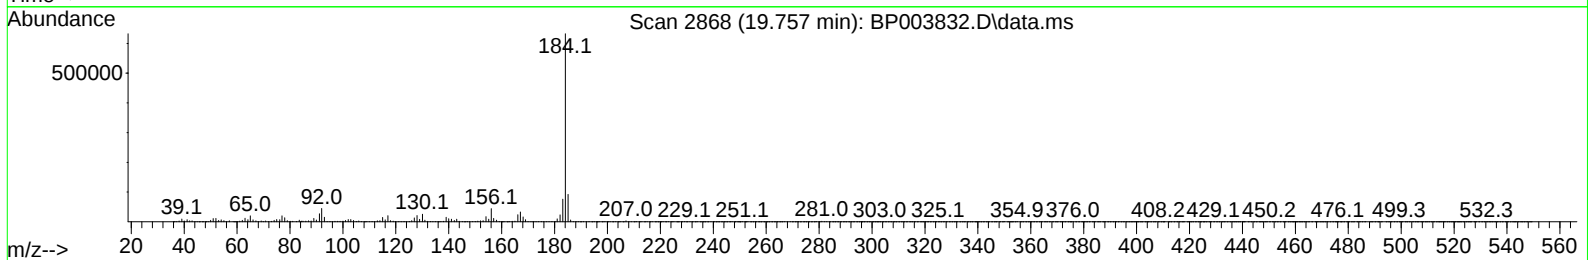


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110620\
Data File : BP003832.D
Acq On : 06 Nov 2020 09:38
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 06 15:17:06 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP110320.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 06 11:33:14 2020
Response via : Initial Calibration

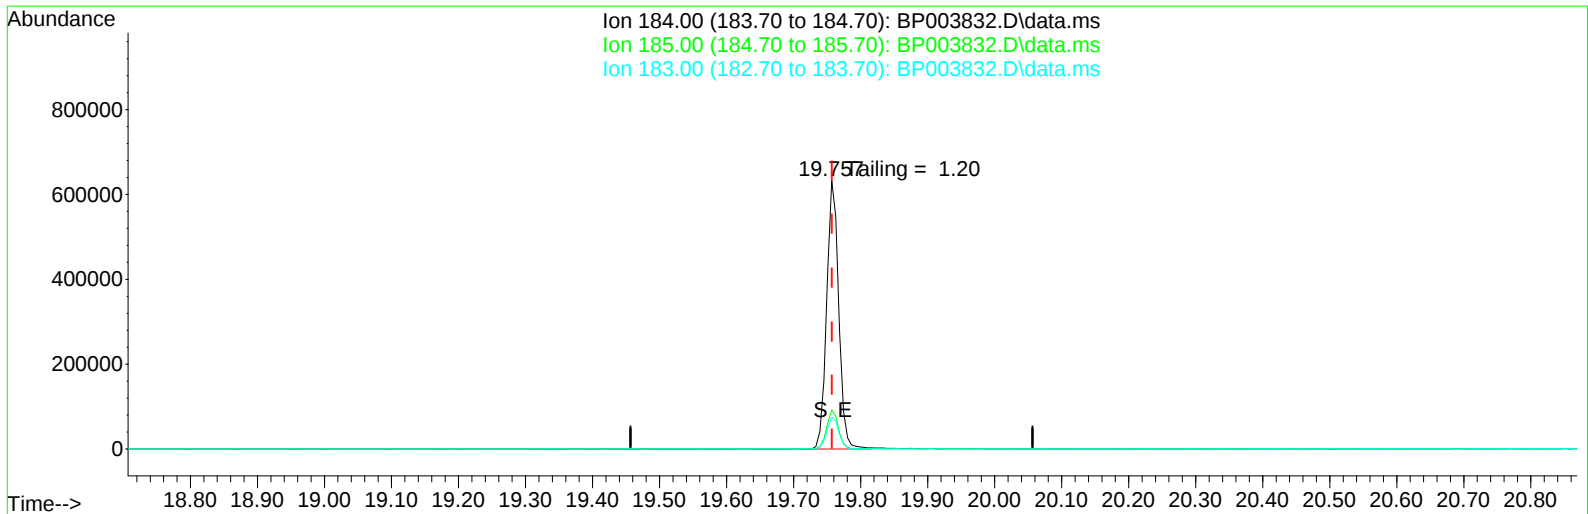




TIC: BP003832.D\data.ms

(77) Benzidine**19.757min (-0.000) 45282.97 ng****response 792542**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	14.57
183.00	12.00	11.97
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110620\
Data File : BP003832.D
Acq On : 06 Nov 2020 09:38
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 06 15:17:06 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP110320.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 06 11:33:14 2020
Response via : Initial Calibration

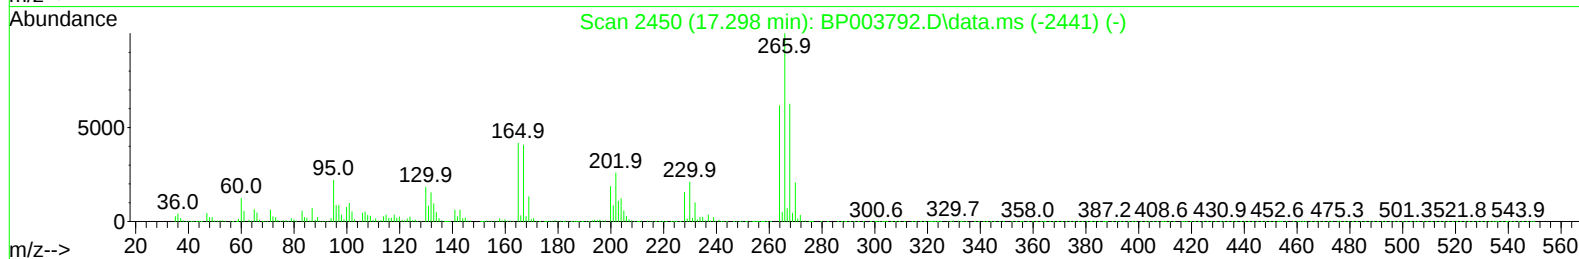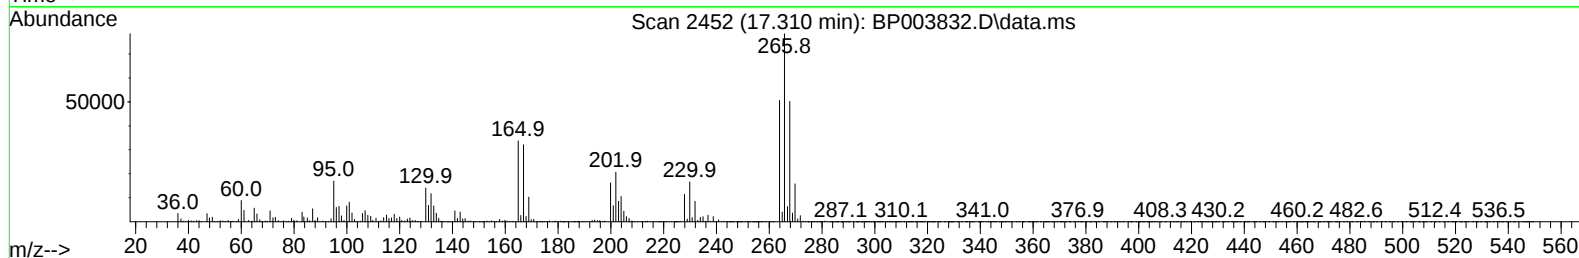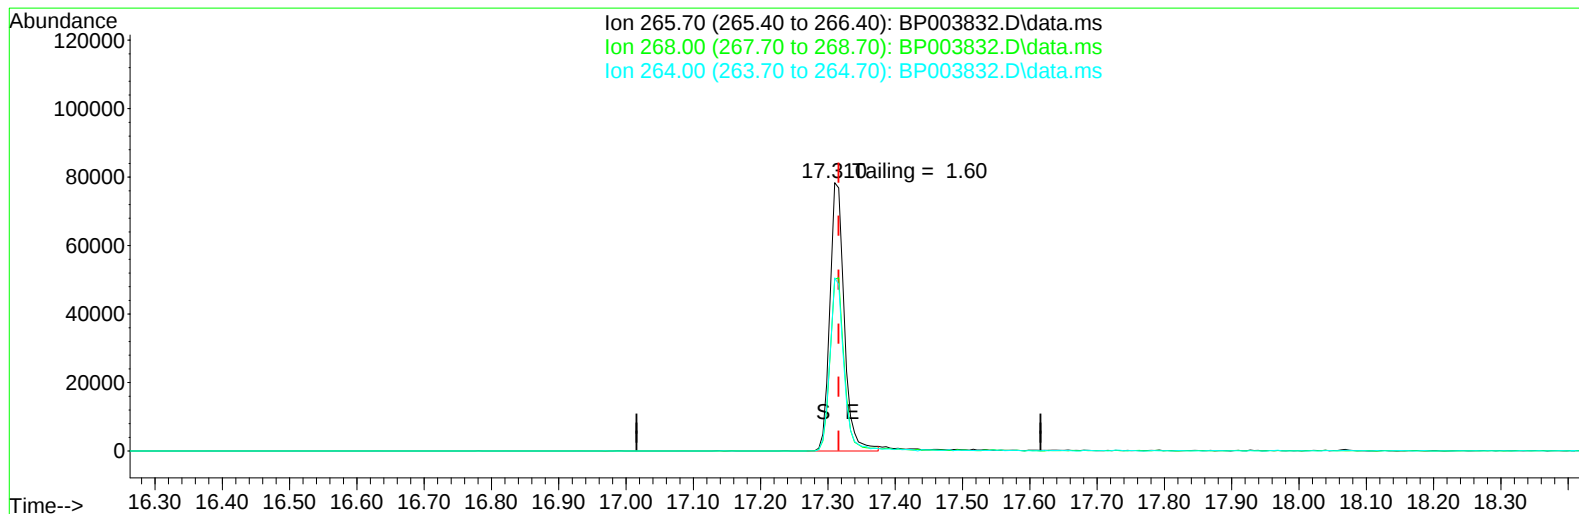

TIC: BP003832.D\data.ms

(70) Pentachlorophenol (C)

17.310min (-0.006) 51829.55 ng

response 118831

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.90	63.98
264.00	63.30	64.53
0.00	0.00	0.00