

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110620\
 Data File : BP003834.D
 Acq On : 06 Nov 2020 10:46
 Operator : CG/JU
 Sample : PB132804BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 PB132804BL

Quant Time: Nov 06 11:40:53 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP110320.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Nov 06 11:33:14 2020
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.299	152	195681	20.00	ng	0.00
21) Naphthalene-d8	11.134	136	731456	20.00	ng	# 0.00
39) Acenaphthene-d10	14.916	164	431861	20.00	ng	0.00
64) Phenanthrene-d10	17.645	188	868277	20.00	ng	# 0.00
76) Chrysene-d12	21.663	240	702428	20.00	ng	0.00
86) Perylene-d12	24.139	264	702317	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.822	112	1478492	126.10	ng	0.00
7) Phenol-d6	7.469	99	1855739	110.26	ng	0.00
23) Nitrobenzene-d5	9.463	82	1166614	78.11	ng	0.00
42) 2,4,6-Tribromophenol	16.398	330	651682	120.65	ng	0.00
45) 2-Fluorobiphenyl	13.545	172	2505994	81.12	ng	0.00
79) Terphenyl-d14	20.133	244	3030884	83.36	ng	0.00


Target Compounds	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110620\
Data File : BP003834.D
Acq On : 06 Nov 2020 10:46
Operator : CG/JU
Sample : PB132804BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB132804BL

Quant Time: Nov 06 11:40:53 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP110320.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 06 11:33:14 2020
Response via : Initial Calibration



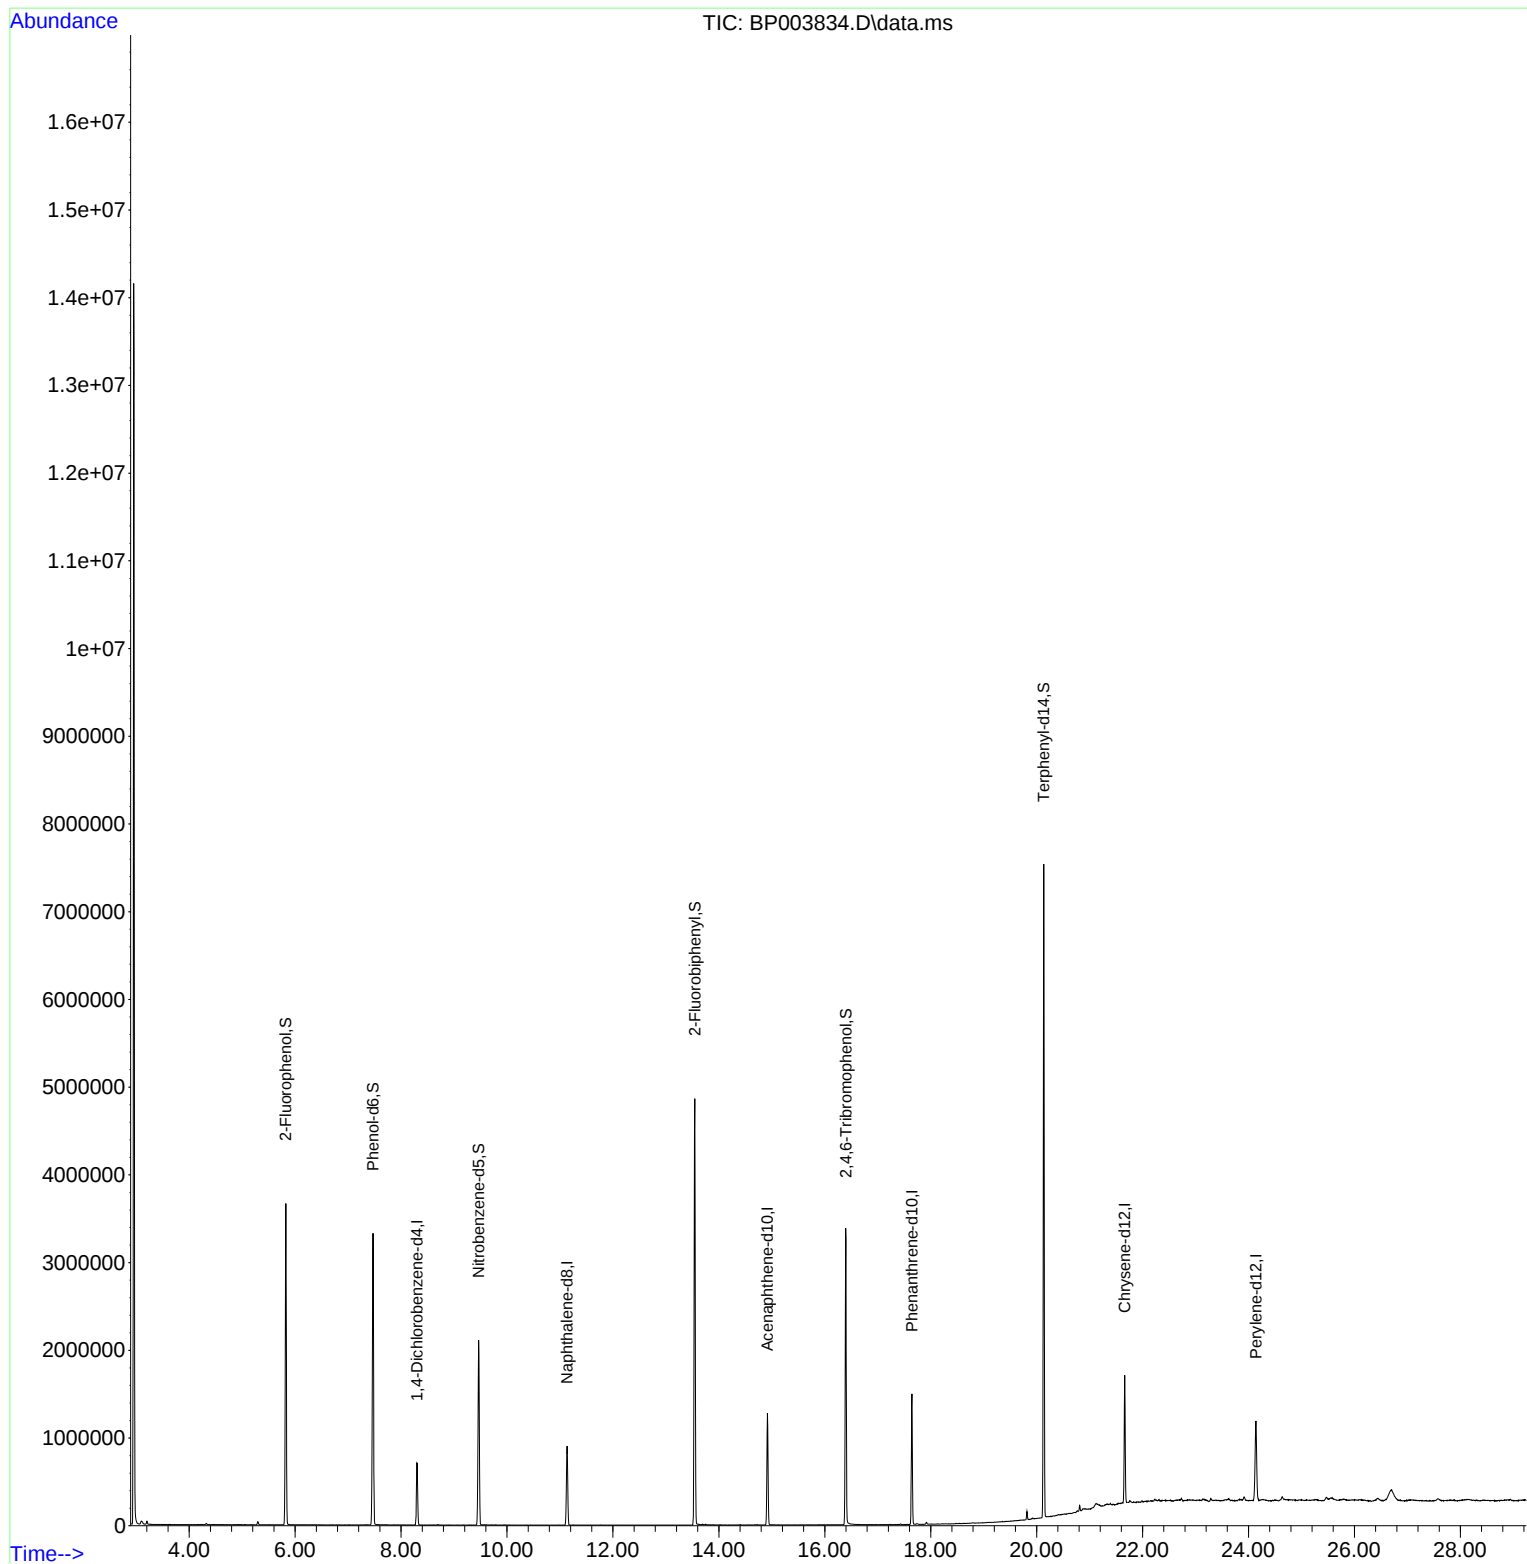




#1
1,4-Dichlorobenzene-d4
Concen: 20.00 ng
RT: 8.299 min Scan# 920
Delta R.T. -0.006 min
Lab File: BP003834.D
Acq: 06 Nov 2020 10:46




Instrument :
BNA_P
ClientSampleId :
PB132804BL

Tgt Ion:152 Resp: 195681
Ion Ratio Lower Upper
152 100
150 151.1 123.8 185.6
115 60.6 43.8 65.6

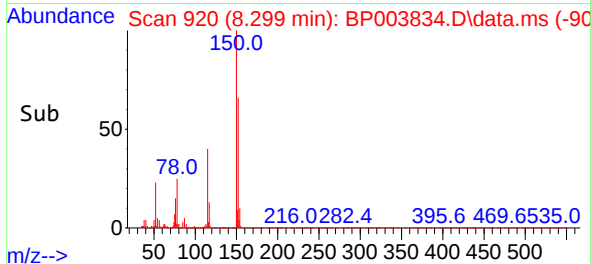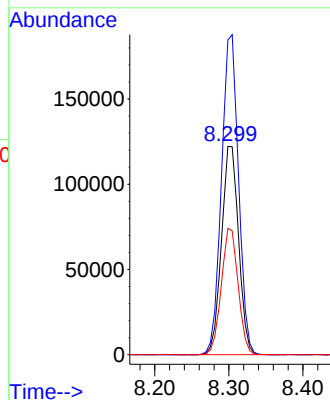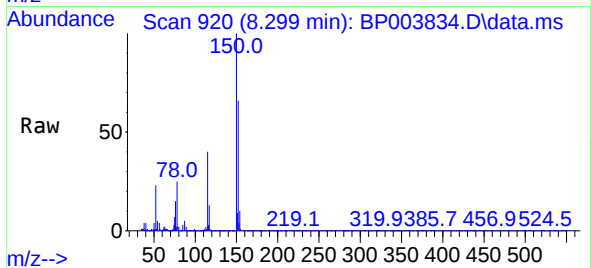

#5
2-Fluorophenol
Concen: 126.10 ng
RT: 5.822 min Scan# 499
Delta R.T. -0.000 min
Lab File: BP003834.D
Acq: 06 Nov 2020 10:46

Tgt Ion:112 Resp: 1478492
Ion Ratio Lower Upper
112 100
64 63.0 32.8 49.2#
63 32.7 17.0 25.4#


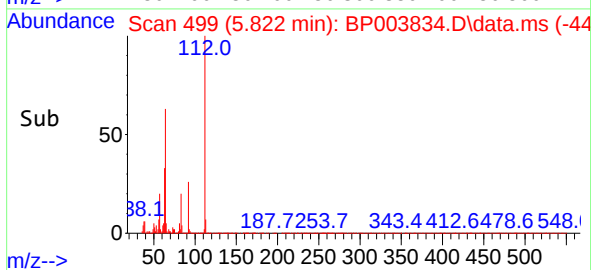
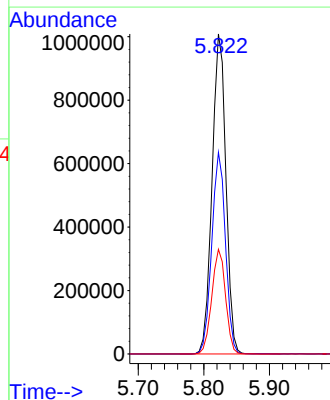
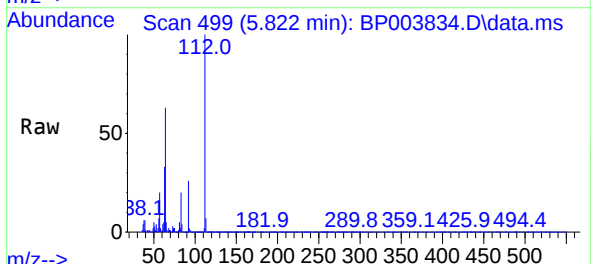




#7
Phenol-d6
Concen: 110.26 ng
RT: 7.469 min Scan# 779
Delta R.T. -0.000 min
Lab File: BP003834.D
Acq: 06 Nov 2020 10:46




Instrument :
BNA_P
ClientSampleId :
PB132804BL


Tgt Ion: 99 Resp: 1855739
Ion Ratio Lower Upper
99 100
42 18.4 8.6 13.0#
71 35.8 23.4 35.2#

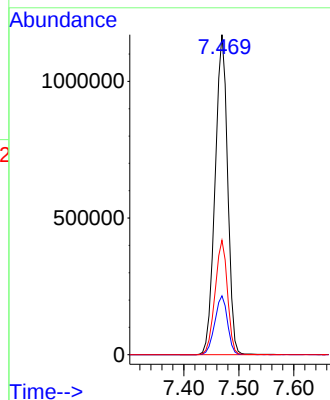

#21
Naphthalene-d8
Concen: 20.00 ng
RT: 11.134 min Scan# 1402
Delta R.T. -0.000 min
Lab File: BP003834.D
Acq: 06 Nov 2020 10:46

Tgt Ion: 136 Resp: 731456
Ion Ratio Lower Upper
136 100
137 11.1 8.6 13.0
54 9.3 3.6 5.4#
68 5.7 3.3 4.9#


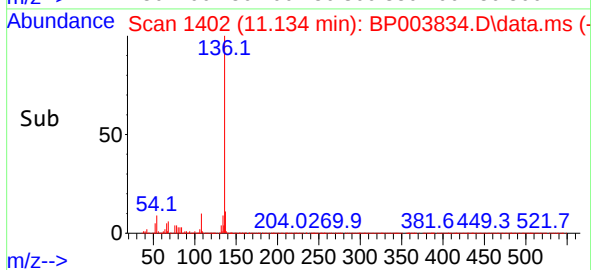
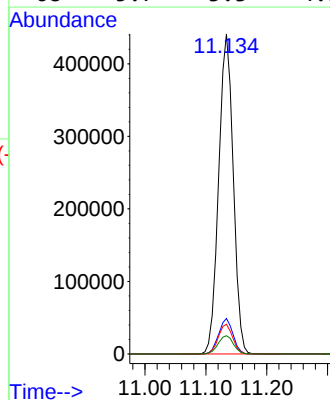
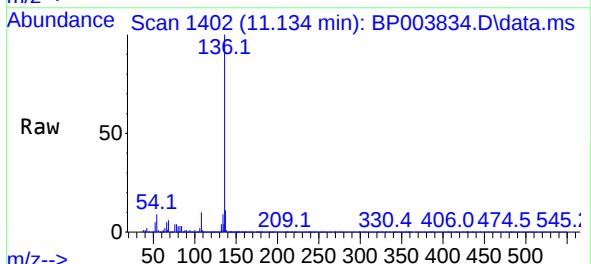




#23
Nitrobenzene-d5
Concen: 78.11 ng
RT: 9.463 min Scan# 1118
Delta R.T. -0.006 min
Lab File: BP003834.D
Acq: 06 Nov 2020 10:46




Instrument :
BNA_P
ClientSampleId :
PB132804BL


Tgt Ion: 82 Resp: 1166614
Ion Ratio Lower Upper
82 100
128 42.5 45.6 68.4#
54 54.7 30.1 45.1#

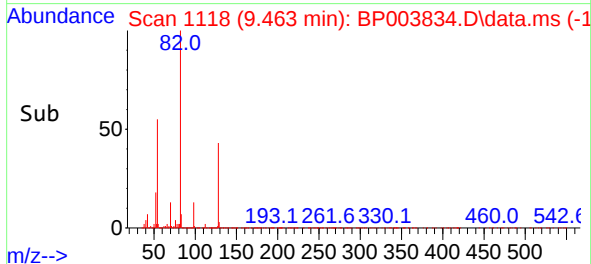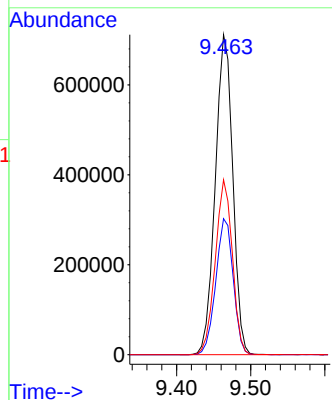

#39
Acenaphthene-d10
Concen: 20.00 ng
RT: 14.916 min Scan# 2045
Delta R.T. -0.000 min
Lab File: BP003834.D
Acq: 06 Nov 2020 10:46

Tgt Ion: 164 Resp: 431861
Ion Ratio Lower Upper
164 100
162 100.0 79.4 119.2
160 42.2 36.1 54.1


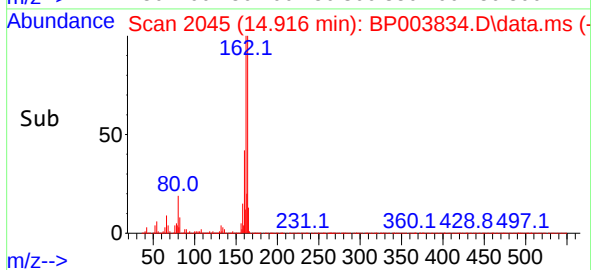
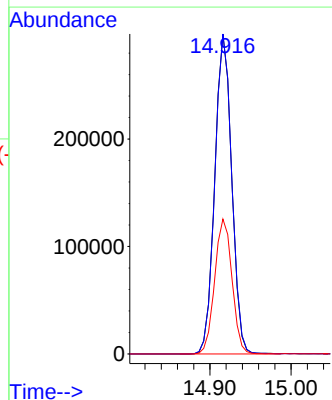
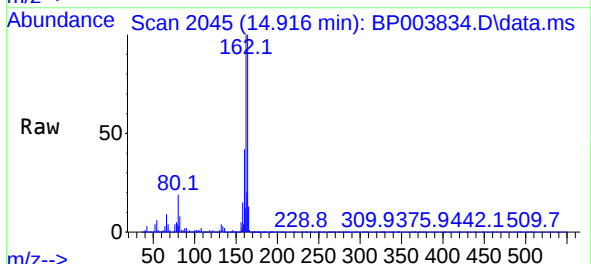




#42
2,4,6-Tribromophenol
Concen: 120.65 ng
RT: 16.398 min Scan# 2297
Delta R.T. -0.000 min
Lab File: BP003834.D
Acq: 06 Nov 2020 10:46




Instrument :
BNA_P
ClientSampleId :
PB132804BL


Tgt Ion:330 Resp: 651682
Ion Ratio Lower Upper
330 100
332 96.8 77.1 115.7
141 30.6 23.4 35.2

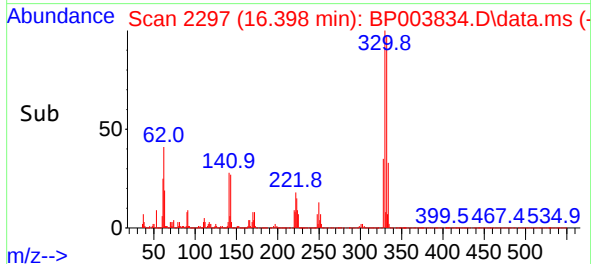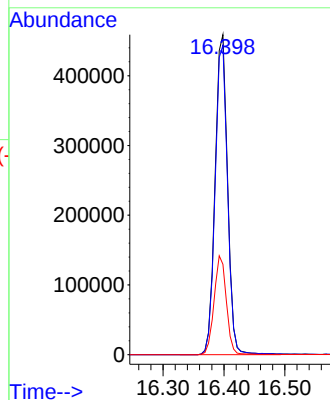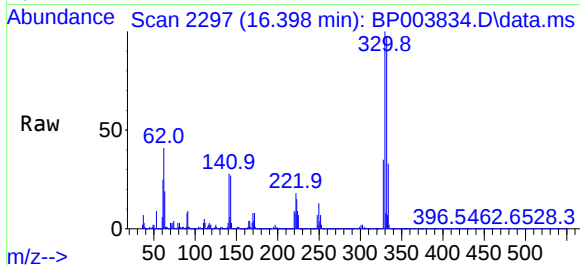

#45
2-Fluorobiphenyl
Concen: 81.12 ng
RT: 13.545 min Scan# 1812
Delta R.T. -0.000 min
Lab File: BP003834.D
Acq: 06 Nov 2020 10:46

Tgt Ion:172 Resp: 2505994
Ion Ratio Lower Upper
172 100
171 34.9 28.5 42.7
170 22.8 19.2 28.8


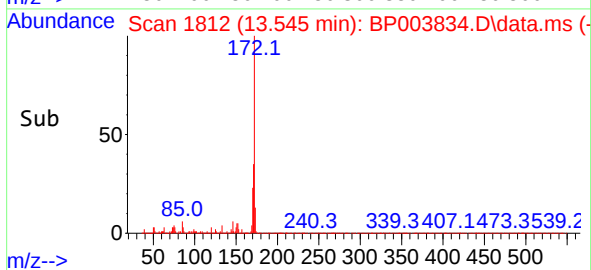
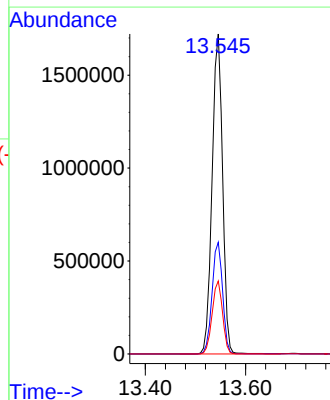
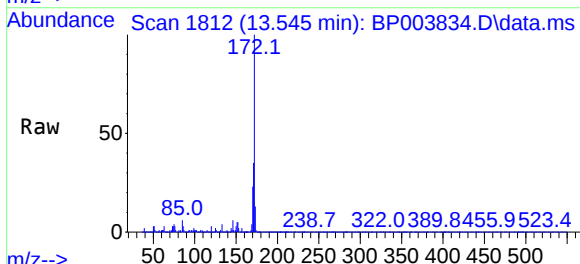


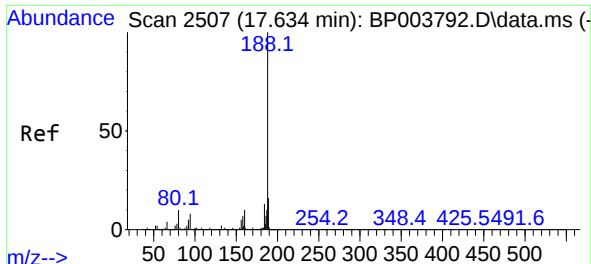

#64
Phenanthrene-d10
Concen: 20.00 ng
RT: 17.645 min Scan# 2509
Delta R.T. -0.000 min
Lab File: BP003834.D
Acq: 06 Nov 2020 10:46




Instrument :
BNA_P
ClientSampleId :
PB132804BL


Tgt Ion:188 Resp: 868277
Ion Ratio Lower Upper
188 100
94 8.3 6.2 9.2
80 9.6 6.2 9.2#

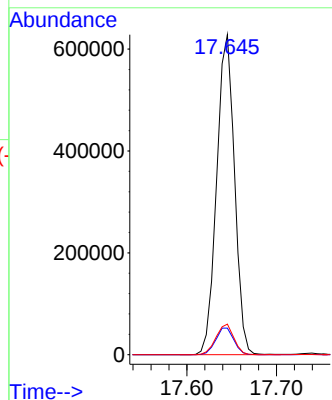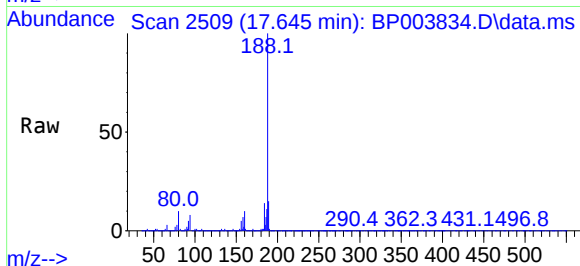

#76
Chrysene-d12
Concen: 20.00 ng
RT: 21.663 min Scan# 3192
Delta R.T. -0.006 min
Lab File: BP003834.D
Acq: 06 Nov 2020 10:46

Tgt Ion:240 Resp: 702428
Ion Ratio Lower Upper
240 100
120 8.7 7.8 11.6
236 24.8 20.8 31.2


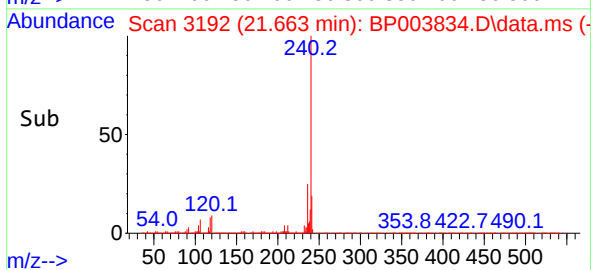
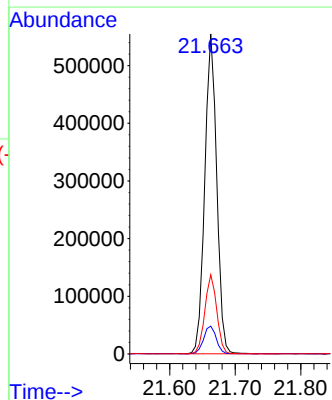
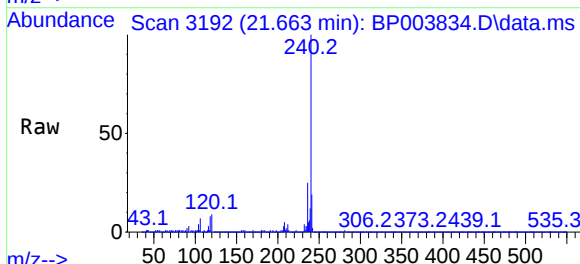




#79
Terphenyl-d14
Concen: 83.36 ng
RT: 20.133 min Scan# 2932
Delta R.T. -0.000 min
Lab File: BP003834.D
Acq: 06 Nov 2020 10:46

Instrument :
BNA_P
ClientSampleId :
PB132804BL

Tgt Ion:244 Resp: 3030884
Ion Ratio Lower Upper
244 100
212 7.0 5.8 8.6
122 9.2 7.8 11.8

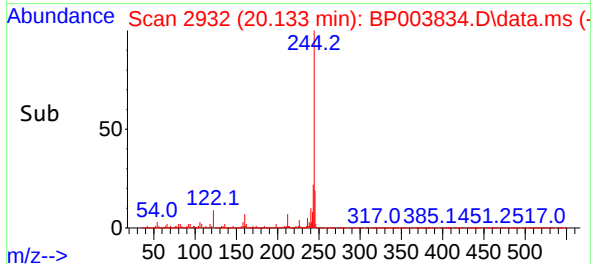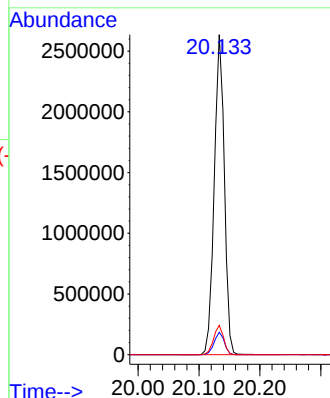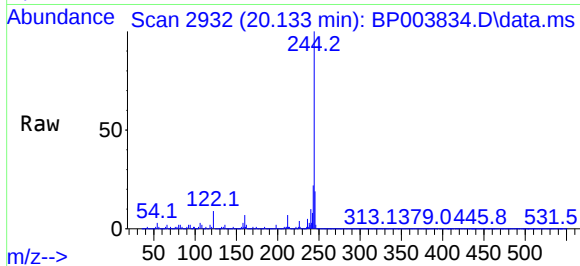

#86
Perylene-d12
Concen: 20.00 ng
RT: 24.139 min Scan# 3613
Delta R.T. -0.006 min
Lab File: BP003834.D
Acq: 06 Nov 2020 10:46

Tgt Ion:264 Resp: 702317
Ion Ratio Lower Upper
264 100
260 23.2 18.8 28.2
265 21.9 17.4 26.2

