

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110620\
 Data File : BP003836.D
 Acq On : 06 Nov 2020 12:30
 Operator : CG/JU
 Sample : L4521-04DL 5X
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 B-3DL

Manual Integrations
 APPROVED

mohammad
 11/10/2020 11:59:11 AM

Quant Time: Nov 06 13:27:35 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP110320.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Nov 06 11:33:14 2020
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.305	152	176873	20.00	ng	0.00
21) Naphthalene-d8	11.134	136	708828	20.00	ng	# 0.00
39) Acenaphthene-d10	14.916	164	438687	20.00	ng	0.00
64) Phenanthrene-d10	17.645	188	906883	20.00	ng	0.00
76) Chrysene-d12	21.669	240	818144	20.00	ng	0.00
86) Perylene-d12	24.145	264	843797	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.822	112	189443	17.88	ng	0.00
7) Phenol-d6	7.463	99	248802	16.35	ng	0.00
23) Nitrobenzene-d5	9.463	82	157464	10.88	ng	0.00
42) 2,4,6-Tribromophenol	16.392	330	92557	16.87	ng	0.00
45) 2-Fluorobiphenyl	13.540	172	343699	10.95	ng	0.00
79) Terphenyl-d14	20.133	244	416607	9.84	ng	0.00
Target Compounds						Qvalue
71) Phenanthrene	17.686	178	843882	16.58	ng	99
72) Anthracene	17.775	178	154101	3.13	ng	98
73) Carbazole	18.028	167	117327	2.57	ng	98
75) Fluoranthene	19.616	202	1885025	32.10	ng	99
78) Pyrene	19.963	202	1571147	28.30	ng	98
81) Benzo(a)anthracene	21.651	228	738584	13.69	ng	98
83) Chrysene	21.704	228	775302	14.96	ng	96
87) Indeno(1,2,3-cd)pyrene	26.692	276	511382	8.40	ng	# 94
88) Benzo(b)fluoranthene	23.392	252	1017582m	18.43	ng	
89) Benzo(k)fluoranthene	23.433	252	357383m	6.55	ng	
90) Benzo(a)pyrene	24.033	252	692867	13.55	ng	98
91) Dibenzo(a,h)anthracene	26.686	278	125400m	2.47	ng	
92) Benzo(g,h,i)perylene	27.480	276	511513	10.42	ng	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110620\
Data File : BP003836.D
Acq On : 06 Nov 2020 12:30
Operator : CG/JU
Sample : L4521-04DL 5X
Misc :
ALS Vial : 5 Sample Multiplier: 1


Instrument :
BNA_P
ClientSampled :
B-3DL

Manual Integrations
APPROVED

mohammad
11/10/2020 11:59:11 AM

Quant Time: Nov 06 13:27:35 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP110320.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 06 11:33:14 2020
Response via : Initial Calibration

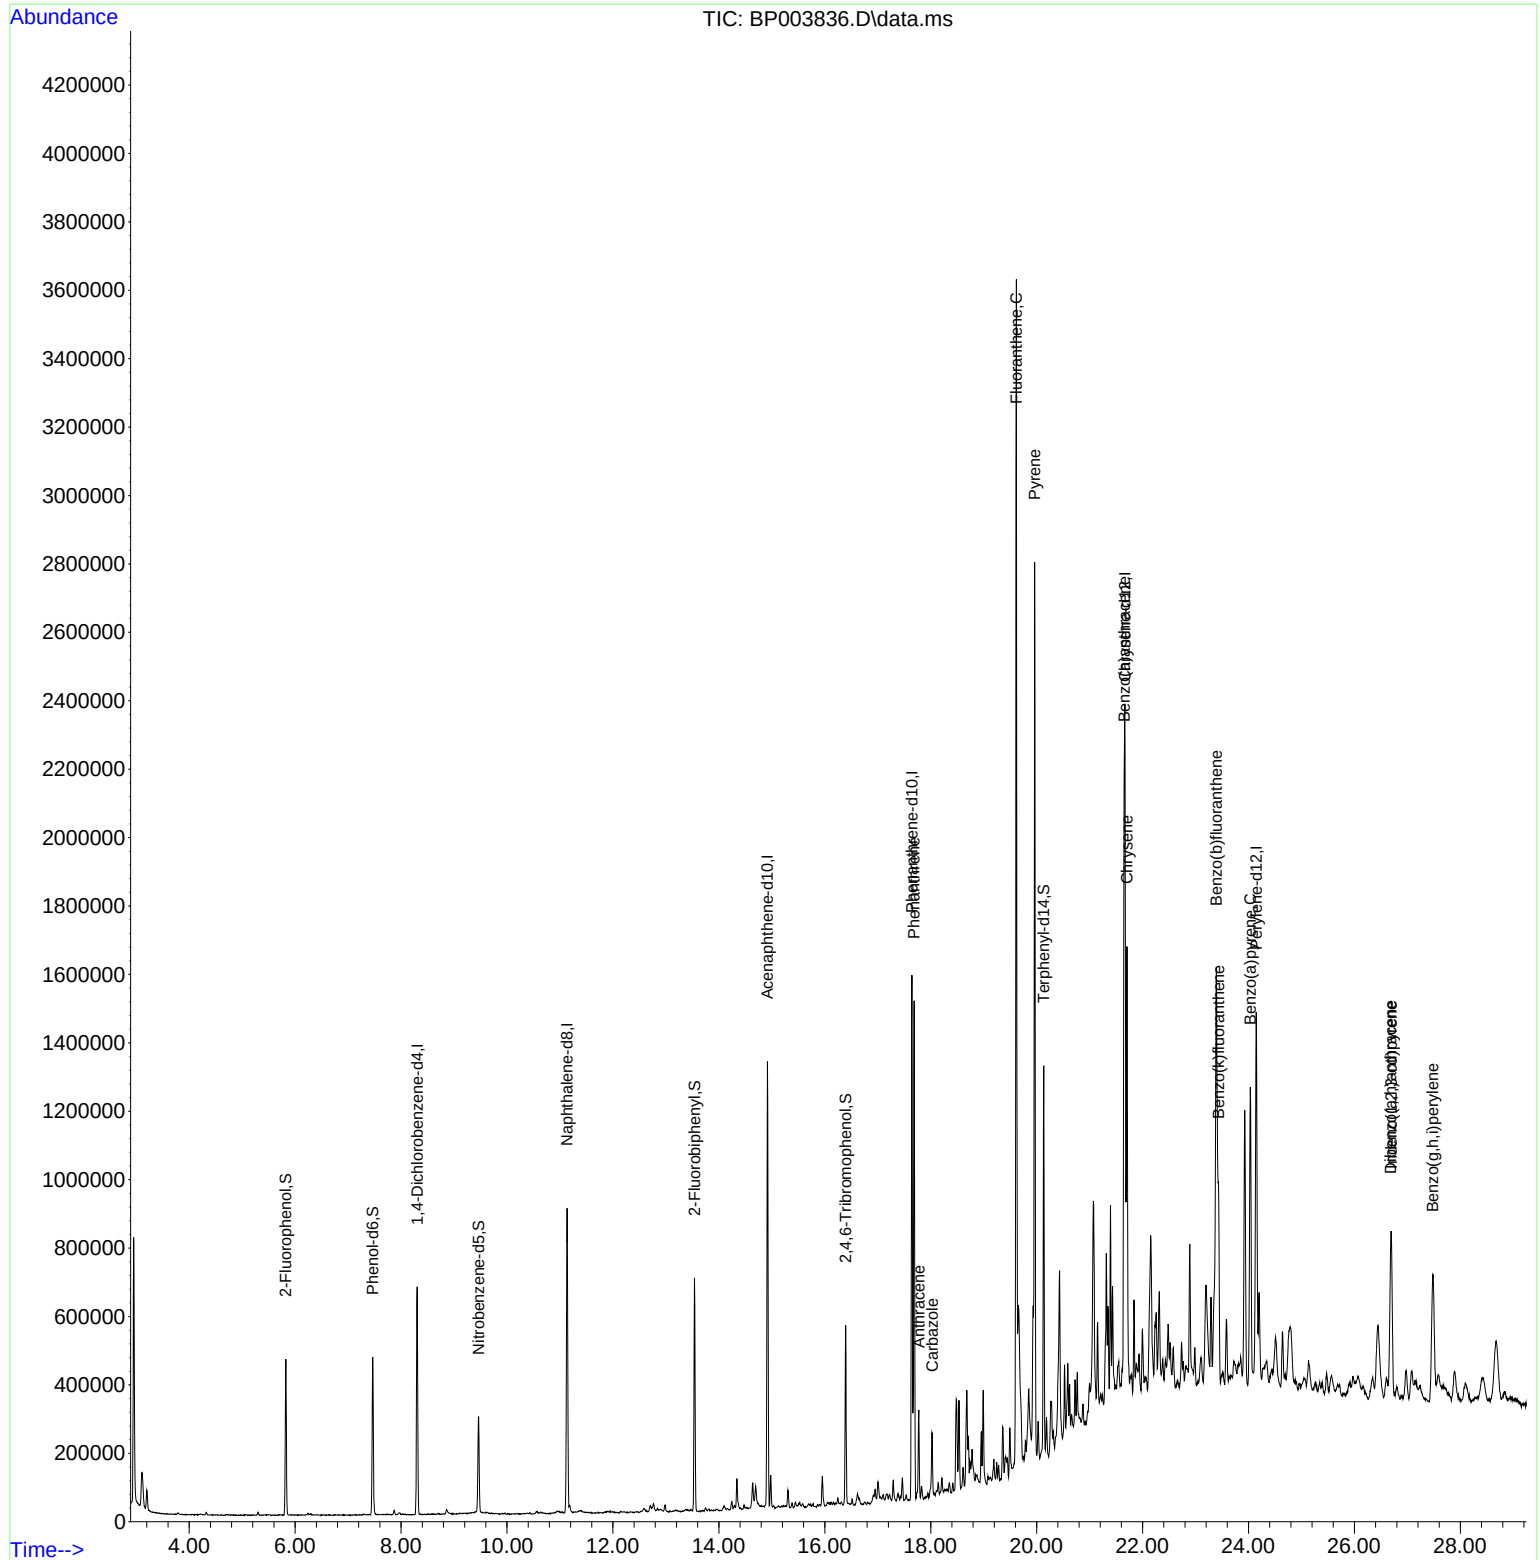







#1
1,4-Dichlorobenzene-d4
Concen: 20.00 ng
RT: 8.305 min Scan# 921
Delta R.T. -0.000 min
Lab File: BP003836.D
Acq: 06 Nov 2020 12:30

Tgt Ion:152 Resp: 176873
Ion Ratio Lower Upper
152 100
150 158.6 123.8 185.6
115 60.5 43.8 65.6

Instrument :
BNA_P
ClientSampleId :
B-3DL




Manual Integrations
APPROVED


mohammad
11/10/2020 11:59:11 AM



#5
2-Fluorophenol
Concen: 17.88 ng
RT: 5.822 min Scan# 499
Delta R.T. -0.000 min
Lab File: BP003836.D
Acq: 06 Nov 2020 12:30


Tgt Ion:112 Resp: 189443
Ion Ratio Lower Upper
112 100
64 65.0 32.8 49.2#
63 32.5 17.0 25.4#

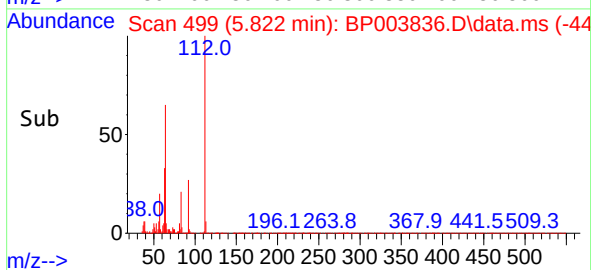



#7
Phenol-d6
Concen: 16.35 ng
RT: 7.463 min Scan# 778
Delta R.T. -0.006 min
Lab File: BP003836.D
Acq: 06 Nov 2020 12:30




Instrument :
BNA_P
ClientSampled :
B-3DL




Tgt Ion: 99 Resp: 248802
Ion Ratio Lower Upper
99 100
42 19.3 8.6 13.0#
71 34.9 23.4 35.2

Manual Integrations
APPROVED



mohammad
11/10/2020 11:59:11 AM

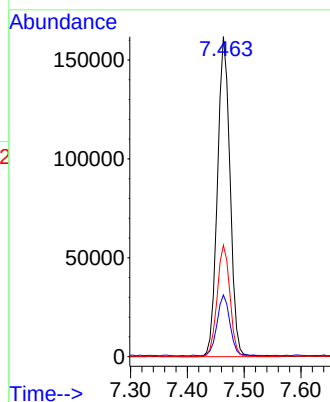


#21
Naphthalene-d8
Concen: 20.00 ng
RT: 11.134 min Scan# 1402
Delta R.T. -0.000 min
Lab File: BP003836.D
Acq: 06 Nov 2020 12:30



Tgt Ion: 136 Resp: 708828
Ion Ratio Lower Upper
136 100
137 10.9 8.6 13.0
54 9.2 3.6 5.4#
68 5.9 3.3 4.9#

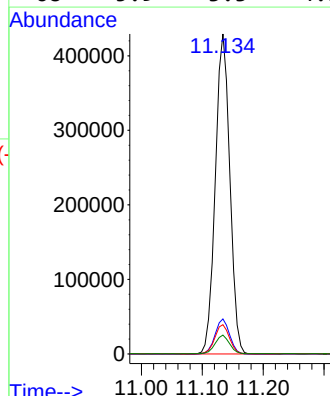







#23
Nitrobenzene-d5
Concen: 10.88 ng
RT: 9.463 min Scan# 1118
Delta R.T. -0.006 min
Lab File: BP003836.D
Acq: 06 Nov 2020 12:30

Tgt Ion: 82 Resp: 157464
Ion Ratio Lower Upper
82 100
128 41.2 45.6 68.4#
54 50.5 30.1 45.1#

Instrument :
BNA_P
ClientSampled :
B-3DL




Manual Integrations
APPROVED


mohammad
11/10/2020 11:59:11 AM



#39
Acenaphthene-d10
Concen: 20.00 ng
RT: 14.916 min Scan# 2045
Delta R.T. -0.000 min
Lab File: BP003836.D
Acq: 06 Nov 2020 12:30

Tgt Ion: 164 Resp: 438687
Ion Ratio Lower Upper
164 100
162 98.7 79.4 119.2
160 42.8 36.1 54.1









#42
2,4,6-Tribromophenol
Concen: 16.87 ng
RT: 16.392 min Scan# 2296
Delta R.T. -0.006 min
Lab File: BP003836.D
Acq: 06 Nov 2020 12:30

Tgt Ion:	330	Resp:	92557
Ion Ratio	Lower	Upper	
330	100		
332	96.9	77.1	115.7
141	31.8	23.4	35.2

Instrument :
BNA_P
ClientSampled :
B-3DL




Manual Integrations
APPROVED


mohammad
11/10/2020 11:59:11 AM

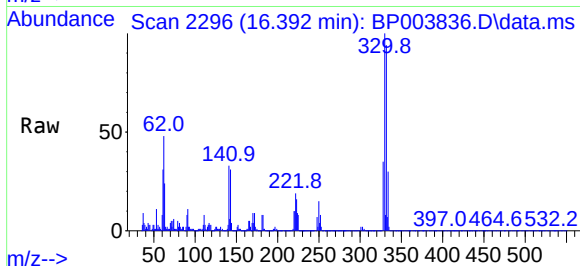

#45
2-Fluorobiphenyl
Concen: 10.95 ng
RT: 13.540 min Scan# 1811
Delta R.T. -0.006 min
Lab File: BP003836.D
Acq: 06 Nov 2020 12:30


Tgt Ion:	172	Resp:	343699
Ion Ratio	Lower	Upper	
172	100		
171	34.5	28.5	42.7
170	22.0	19.2	28.8

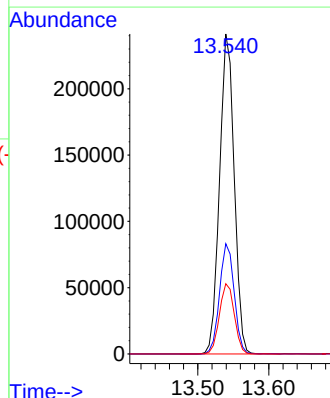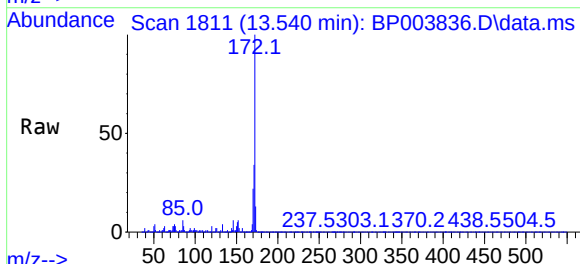



#64
Phenanthrene-d10
Concen: 20.00 ng
RT: 17.645 min Scan# 2509
Delta R.T. -0.000 min
Lab File: BP003836.D
Acq: 06 Nov 2020 12:30




Instrument :
BNA_P
ClientSampled :
B-3DL

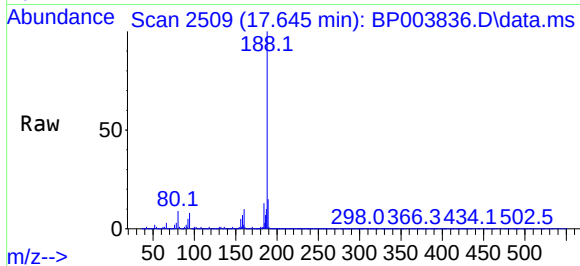


Tgt Ion:188 Resp: 906883
Ion Ratio Lower Upper
188 100
94 8.0 6.2 9.2
80 9.2 6.2 9.2

Manual Integrations
APPROVED



mohammad
11/10/2020 11:59:11 AM




#71
Phenanthrene
Concen: 16.58 ng
RT: 17.686 min Scan# 2516
Delta R.T. -0.000 min
Lab File: BP003836.D
Acq: 06 Nov 2020 12:30

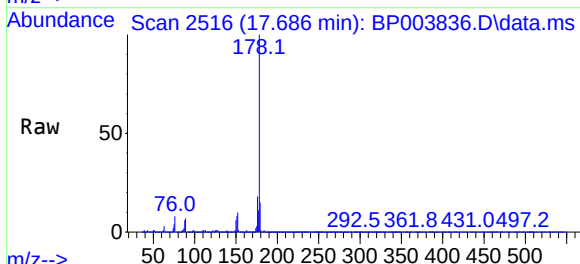


Tgt Ion:178 Resp: 843882
Ion Ratio Lower Upper
178 100
176 18.1 15.3 22.9
179 15.4 12.5 18.7

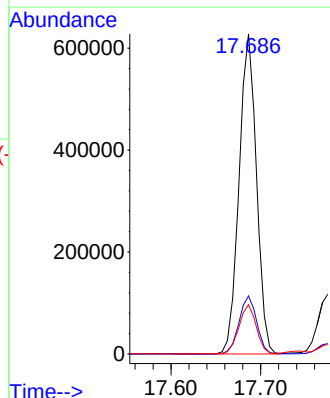



#72
 Anthracene
 Concen: 3.13 ng
 RT: 17.775 min Scan# 2531
 Delta R.T. -0.000 min
 Lab File: BP003836.D
 Acq: 06 Nov 2020 12:30




Instrument :
 BNA_P
 ClientSampled :
 B-3DL



Tgt Ion:178 Resp: 154101
 Ion Ratio Lower Upper
 178 100
 176 17.6 15.0 22.4
 179 15.9 12.5 18.7




Manual Integrations
 APPROVED


mohammad
 11/10/2020 11:59:11 AM

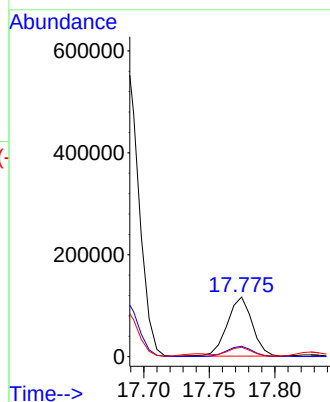

#73
 Carbazole
 Concen: 2.57 ng
 RT: 18.028 min Scan# 2574
 Delta R.T. -0.000 min
 Lab File: BP003836.D
 Acq: 06 Nov 2020 12:30


Tgt Ion:167 Resp: 117327
 Ion Ratio Lower Upper
 167 100
 166 20.9 17.6 26.4
 139 12.2 10.2 15.4

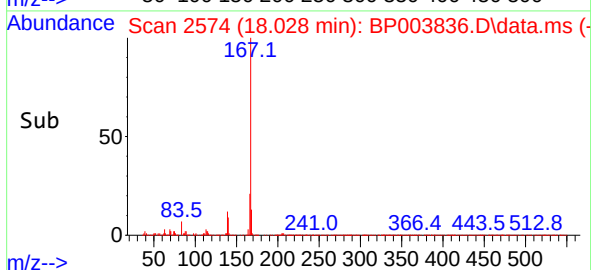



#75
Fluoranthene
Concen: 32.10 ng
RT: 19.616 min Scan# 2844
Delta R.T. -0.000 min
Lab File: BP003836.D
Acq: 06 Nov 2020 12:30




Instrument :
BNA_P
ClientSampled :
B-3DL



Tgt Ion:202 Resp: 1885025
Ion Ratio Lower Upper
202 100
101 9.6 0.0 29.4
203 17.6 0.0 37.8




Manual Integrations
APPROVED


mohammad
11/10/2020 11:59:11 AM

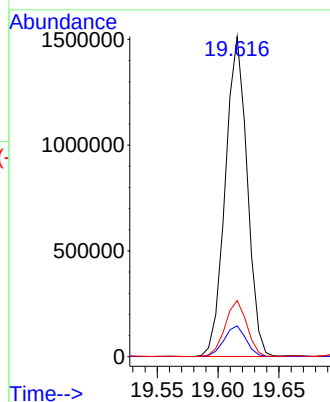

#76
Chrysene-d12
Concen: 20.00 ng
RT: 21.669 min Scan# 3193
Delta R.T. -0.000 min
Lab File: BP003836.D
Acq: 06 Nov 2020 12:30


Tgt Ion:240 Resp: 818144
Ion Ratio Lower Upper
240 100
120 8.8 7.8 11.6
236 25.1 20.8 31.2

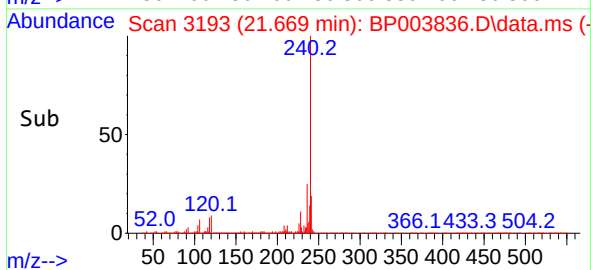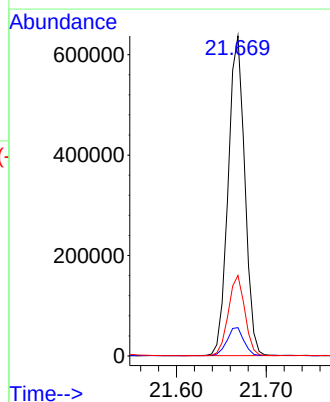



#78
Pyrene
Concen: 28.30 ng
RT: 19.963 min Scan# 2903
Delta R.T. -0.000 min
Lab File: BP003836.D
Acq: 06 Nov 2020 12:30




Instrument :
BNA_P
ClientSampled :
B-3DL




Tgt Ion:202 Resp: 1571147
Ion Ratio Lower Upper
202 100
200 20.1 17.1 25.7
203 17.6 14.2 21.2

Manual Integrations
APPROVED



mohammad
11/10/2020 11:59:11 AM




#79
Terphenyl-d14
Concen: 9.84 ng
RT: 20.133 min Scan# 2932
Delta R.T. -0.000 min
Lab File: BP003836.D
Acq: 06 Nov 2020 12:30




Tgt Ion:244 Resp: 416607
Ion Ratio Lower Upper
244 100
212 6.9 5.8 8.6
122 8.5 7.8 11.8

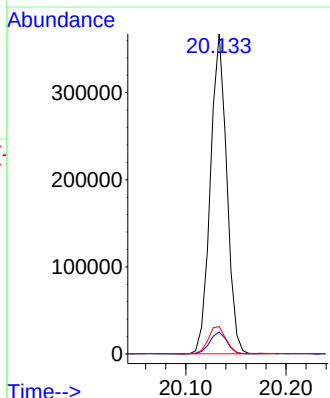



#81
Benzo(a)anthracene
Concen: 13.69 ng
RT: 21.651 min Scan# 3190
Delta R.T. -0.000 min
Lab File: BP003836.D
Acq: 06 Nov 2020 12:30




Instrument :
BNA_P
ClientSampleId :
B-3DL



Tgt Ion:228 Resp: 738584
Ion Ratio Lower Upper
228 100
226 26.1 22.1 33.1
229 20.5 15.9 23.9




Manual Integrations
APPROVED


mohammad
11/10/2020 11:59:11 AM

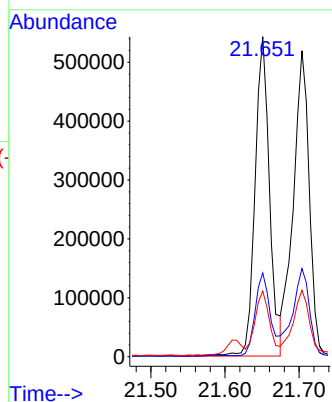

#83
Chrysene
Concen: 14.96 ng
RT: 21.704 min Scan# 3199
Delta R.T. -0.000 min
Lab File: BP003836.D
Acq: 06 Nov 2020 12:30


Tgt Ion:228 Resp: 775302
Ion Ratio Lower Upper
228 100
226 28.8 24.4 36.6
229 21.7 15.8 23.6

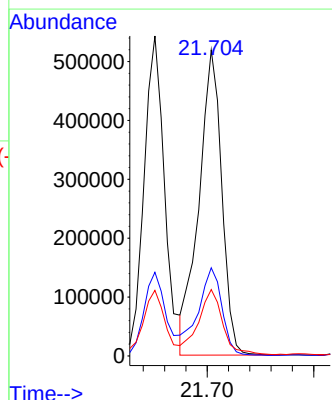



#86
Perylene-d12
Concen: 20.00 ng
RT: 24.145 min Scan# 3614
Delta R.T. -0.000 min
Lab File: BP003836.D
Acq: 06 Nov 2020 12:30




Instrument :
BNA_P
ClientSampled :
B-3DL




Tgt Ion:264 Resp: 843797
Ion Ratio Lower Upper
264 100
260 22.8 18.8 28.2
265 21.5 17.4 26.2

Manual Integrations
APPROVED



mohammad
11/10/2020 11:59:11 AM




#87
Indeno(1,2,3-cd)pyrene
Concen: 8.40 ng
RT: 26.692 min Scan# 4047
Delta R.T. -0.012 min
Lab File: BP003836.D
Acq: 06 Nov 2020 12:30




Tgt Ion:276 Resp: 511382
Ion Ratio Lower Upper
276 100
138 18.6 18.7 28.1#
277 24.5 20.4 30.6

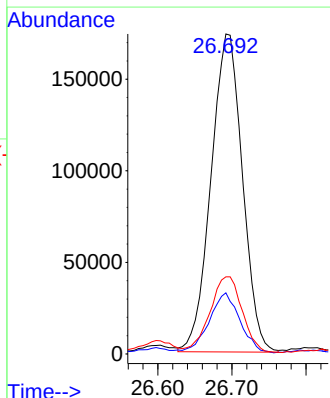

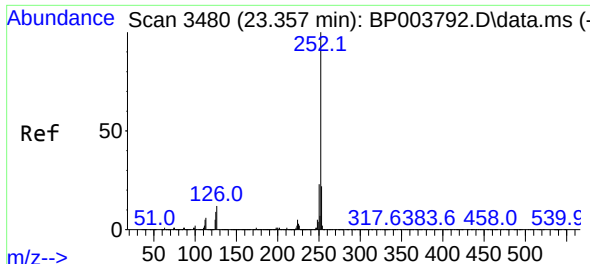

#88
Benzo(b)fluoranthene
Concen: 18.43 ng m
RT: 23.392 min Scan# 3486
Delta R.T. -0.000 min
Lab File: BP003836.D
Acq: 06 Nov 2020 12:30




Instrument :
BNA_P
ClientSampled :
B-3DL

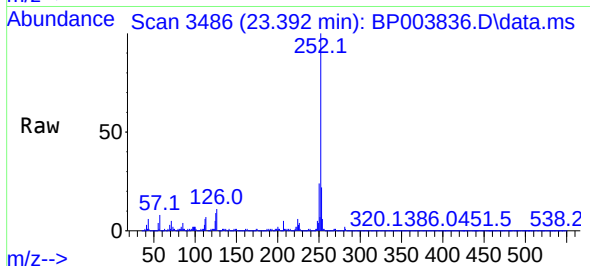


Tgt Ion:252 Resp: 1017582
Ion Ratio Lower Upper
252 100
253 22.3 17.6 26.4
125 9.0 7.3 10.9

Manual Integrations
APPROVED



mohammad
11/10/2020 11:59:11 AM

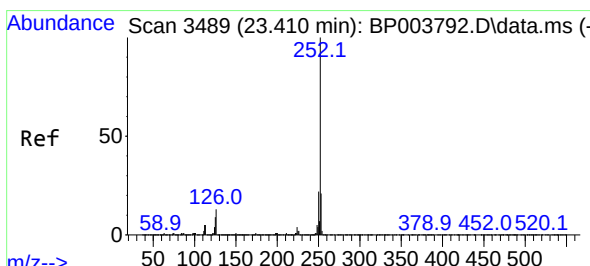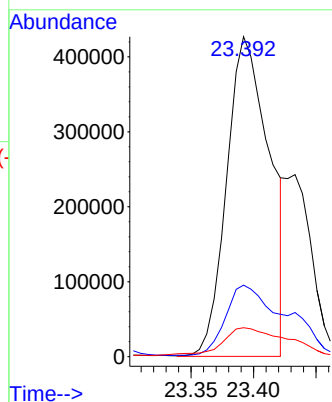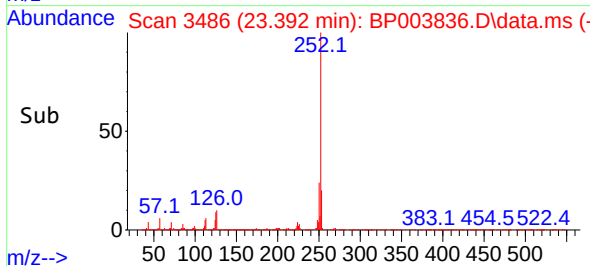


#89
Benzo(k)fluoranthene
Concen: 6.55 ng m
RT: 23.433 min Scan# 3493
Delta R.T. -0.006 min
Lab File: BP003836.D
Acq: 06 Nov 2020 12:30

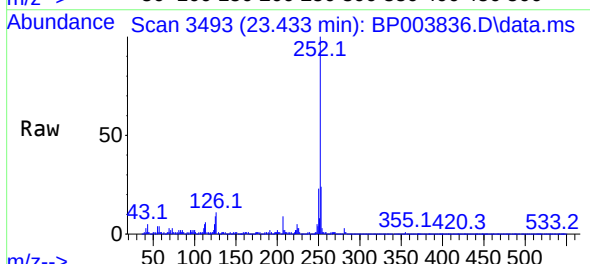

Tgt Ion:252 Resp: 357383
Ion Ratio Lower Upper
252 100
253 24.3 17.8 26.8
125 9.4 7.4 11.2

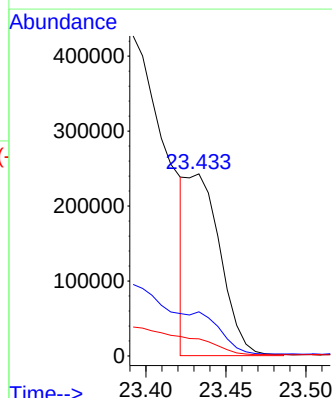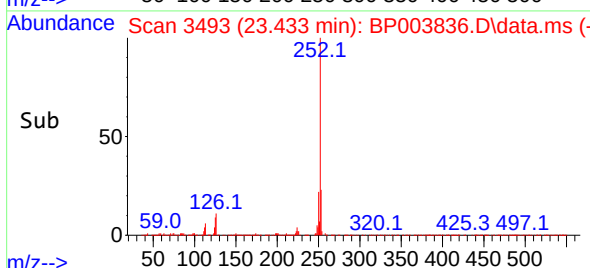







#90
Benzo(a)pyrene
Concen: 13.55 ng
RT: 24.033 min Scan# 3595
Delta R.T. -0.000 min
Lab File: BP003836.D
Acq: 06 Nov 2020 12:30

Tgt Ion:	252	Resp:	692867
Ion Ratio	Lower	Upper	
252	100		
253	22.4	17.4	26.0
125	9.3	8.2	12.4

Instrument :
BNA_P
ClientSampled :
B-3DL




Manual Integrations
APPROVED


mohammad
11/10/2020 11:59:11 AM



#91
Dibenzo(a,h)anthracene
Concen: 2.47 ng m
RT: 26.686 min Scan# 4046
Delta R.T. -0.018 min
Lab File: BP003836.D
Acq: 06 Nov 2020 12:30


Tgt Ion:	278	Resp:	125400
Ion Ratio	Lower	Upper	
278	100		
139	19.5	12.4	18.6#
279	23.0	19.0	28.6

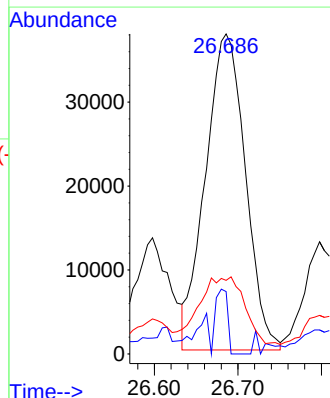



#92
Benzo(g,h,i)perylene
Concen: 10.42 ng
RT: 27.480 min Scan# 4181
Delta R.T. -0.012 min
Lab File: BP003836.D
Acq: 06 Nov 2020 12:30

Instrument :
BNA_P
ClientSampled :
B-3DL



Tgt Ion:276 Resp: 511513
Ion Ratio Lower Upper
276 100
277 24.0 19.0 28.6
138 18.6 16.6 24.8

Manual Integrations
APPROVED

mohammad
11/10/2020 11:59:11 AM

