
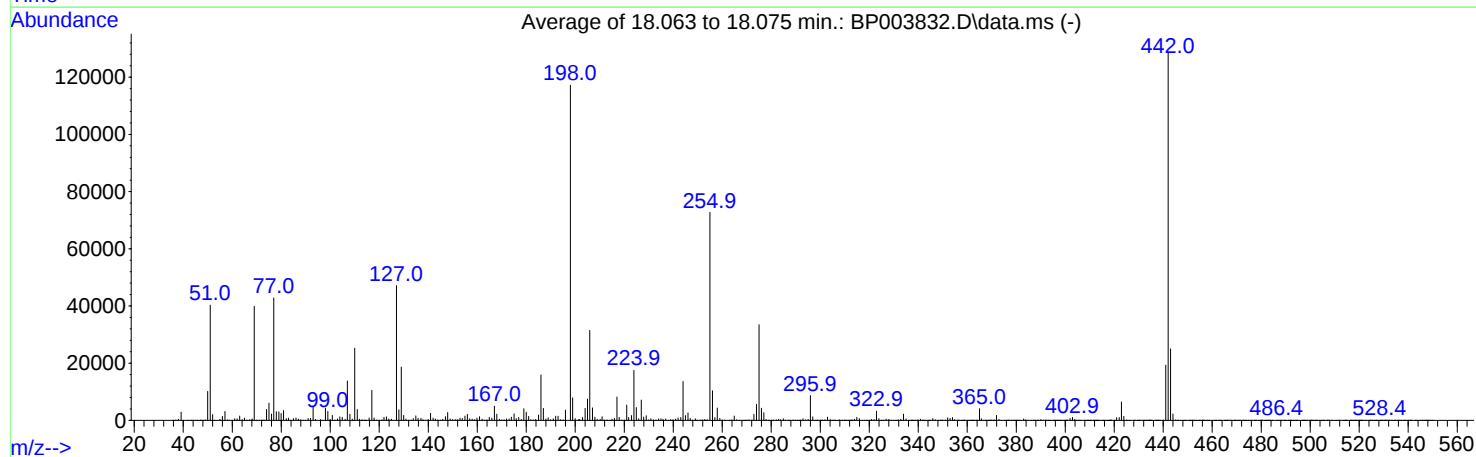


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110620\
 Data File : BP003832.D
 Acq On : 06 Nov 2020 09:38
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP110320.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Nov 06 11:33:14 2020

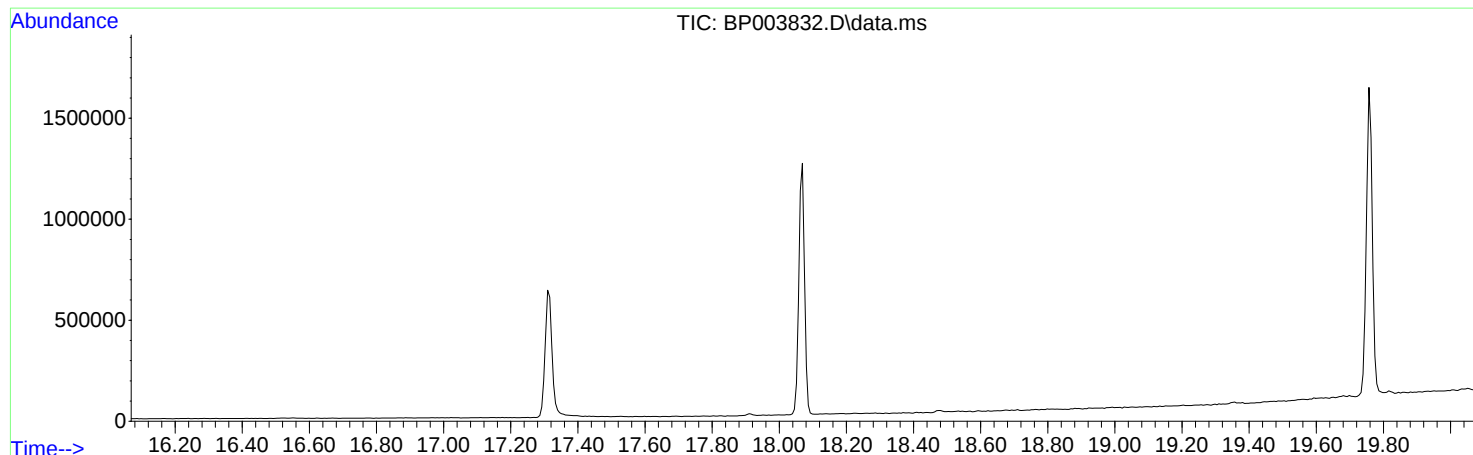

AutoFind: Scans 2580, 2581, 2582; Background Corrected with Scan 2569

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	34.4	40302	PASS
68	69	0.00	2	1.3	522	PASS
69	198	0.00	100	34.0	39864	PASS
70	69	0.00	2	0.2	96	PASS
127	198	10	80	40.2	47097	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	117184	PASS
199	198	5	9	6.8	7911	PASS
275	198	10	60	28.5	33440	PASS
365	198	1	100	3.5	4091	PASS
441	198	0.01	100	16.5	19301	PASS
442	442	100	100	100.0	128624	PASS
443	442	15	24	19.5	25032	PASS