




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110722\
 Data File : BP012532.D
 Acq On : 07 Nov 2022 15:36
 Operator : CG/JU
 Sample : N5353-20
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DBXB3

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 11/08/2022
 Supervised By :mohammad ahmed 11/14/2022

Quant Time: Nov 07 21:41:20 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Nov 04 02:53:36 2022
 Response via : Initial Calibration

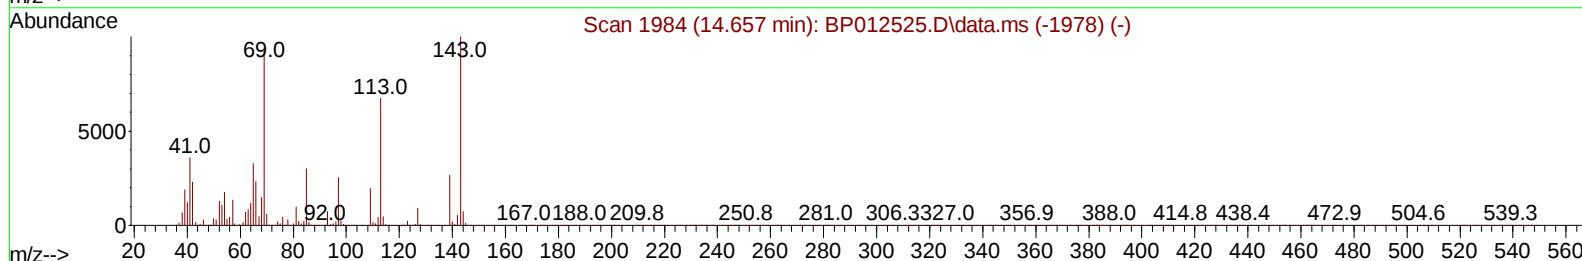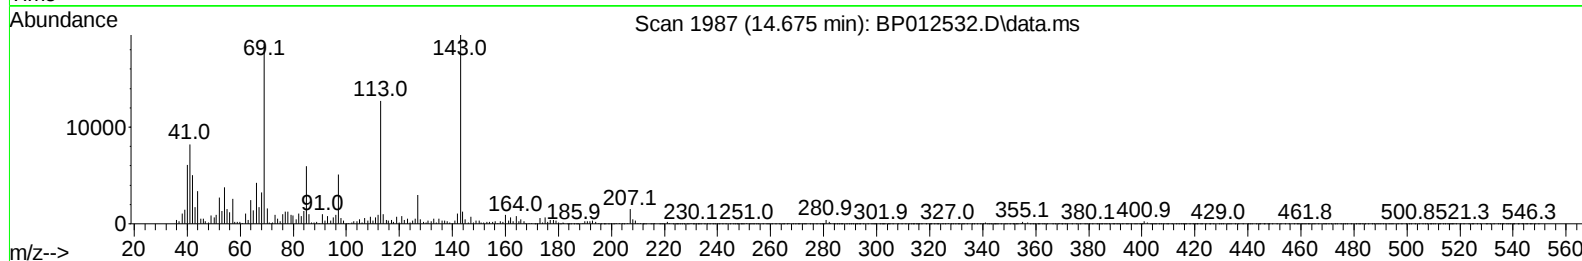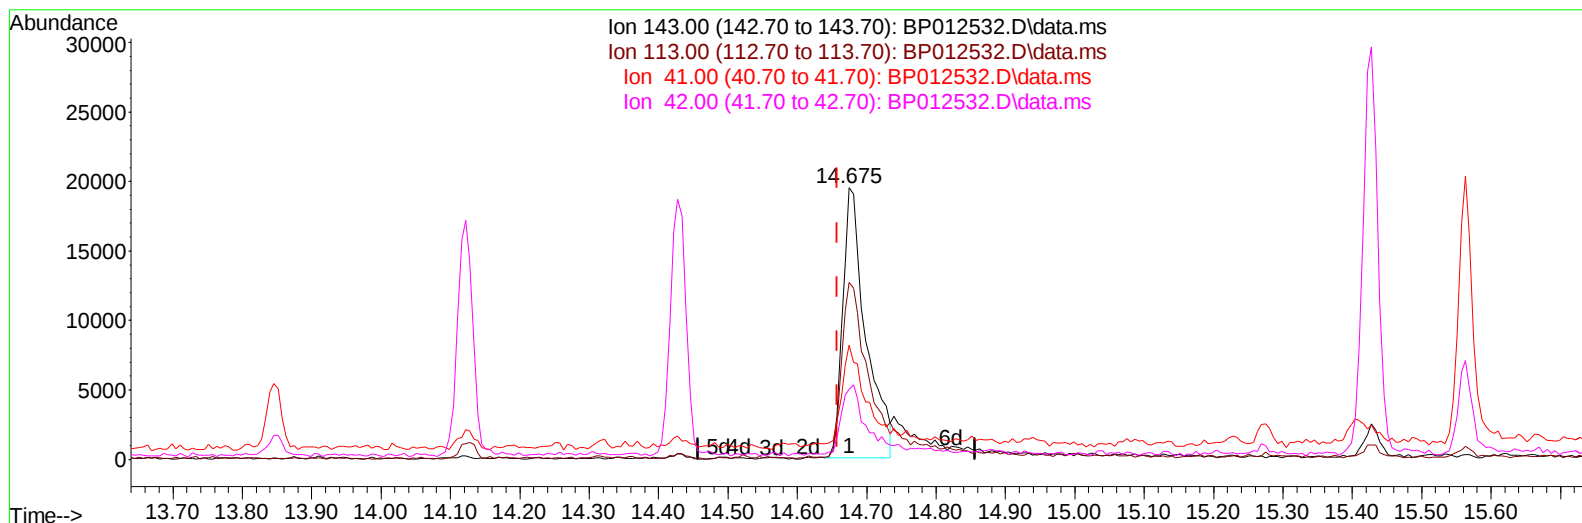

TIC: BP012532.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.675min (+ 0.018) 2.84 ng/u1

response 45064

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	65.10	65.20
41.00	34.50	42.09#
42.00	23.60	25.73




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110722\
 Data File : BP012532.D
 Acq On : 07 Nov 2022 15:36
 Operator : CG/JU
 Sample : N5353-20
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DBXB3

Manual IntegrationsAPPROVED

Quant Time: Nov 07 21:41:20 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Nov 04 02:53:36 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 11/08/2022
 Supervised By :mohammad ahmed 11/14/2022

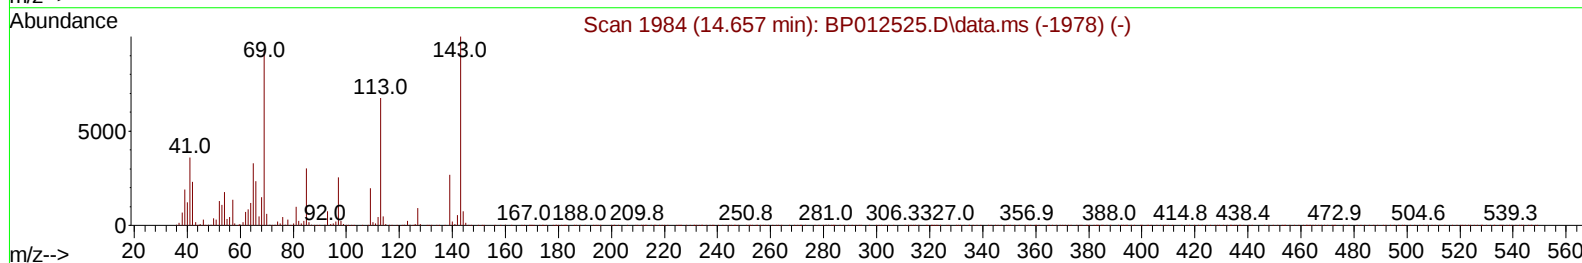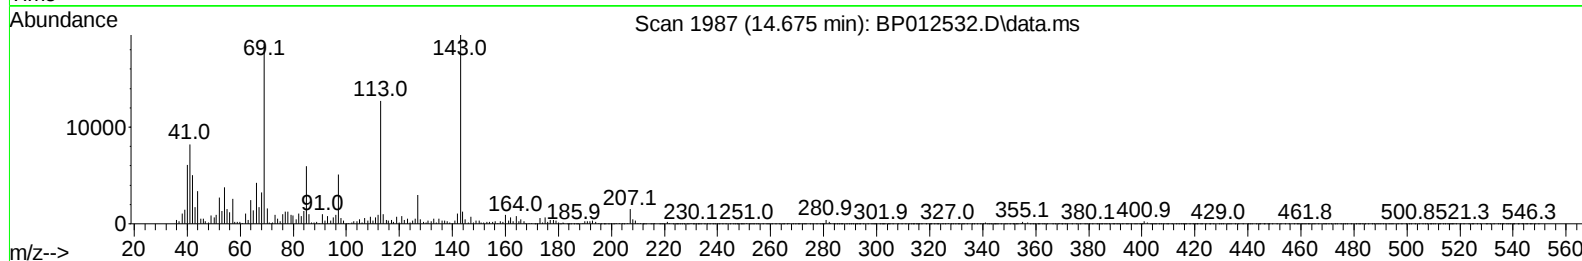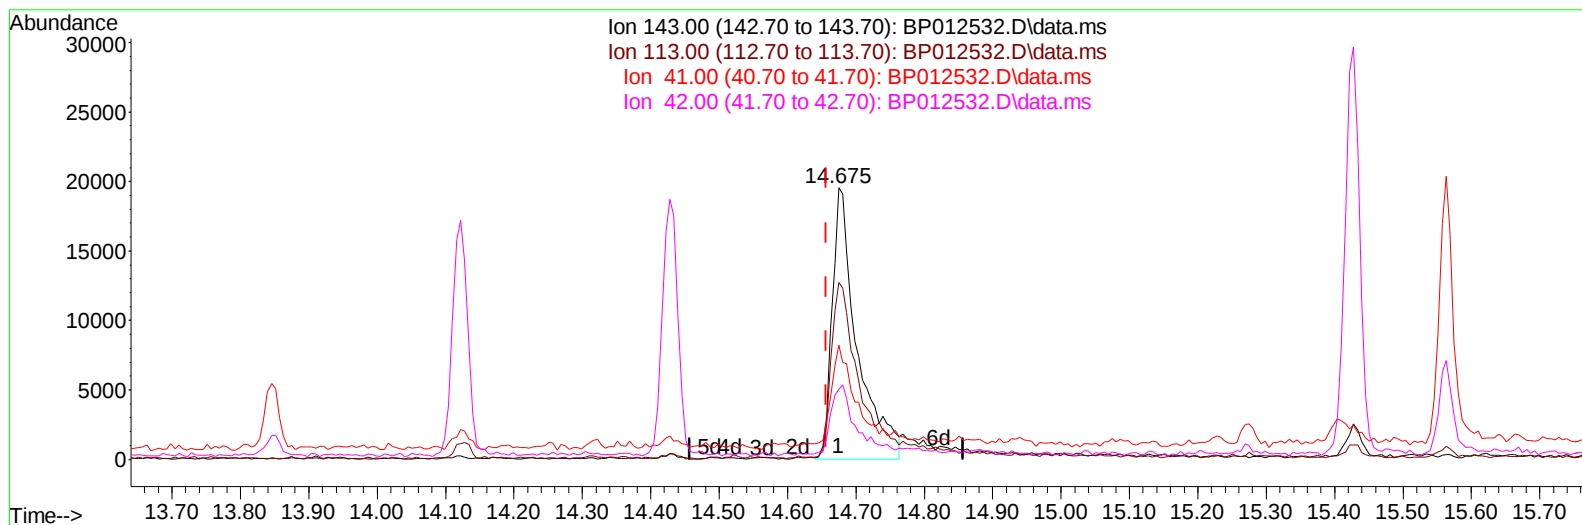

TIC: BP012532.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.675min (+ 0.018) 3.13 ng/ul m

response 49763

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	65.10	65.20
41.00	34.50	42.09#
42.00	23.60	25.73

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110722\
 Data File : BP012532.D
 Acq On : 07 Nov 2022 15:36
 Operator : CG/JU
 Sample : N5353-20
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DBXB3

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 11/08/2022
 Supervised By :mohammad ahmed 11/14/2022

Quant Time: Nov 07 21:41:20 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Nov 04 02:53:36 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.775	152	381676	20.000	ng/ul	0.00
20) Naphthalene-d8	10.575	136	1803591	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.428	164	1225763	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.192	188	2644691	20.000	ng/ul	0.00
79) Chrysene-d12	21.286	240	2207084	20.000	ng/ul	0.00
88) Perylene-d12	23.668	264	2035839	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.234	96	32698	3.449	ng/uL	0.00
4) Pyridine-d5	3.658	84	195153	7.167	ng/ul	0.00
7) Phenol-d5	6.958	99	168492	4.922	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.116	67	504223	24.673	ng/ul	0.00
11) 2-Chlorophenol-d4	7.311	132	493037	19.722	ng/ul	0.00
15) 4-Methylphenol-d8	8.499	113	339167	12.527	ng/ul	0.00
21) Nitrobenzene-d5	8.946	128	352288	30.121	ng/ul	0.00
24) 2-Nitrophenol-d4	9.669	143	360482	29.695	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.204	165	632520	24.042	ng/ul	0.00
31) 4-Chloroaniline-d4	10.728	131	871302	22.243	ng/ul	0.00
46) Dimethylphthalate-d6	13.845	166	2456214	29.272	ng/ul	0.00
49) Acenaphthylene-d8	14.122	160	2599438	27.108	ng/ul	0.00
54) 4-Nitrophenol-d4	14.675	143	49763m	3.134	ng/ul	0.02
60) Fluorene-d10	15.428	176	2107368	29.333	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.563	200	342286	24.858	ng/ul	0.00
73) Anthracene-d10	17.292	188	3486992	30.600	ng/ul	0.00
81) Pyrene-d10	19.533	212	3923563	35.408	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.516	264	3094147	31.105	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110722\
Data File : BP012532.D
Acq On : 07 Nov 2022 15:36
Operator : CG/JU
Sample : N5353-20
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DBXB3

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 11/08/2022
Supervised By :mohammad ahmed 11/14/2022

Quant Time: Nov 07 21:41:20 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Nov 04 02:53:36 2022
Response via : Initial Calibration

