




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110722\
 Data File : BP012533.D
 Acq On : 07 Nov 2022 16:11
 Operator : CG/JU
 Sample : N5353-12
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DBWV2

Manual IntegrationsAPPROVED

Quant Time: Nov 07 21:41:30 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Nov 04 02:53:36 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 11/08/2022
 Supervised By :mohammad ahmed 11/14/2022

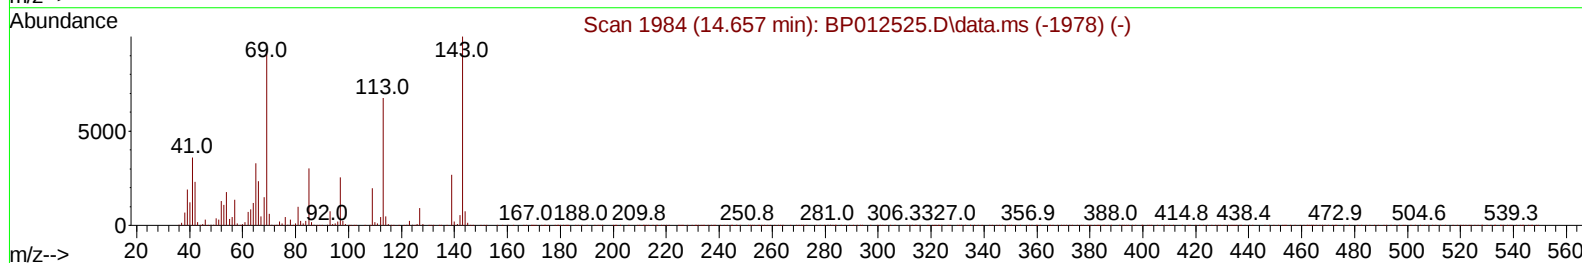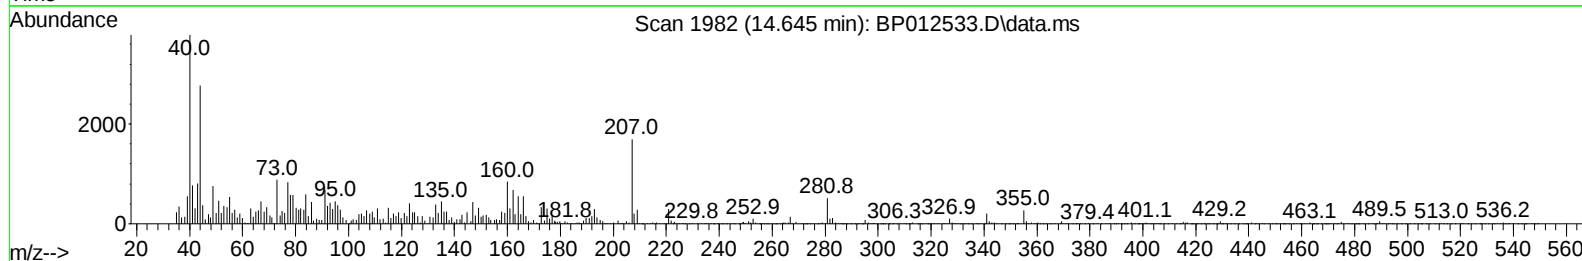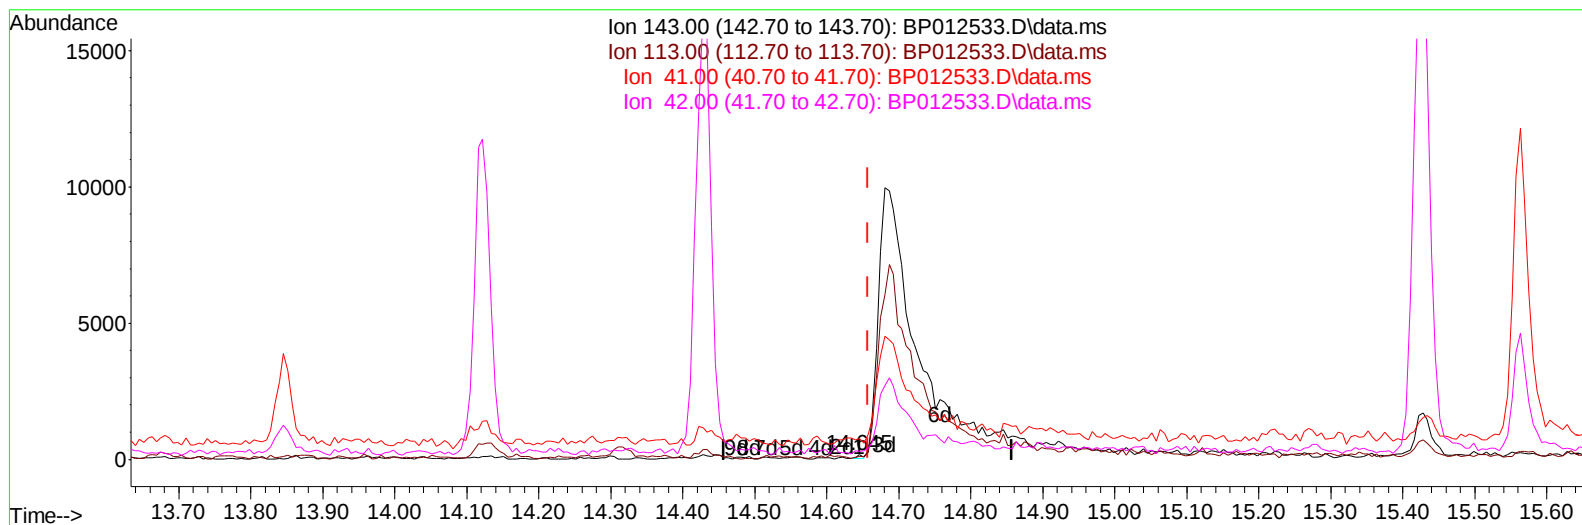

TIC: BP012533.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.645min (-0.012) 0.01 ng/u1

response 90

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	65.10	49.74#
41.00	34.50	395.90#
42.00	23.60	155.38#




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110722\
 Data File : BP012533.D
 Acq On : 07 Nov 2022 16:11
 Operator : CG/JU
 Sample : N5353-12
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DBWV2

Manual IntegrationsAPPROVED

Quant Time: Nov 07 21:41:30 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Nov 04 02:53:36 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 11/08/2022
 Supervised By :mohammad ahmed 11/14/2022

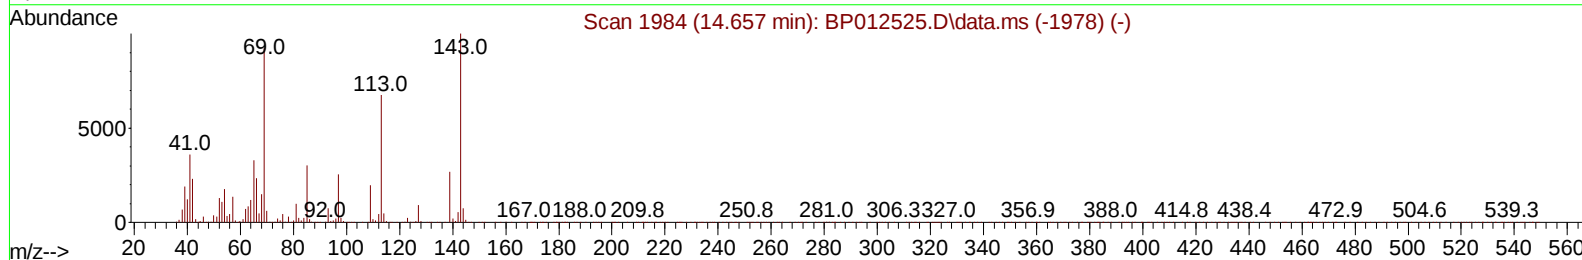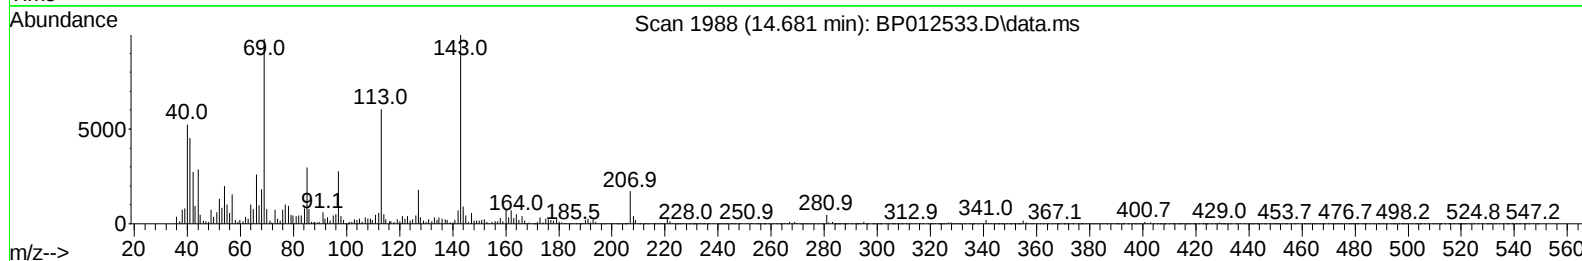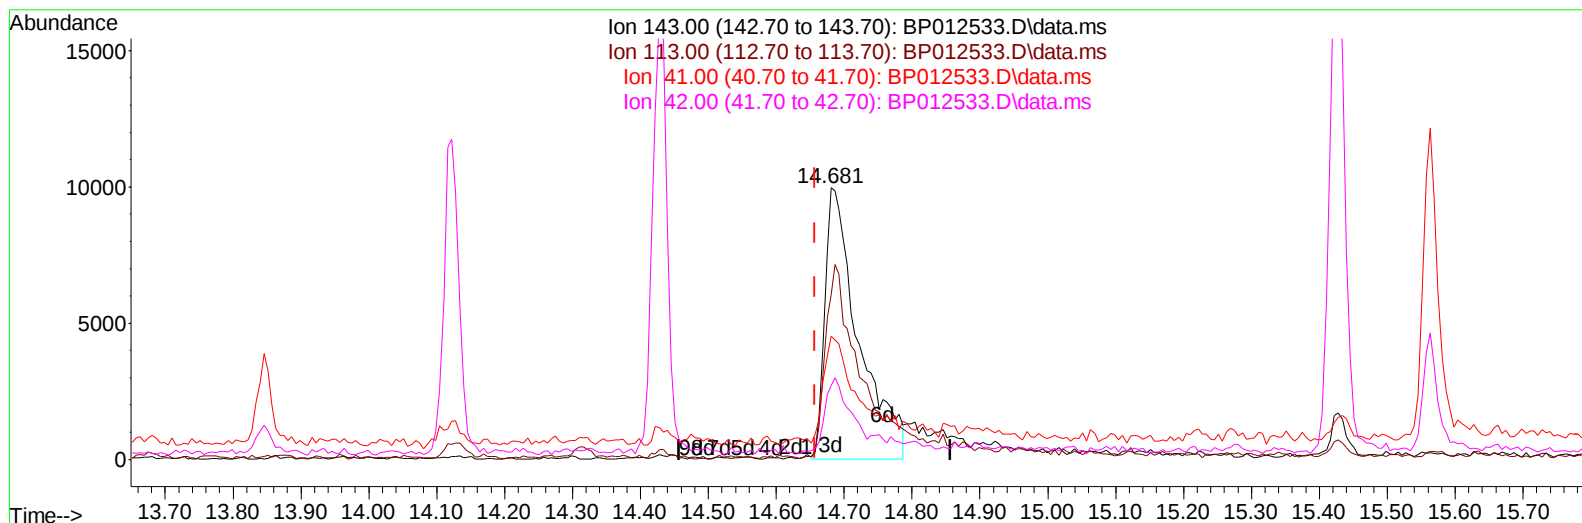

TIC: BP012533.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.681min (+ 0.024) 2.69 ng/ul m

response 34284

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	65.10	60.76
41.00	34.50	45.32#
42.00	23.60	27.33

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110722\
 Data File : BP012533.D
 Acq On : 07 Nov 2022 16:11
 Operator : CG/JU
 Sample : N5353-12
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DBVV2

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 11/08/2022
 Supervised By :mohammad ahmed 11/14/2022

Quant Time: Nov 07 21:41:30 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Nov 04 02:53:36 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.775	152	293399	20.000	ng/ul	0.00
20) Naphthalene-d8	10.575	136	1430194	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.428	164	982542	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.192	188	2211426	20.000	ng/ul	0.00
79) Chrysene-d12	21.286	240	2023999	20.000	ng/ul	0.00
88) Perylene-d12	23.669	264	1845129	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.228	96	27122	3.722	ng/uL	0.00
4) Pyridine-d5	3.664	84	109118	5.213	ng/ul	0.01
7) Phenol-d5	6.958	99	131811	5.009	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.116	67	347676	22.131	ng/ul	0.00
11) 2-Chlorophenol-d4	7.311	132	347572	18.086	ng/ul	0.00
15) 4-Methylphenol-d8	8.499	113	251054	12.062	ng/ul	0.00
21) Nitrobenzene-d5	8.952	128	236502	25.500	ng/ul	0.00
24) 2-Nitrophenol-d4	9.669	143	254100	26.396	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.205	165	447038	21.428	ng/ul	0.00
31) 4-Chloroaniline-d4	10.734	131	618708	19.918	ng/ul	0.00
46) Dimethylphthalate-d6	13.845	166	1642886	24.426	ng/ul	0.00
49) Acenaphthylene-d8	14.122	160	1807471	23.515	ng/ul	0.00
54) 4-Nitrophenol-d4	14.681	143	34284m	2.693	ng/ul	0.02
60) Fluorene-d10	15.428	176	1464244	25.427	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.563	200	216078	18.767	ng/ul	0.00
73) Anthracene-d10	17.292	188	2469833	25.920	ng/ul	0.00
81) Pyrene-d10	19.533	212	2842606	27.973	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.516	264	2299257	25.503	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110722\
Data File : BP012533.D
Acq On : 07 Nov 2022 16:11
Operator : CG/JU
Sample : N5353-12
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DBVV2

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 11/08/2022
Supervised By :mohammad ahmed 11/14/2022

Quant Time: Nov 07 21:41:30 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Nov 04 02:53:36 2022
Response via : Initial Calibration

