




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110722\
 Data File : BP012534.D
 Acq On : 07 Nov 2022 16:46
 Operator : CG/JU
 Sample : N5353-19
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DBXB2

Manual IntegrationsAPPROVED

Quant Time: Nov 07 21:41:40 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Nov 04 02:53:36 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 11/08/2022
 Supervised By :mohammad ahmed 11/14/2022

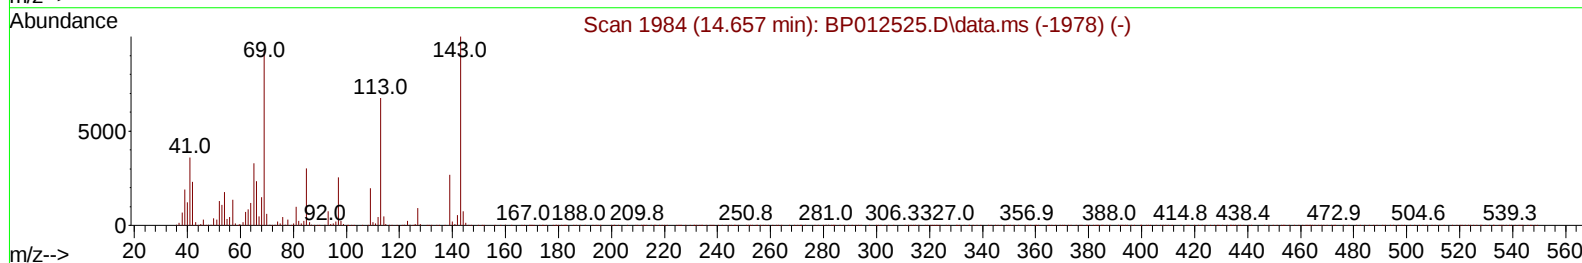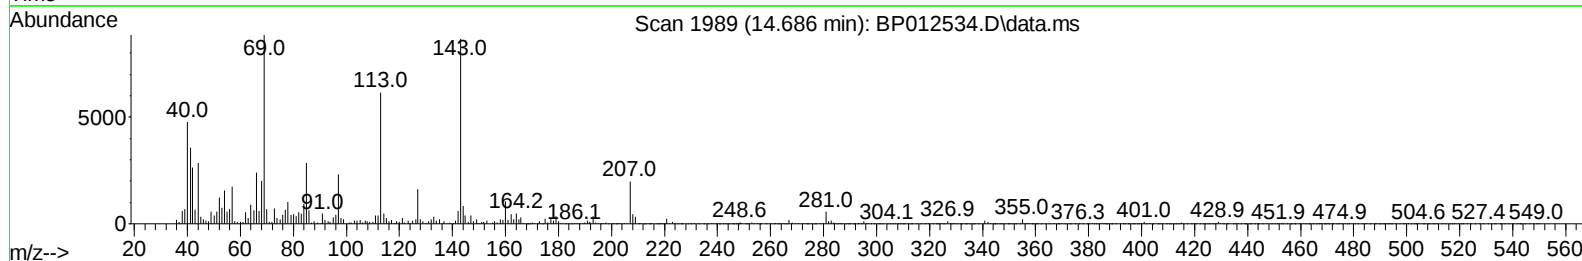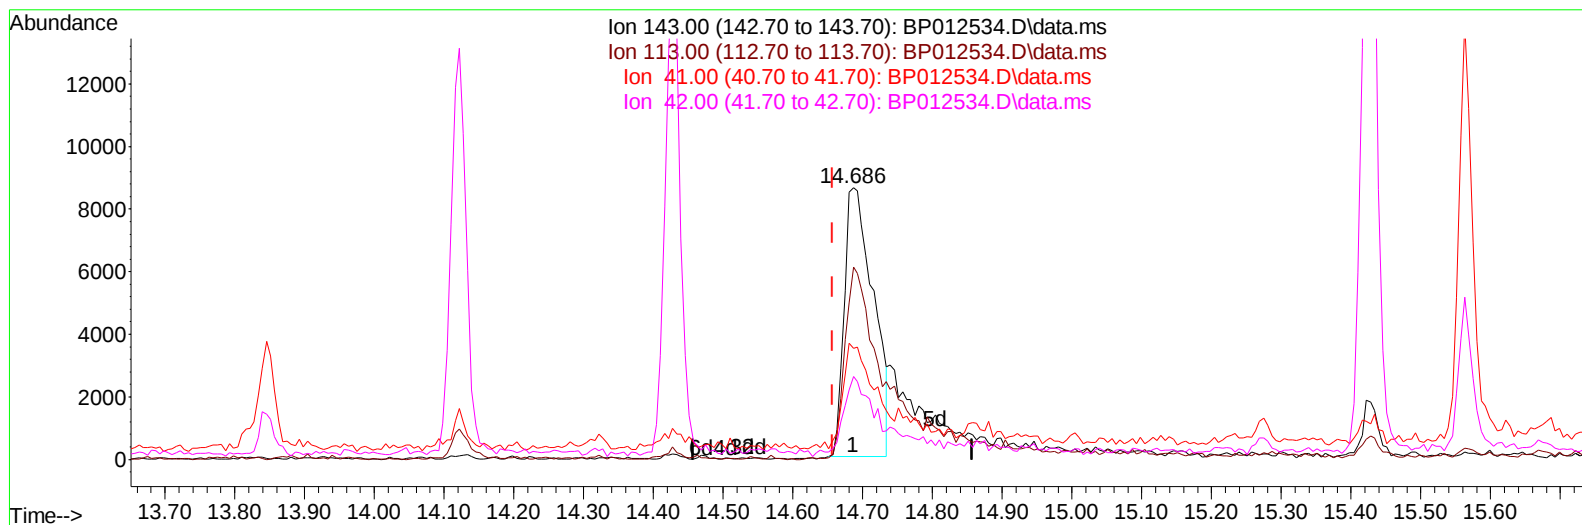

TIC: BP012534.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.686min (+ 0.029) 2.03 ng/u1

response 24779

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	65.10	70.92
41.00	34.50	41.03
42.00	23.60	30.48#




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110722\
Data File : BP012534.D
Acq On : 07 Nov 2022 16:46
Operator : CG/JU
Sample : N5353-19
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DBXB2

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 11/08/2022
Supervised By :mohammad ahmed 11/14/2022

Quant Time: Nov 07 21:41:40 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Nov 04 02:53:36 2022
Response via : Initial Calibration

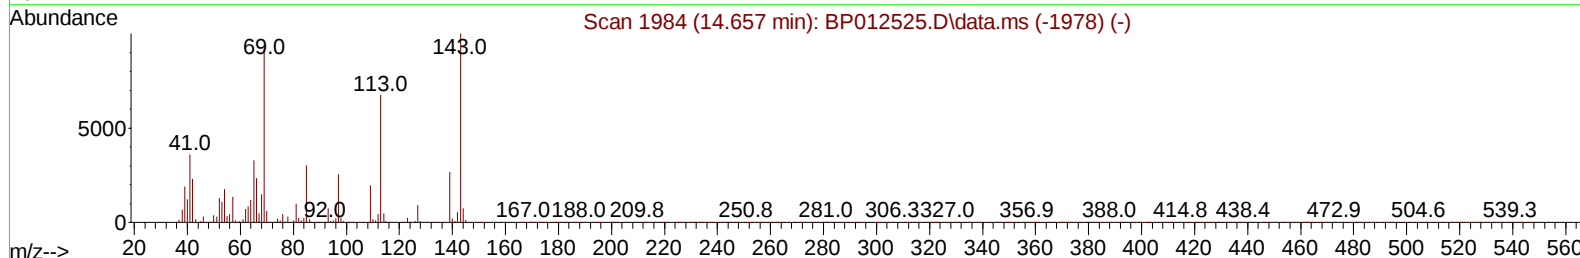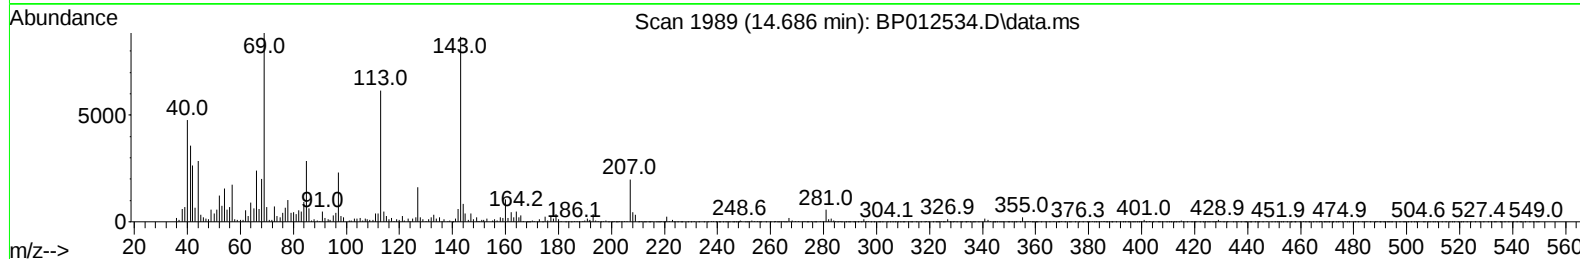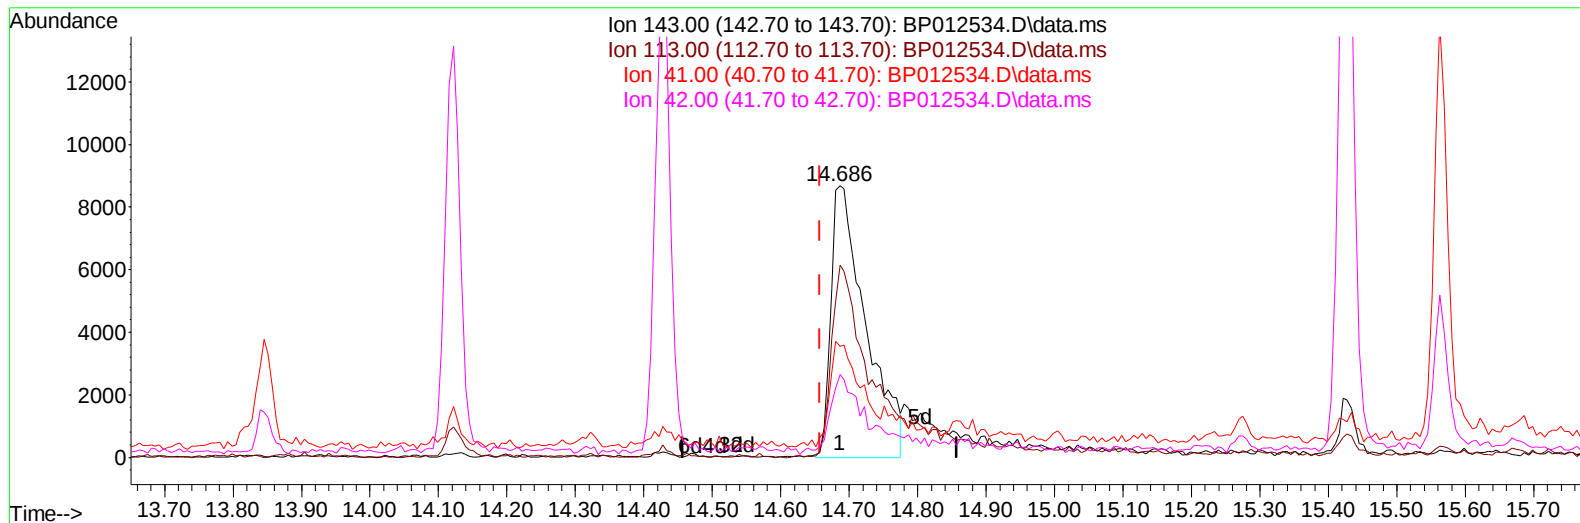

TIC: BP012534.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.686min (+ 0.029) 2.51 ng/ul m

response 30577

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	65.10	70.92
41.00	34.50	41.03
42.00	23.60	30.48#

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110722\
 Data File : BP012534.D
 Acq On : 07 Nov 2022 16:46
 Operator : CG/JU
 Sample : N5353-19
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DBXB2

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 11/08/2022
 Supervised By :mohammad ahmed 11/14/2022

Quant Time: Nov 07 21:41:40 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Nov 04 02:53:36 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.775	152	278956	20.000	ng/ul	0.00
20) Naphthalene-d8	10.575	136	1366827	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.428	164	941189	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.192	188	2157410	20.000	ng/ul	0.00
79) Chrysene-d12	21.286	240	1955536	20.000	ng/ul	0.00
88) Perylene-d12	23.668	264	1788723	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.228	96	25875	3.735	ng/uL	0.00
4) Pyridine-d5	3.663	84	101617	5.106	ng/ul	0.01
7) Phenol-d5	6.957	99	122064	4.879	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.116	67	370613	24.813	ng/ul	0.00
11) 2-Chlorophenol-d4	7.310	132	354687	19.412	ng/ul	0.00
15) 4-Methylphenol-d8	8.499	113	227138	11.478	ng/ul	0.00
21) Nitrobenzene-d5	8.946	128	256836	28.977	ng/ul	0.00
24) 2-Nitrophenol-d4	9.669	143	270284	29.379	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.204	165	465004	23.323	ng/ul	0.00
31) 4-Chloroaniline-d4	10.734	131	518374	17.462	ng/ul	0.00
46) Dimethylphthalate-d6	13.845	166	1845590	28.645	ng/ul	0.00
49) Acenaphthylene-d8	14.122	160	1957235	26.582	ng/ul	0.00
54) 4-Nitrophenol-d4	14.686	143	30577m	2.508	ng/ul	0.03
60) Fluorene-d10	15.428	176	1636171	29.661	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.563	200	250980	22.344	ng/ul	0.00
73) Anthracene-d10	17.292	188	2578372	27.737	ng/ul	0.00
81) Pyrene-d10	19.533	212	3112943	31.706	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.515	264	2600625	29.756	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110722\
Data File : BP012534.D
Acq On : 07 Nov 2022 16:46
Operator : CG/JU
Sample : N5353-19
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DBXB2

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 11/08/2022
Supervised By :mohammad ahmed 11/14/2022

Quant Time: Nov 07 21:41:40 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Nov 04 02:53:36 2022
Response via : Initial Calibration

