




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110722\
Data File : BP012536.D
Acq On : 07 Nov 2022 17:57
Operator : CG/JU
Sample : N5353-16
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DBWX1

Manual IntegrationsAPPROVED

Quant Time: Nov 07 21:42:00 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Nov 04 02:53:36 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 11/08/2022
Supervised By :mohammad ahmed 11/14/2022

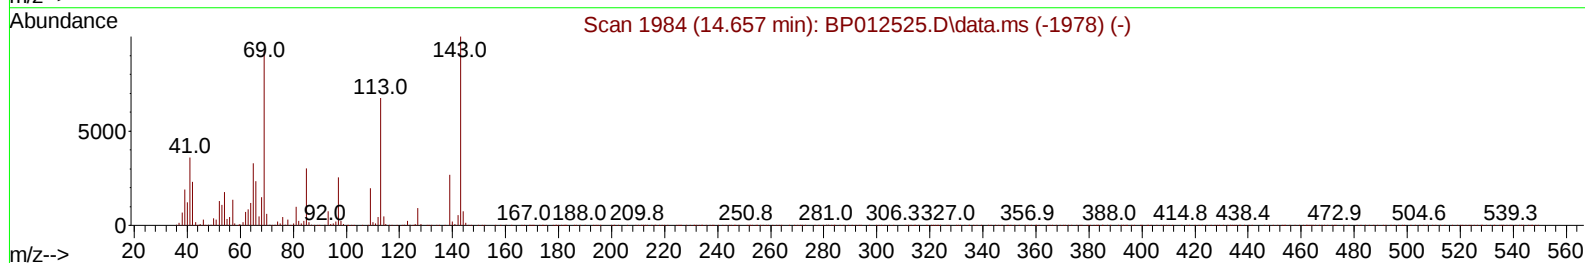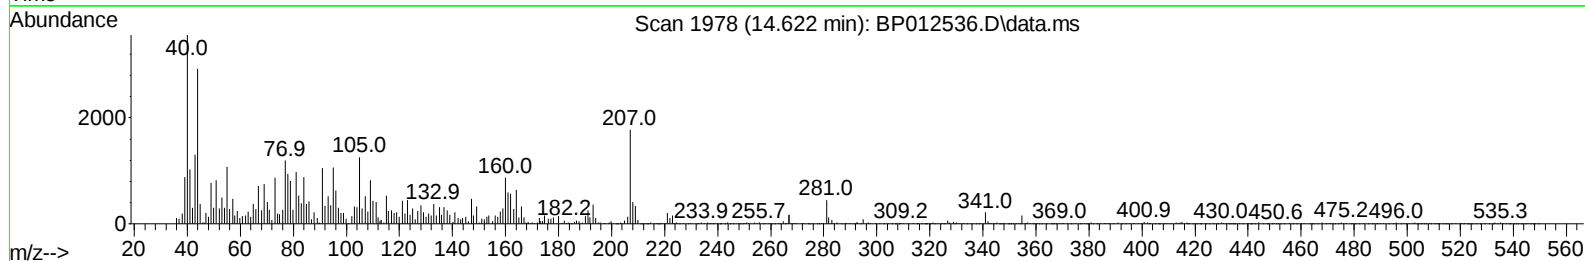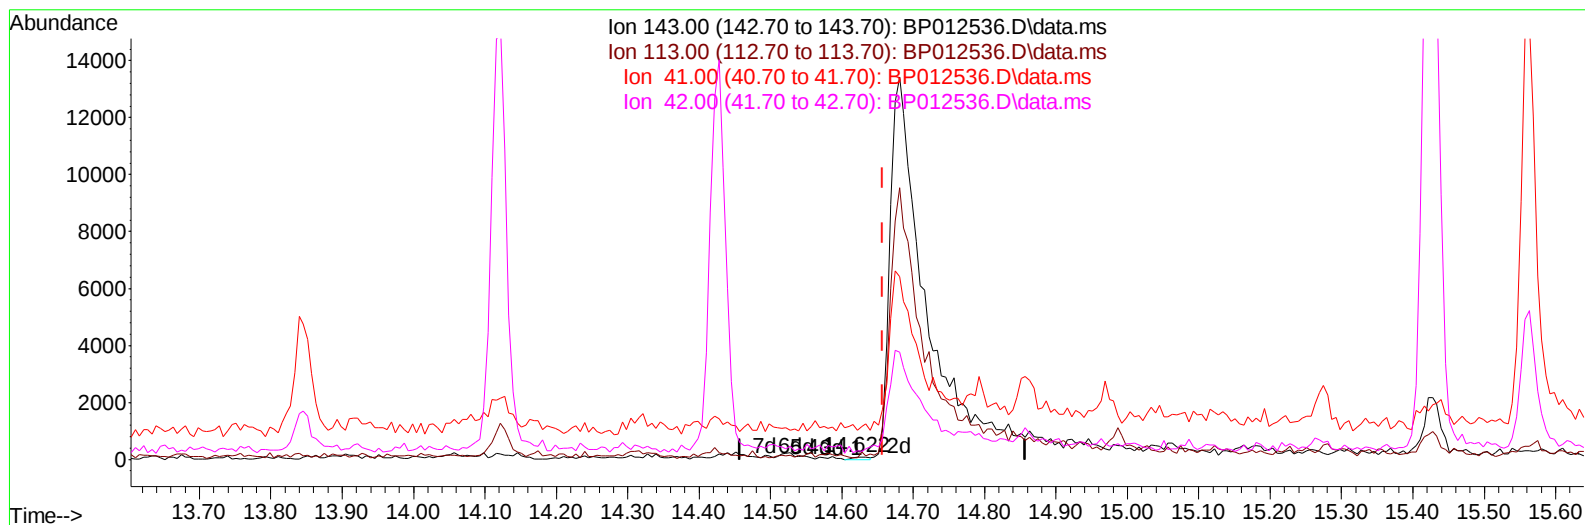

TIC: BP012536.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.622min (-0.035) 0.01 ng/u1

response 139

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	65.10	76.67
41.00	34.50	1138.89#
42.00	23.60	335.56#




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110722\
 Data File : BP012536.D
 Acq On : 07 Nov 2022 17:57
 Operator : CG/JU
 Sample : N5353-16
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DBWX1

Manual IntegrationsAPPROVED

Quant Time: Nov 07 21:42:00 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Nov 04 02:53:36 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 11/08/2022
 Supervised By :mohammad ahmed 11/14/2022

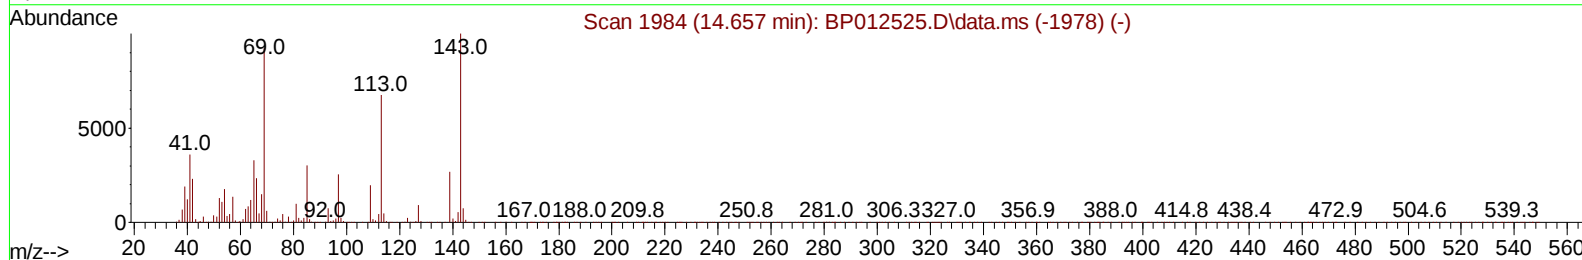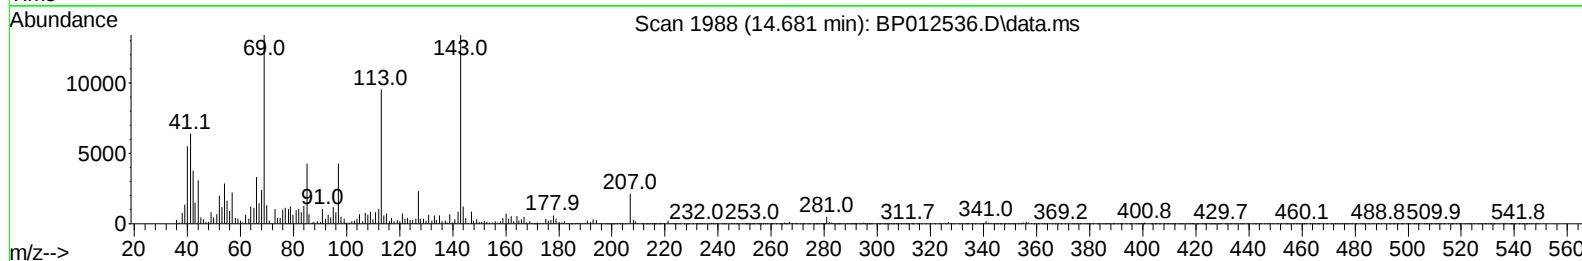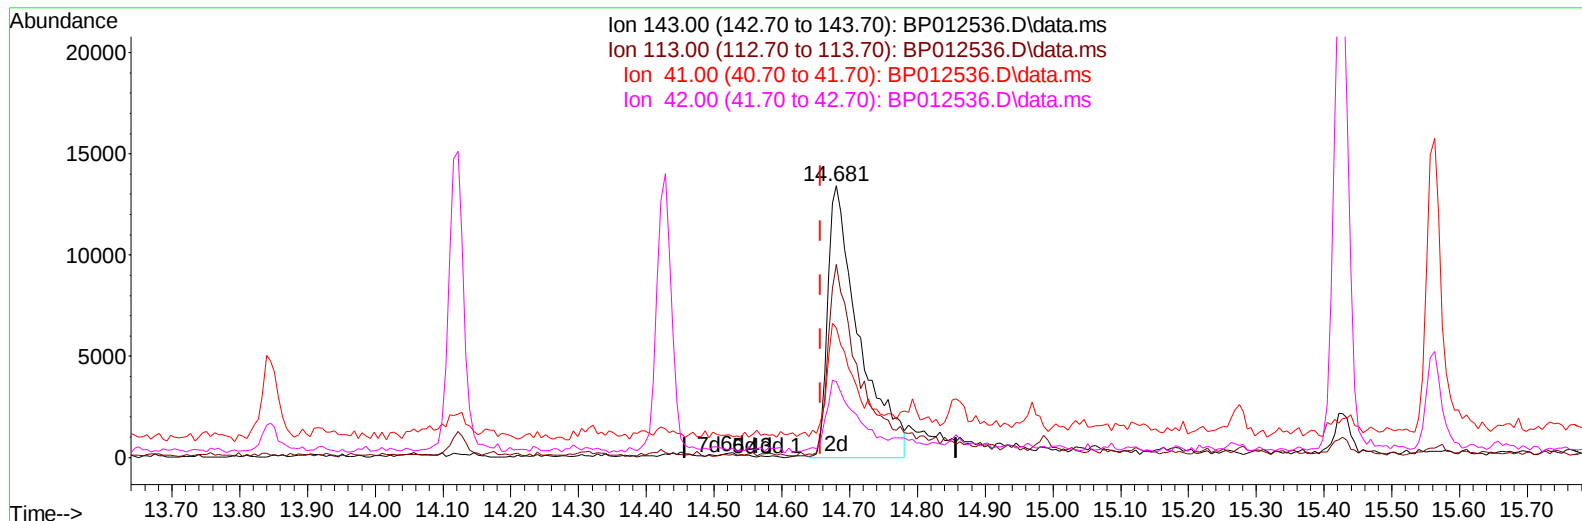

TIC: BP012536.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.681min (+ 0.023) 4.01 ng/ul m

response 42951

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	65.10	71.05
41.00	34.50	47.79#
42.00	23.60	28.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110722\
 Data File : BP012536.D
 Acq On : 07 Nov 2022 17:57
 Operator : CG/JU
 Sample : N5353-16
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DBWX1

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 11/08/2022
 Supervised By :mohammad ahmed 11/14/2022

Quant Time: Nov 07 21:42:00 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Nov 04 02:53:36 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.775	152	247843	20.000	ng/ul	0.00
20) Naphthalene-d8	10.575	136	1197036	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.428	164	827012	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.192	188	1852747	20.000	ng/ul	0.00
79) Chrysene-d12	21.286	240	1687809	20.000	ng/ul	0.00
88) Perylene-d12	23.668	264	1532866	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.228	96	23544	3.825	ng/uL	0.00
4) Pyridine-d5	3.663	84	124750	7.055	ng/ul	0.01
7) Phenol-d5	6.957	99	147951	6.656	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.116	67	430835	32.466	ng/ul	0.00
11) 2-Chlorophenol-d4	7.310	132	428006	26.366	ng/ul	0.00
15) 4-Methylphenol-d8	8.499	113	303135	17.242	ng/ul	0.00
21) Nitrobenzene-d5	8.946	128	299144	38.537	ng/ul	0.00
24) 2-Nitrophenol-d4	9.669	143	310197	38.500	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.204	165	562977	32.242	ng/ul	0.00
31) 4-Chloroaniline-d4	10.728	131	665906	25.613	ng/ul	0.00
46) Dimethylphthalate-d6	13.845	166	2112709	37.318	ng/ul	0.00
49) Acenaphthylene-d8	14.122	160	2254635	34.849	ng/ul	0.00
54) 4-Nitrophenol-d4	14.681	143	42951m	4.009	ng/ul	0.02
60) Fluorene-d10	15.428	176	1866155	38.500	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.563	200	283283	29.367	ng/ul	0.00
73) Anthracene-d10	17.292	188	3104249	38.885	ng/ul	0.00
81) Pyrene-d10	19.533	212	3609039	42.590	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.515	264	2970358	39.659	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110722\
Data File : BP012536.D
Acq On : 07 Nov 2022 17:57
Operator : CG/JU
Sample : N5353-16
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DBWX1

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 11/08/2022
Supervised By :mohammad ahmed 11/14/2022

Quant Time: Nov 07 21:42:00 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Nov 04 02:53:36 2022
Response via : Initial Calibration

