




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110722\
 Data File : BP012537.D
 Acq On : 07 Nov 2022 18:32
 Operator : CG/JU
 Sample : N5353-09
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DBWR9

Manual IntegrationsAPPROVED

Quant Time: Nov 07 21:42:10 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Nov 04 02:53:36 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 11/08/2022
 Supervised By :mohammad ahmed 11/14/2022

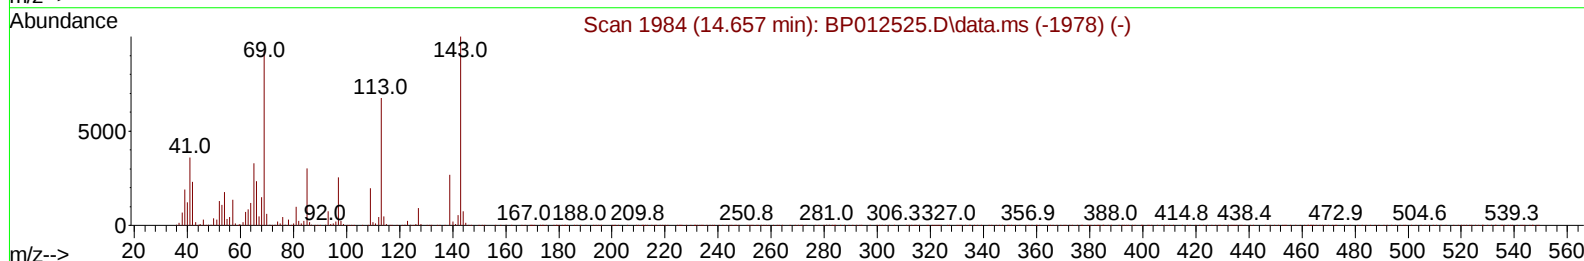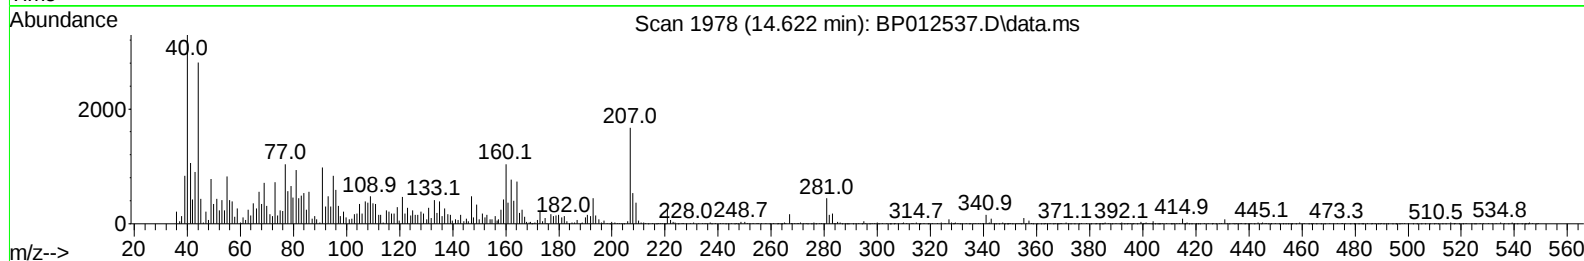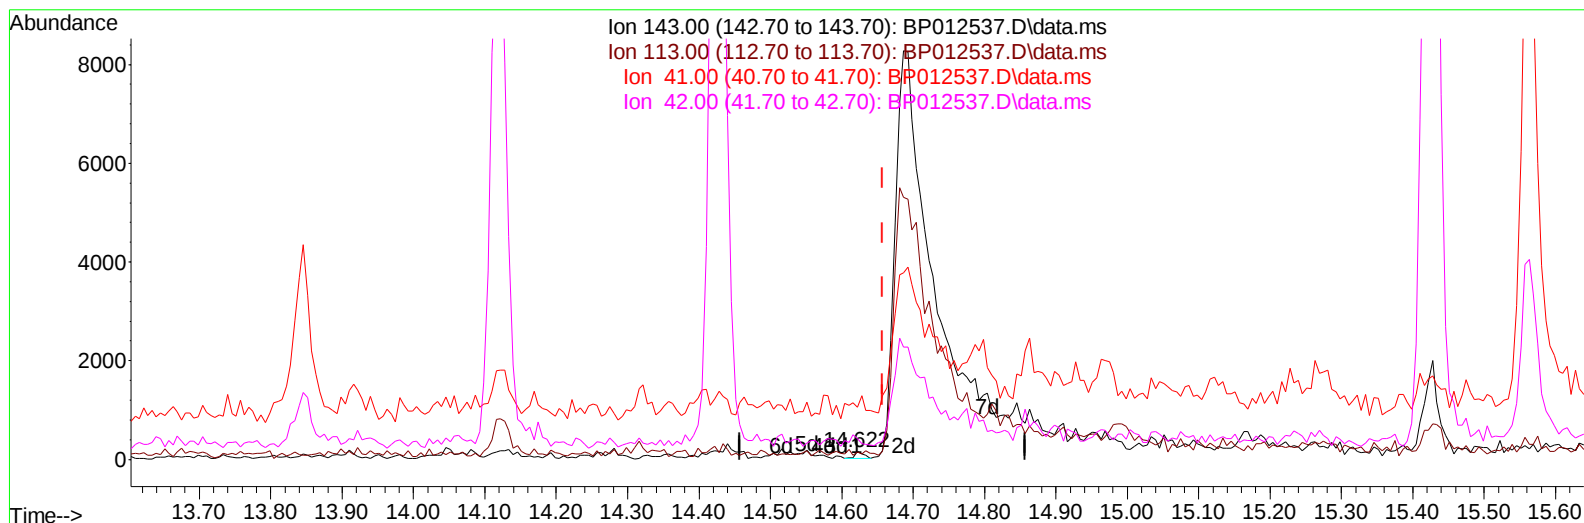

TIC: BP012537.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.622min (-0.035) 0.01 ng/u1

response 108

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	65.10	108.86#
41.00	34.50	673.42#
42.00	23.60	271.52#




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110722\
 Data File : BP012537.D
 Acq On : 07 Nov 2022 18:32
 Operator : CG/JU
 Sample : N5353-09
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DBWR9

Manual IntegrationsAPPROVED

Quant Time: Nov 07 21:42:10 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Nov 04 02:53:36 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 11/08/2022
 Supervised By :mohammad ahmed 11/14/2022

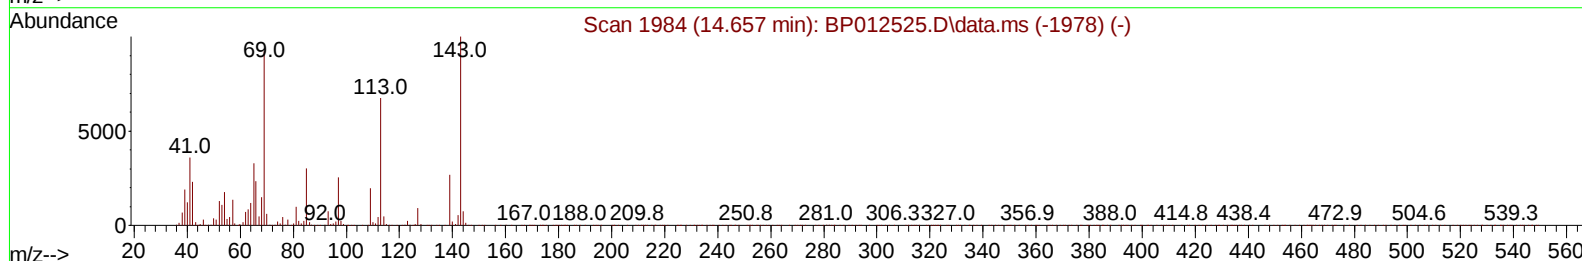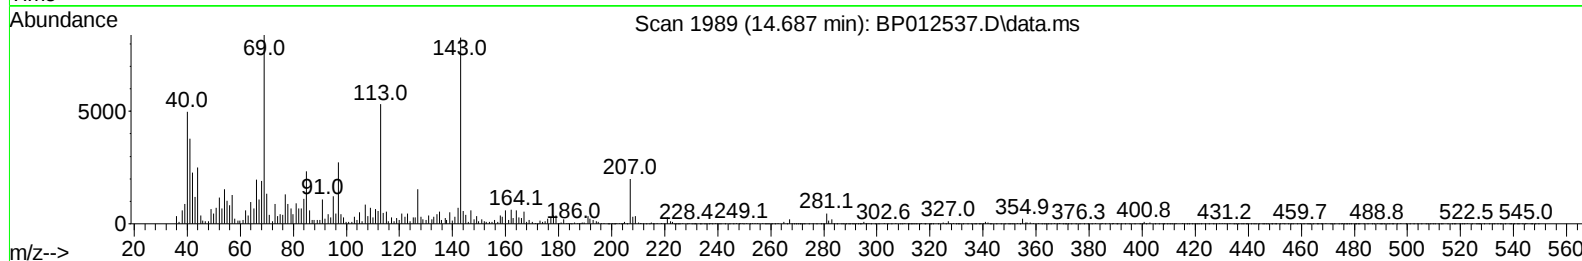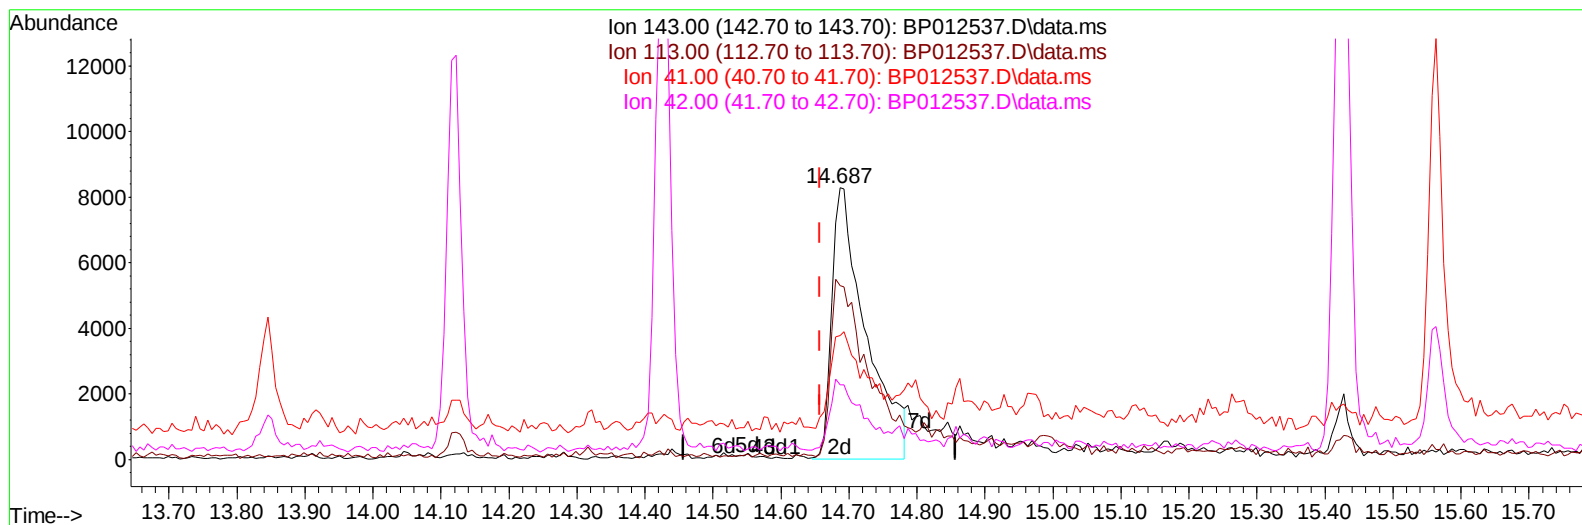

TIC: BP012537.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.687min (+ 0.029) 2.29 ng/ul m

response 28707

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	65.10	64.09
41.00	34.50	45.69#
42.00	23.60	27.49

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110722\
 Data File : BP012537.D
 Acq On : 07 Nov 2022 18:32
 Operator : CG/JU
 Sample : N5353-09
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DBWR9

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 11/08/2022
 Supervised By :mohammad ahmed 11/14/2022

Quant Time: Nov 07 21:42:10 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Nov 04 02:53:36 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.775	152	288229	20.000	ng/ul	0.00
20) Naphthalene-d8	10.575	136	1411696	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.428	164	967987	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.192	188	2211242	20.000	ng/ul	0.00
79) Chrysene-d12	21.286	240	2033400	20.000	ng/ul	0.00
88) Perylene-d12	23.668	264	1850189	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.228	96	23934	3.344	ng/uL	0.00
4) Pyridine-d5	3.664	84	90152	4.384	ng/ul	0.01
7) Phenol-d5	6.958	99	111703	4.321	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.116	67	344994	22.355	ng/ul	0.00
11) 2-Chlorophenol-d4	7.311	132	333664	17.674	ng/ul	0.00
15) 4-Methylphenol-d8	8.499	113	221395	10.828	ng/ul	0.00
21) Nitrobenzene-d5	8.946	128	234132	25.575	ng/ul	0.00
24) 2-Nitrophenol-d4	9.669	143	243618	25.639	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.204	165	434146	21.083	ng/ul	0.00
31) 4-Chloroaniline-d4	10.728	131	596510	19.455	ng/ul	0.00
46) Dimethylphthalate-d6	13.845	166	1677536	25.316	ng/ul	0.00
49) Acenaphthylene-d8	14.122	160	1777143	23.468	ng/ul	0.00
54) 4-Nitrophenol-d4	14.687	143	28707m	2.289	ng/ul	0.03
60) Fluorene-d10	15.428	176	1482926	26.138	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.563	200	215436	18.713	ng/ul	0.00
73) Anthracene-d10	17.292	188	2561129	26.881	ng/ul	0.00
81) Pyrene-d10	19.533	212	3038535	29.763	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.510	264	2451264	27.115	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110722\
Data File : BP012537.D
Acq On : 07 Nov 2022 18:32
Operator : CG/JU
Sample : N5353-09
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DBWR9

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 11/08/2022
Supervised By :mohammad ahmed 11/14/2022

Quant Time: Nov 07 21:42:10 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Nov 04 02:53:36 2022
Response via : Initial Calibration

