

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110722\
 Data File : BP012526.D
 Acq On : 07 Nov 2022 12:04
 Operator : CG/JU
 Sample : PB148749BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK749

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
 Title : SVOA CALIBRATION

Signal : TIC: BP012526.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.228	37	41	50	rVB	60195	90341	1.27%	0.129%
2	3.740	124	128	130	rBV5	8122	12600	0.18%	0.018%
3	3.964	162	166	171	rVB	15436	21989	0.31%	0.031%
4	6.958	668	675	694	rBV	1009883	1727472	24.32%	2.473%
5	7.117	696	702	717	rVV	781268	1323969	18.64%	1.895%
6	7.311	728	735	751	rBV	1002349	1653050	23.27%	2.366%
7	7.775	807	814	831	rBV	938570	1574188	22.16%	2.253%
8	8.499	930	937	954	rBV	1301181	2278236	32.07%	3.261%
9	8.946	1006	1013	1031	rBV	938255	1671014	23.52%	2.392%
10	9.669	1129	1136	1157	rBV	837805	1450985	20.42%	2.077%
11	10.210	1219	1228	1261	rBV	1122559	2437820	34.32%	3.490%
12	10.581	1283	1291	1309	rBV	1514085	2645246	37.24%	3.787%
13	10.763	1317	1322	1330	rBV7	7156	20331	0.29%	0.029%
14	12.187	1559	1564	1574	rBV5	14490	35731	0.50%	0.051%
15	13.322	1753	1757	1759	rBV5	5139	7552	0.11%	0.011%
16	13.399	1765	1770	1776	rBV7	5254	9017	0.13%	0.013%
17	13.846	1835	1846	1867	rBV	2453637	3740063	52.65%	5.354%
18	14.122	1886	1893	1913	rBV2	2713079	4259277	59.96%	6.097%
19	14.428	1938	1945	1957	rBV	2721810	3995012	56.24%	5.719%
20	14.663	1979	1985	2013	rBV	474679	1362382	19.18%	1.950%
21	15.428	2106	2115	2133	rBV	3782804	5772218	81.25%	8.263%
22	15.563	2133	2138	2153	rVV	538081	870079	12.25%	1.246%
23	15.669	2153	2156	2163	rVB3	22875	39263	0.55%	0.056%
24	16.981	2375	2379	2385	rVB3	8413	14333	0.20%	0.021%
25	17.192	2408	2415	2425	rBV	3441227	5057500	71.19%	7.240%
26	17.292	2426	2432	2456	rVB	4132504	6362989	89.57%	9.109%
27	19.110	2737	2741	2746	rBV3	53187	82374	1.16%	0.118%
28	19.181	2750	2753	2758	rVV	45599	61947	0.87%	0.089%
29	19.534	2807	2813	2828	rBV	5268044	7104029	100.00%	10.169%
30	21.286	3106	3111	3122	rBV	3398703	4657554	65.56%	6.667%
31	23.516	3483	3490	3504	rVB2	2586743	5538916	77.97%	7.929%
32	23.669	3510	3516	3531	rVB	1959684	3980067	56.03%	5.697%




Sum of corrected areas: 69857544

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110722\
Data File : BP012526.D
Acq On : 07 Nov 2022 12:04
Operator : CG/JU
Sample : PB148749BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK749

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

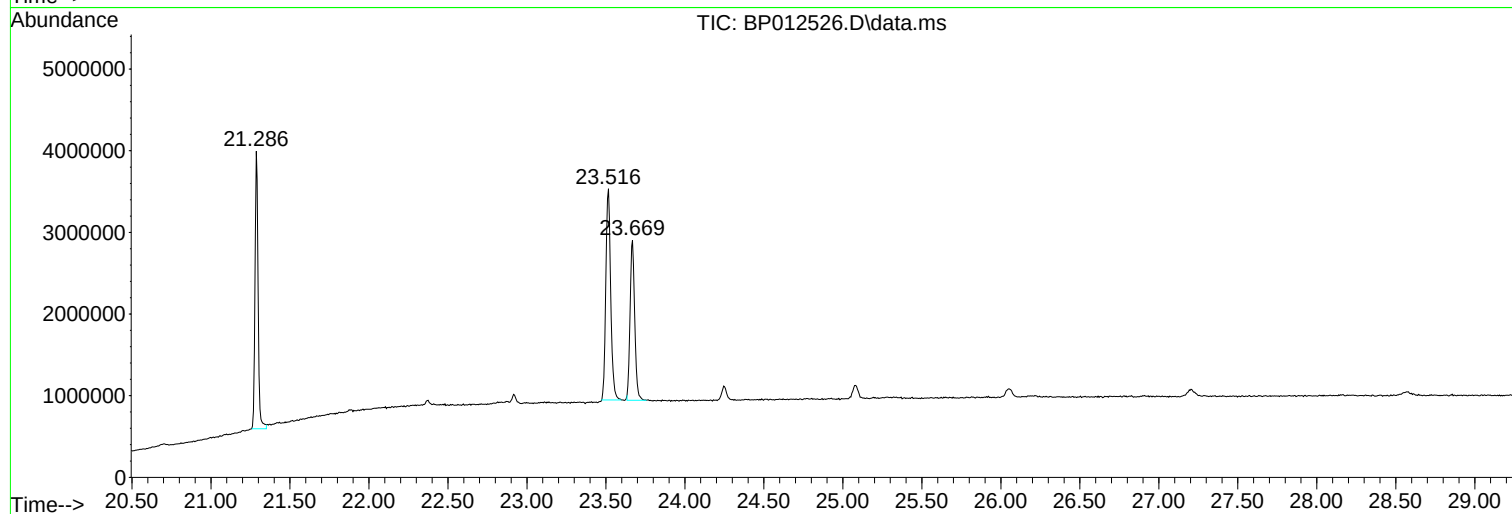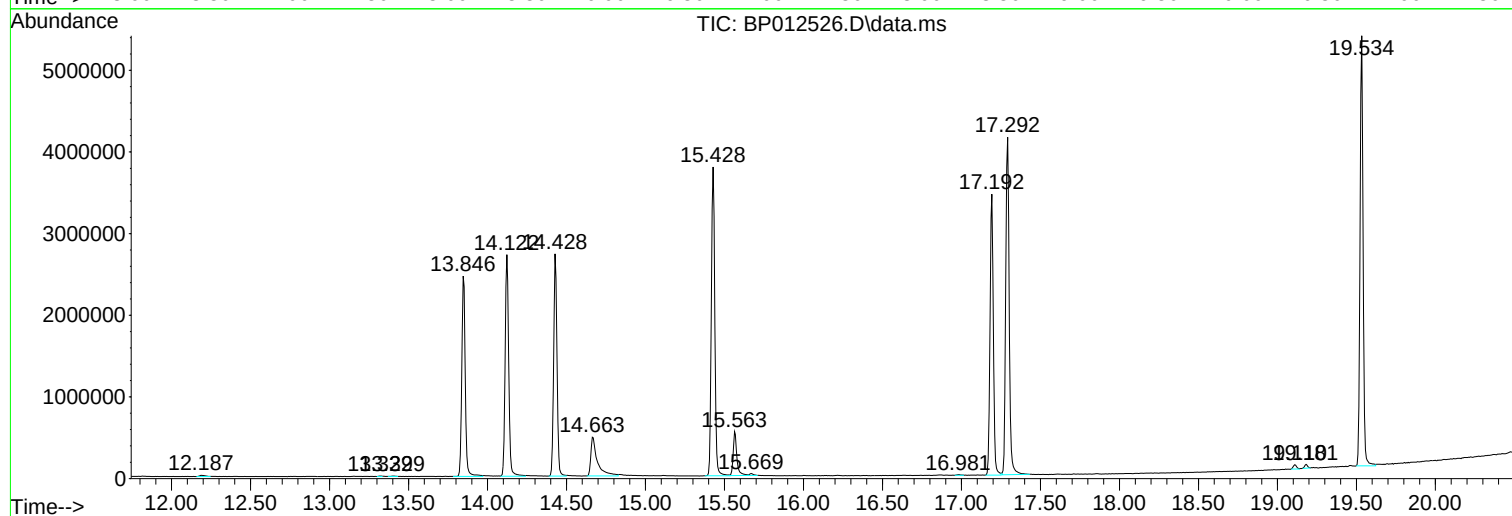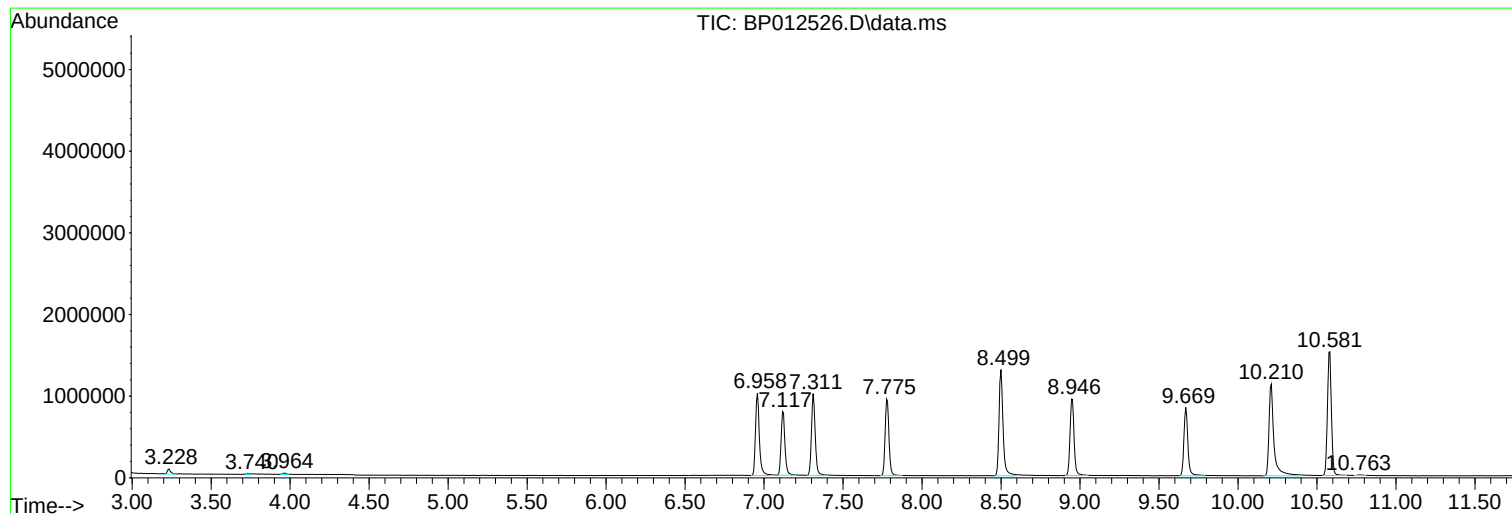

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110722\
Data File : BP012526.D
Acq On : 07 Nov 2022 12:04
Operator : CG/JU
Sample : PB148749BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK749

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110722\
Data File : BP012526.D
Acq On : 07 Nov 2022 12:04
Operator : CG/JU
Sample : PB148749BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK749

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc