

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110722\
 Data File : BP012527.D
 Acq On : 07 Nov 2022 12:39
 Operator : CG/JU
 Sample : PB148750BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK750

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
 Title : SVOA CALIBRATION

Signal : TIC: BP012527.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.228	37	41	52	rVB	71060	106002	1.00%	0.118%
2	3.705	119	122	130	rBV2	16927	42385	0.40%	0.047%
3	3.964	162	166	174	rVB	25847	39560	0.37%	0.044%
4	6.957	668	675	695	rBV	1149839	2032290	19.18%	2.264%
5	7.116	696	702	719	rVB	944987	1584007	14.95%	1.765%
6	7.310	728	735	752	rBV	1187989	1973048	18.62%	2.198%
7	7.775	805	814	827	rBV	927791	1586814	14.98%	1.768%
8	8.499	930	937	960	rBV	1677802	2943593	27.79%	3.279%
9	8.946	1006	1013	1028	rBV	1247380	2178203	20.56%	2.427%
10	9.669	1129	1136	1151	rBV	1083457	1873281	17.68%	2.087%
11	10.204	1220	1227	1254	rBV	1520446	3157620	29.81%	3.518%
12	10.575	1282	1290	1305	rBV	1693462	2949784	27.84%	3.286%
13	10.763	1316	1322	1333	rBV3	15193	38753	0.37%	0.043%
14	12.187	1557	1564	1573	rBV2	19927	49786	0.47%	0.055%
15	13.404	1764	1771	1776	rBV7	8205	14236	0.13%	0.016%
16	13.845	1837	1846	1860	rBV	3482194	5103563	48.18%	5.685%
17	14.122	1885	1893	1913	rBV	2524289	3803095	35.90%	4.237%
18	14.428	1938	1945	1959	rBV	3015394	4515745	42.63%	5.031%
19	14.663	1979	1985	2013	rBV	782418	2024845	19.11%	2.256%
20	15.428	2108	2115	2133	rBV	5171707	7796948	73.60%	8.686%
21	15.563	2133	2138	2152	rVV	852534	1332401	12.58%	1.484%
22	15.669	2152	2156	2168	rVB	31603	62270	0.59%	0.069%
23	17.192	2408	2415	2425	rBV	4057873	5856727	55.29%	6.524%
24	17.292	2425	2432	2453	rVB	5991571	8855693	83.59%	9.865%
25	19.110	2737	2741	2748	rBV2	82331	119027	1.12%	0.133%
26	19.180	2749	2753	2759	rVV	71649	108329	1.02%	0.121%
27	19.533	2807	2813	2827	rBV	7560522	10593684	100.00%	11.801%
28	21.286	3106	3111	3123	rBV	4416540	5889149	55.59%	6.561%
29	23.515	3483	3490	3504	rVB	3897558	8085953	76.33%	9.008%
30	23.668	3510	3516	3528	rVB2	2451094	5049451	47.66%	5.625%




Sum of corrected areas: 89766242

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110722\
Data File : BP012527.D
Acq On : 07 Nov 2022 12:39
Operator : CG/JU
Sample : PB148750BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK750

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

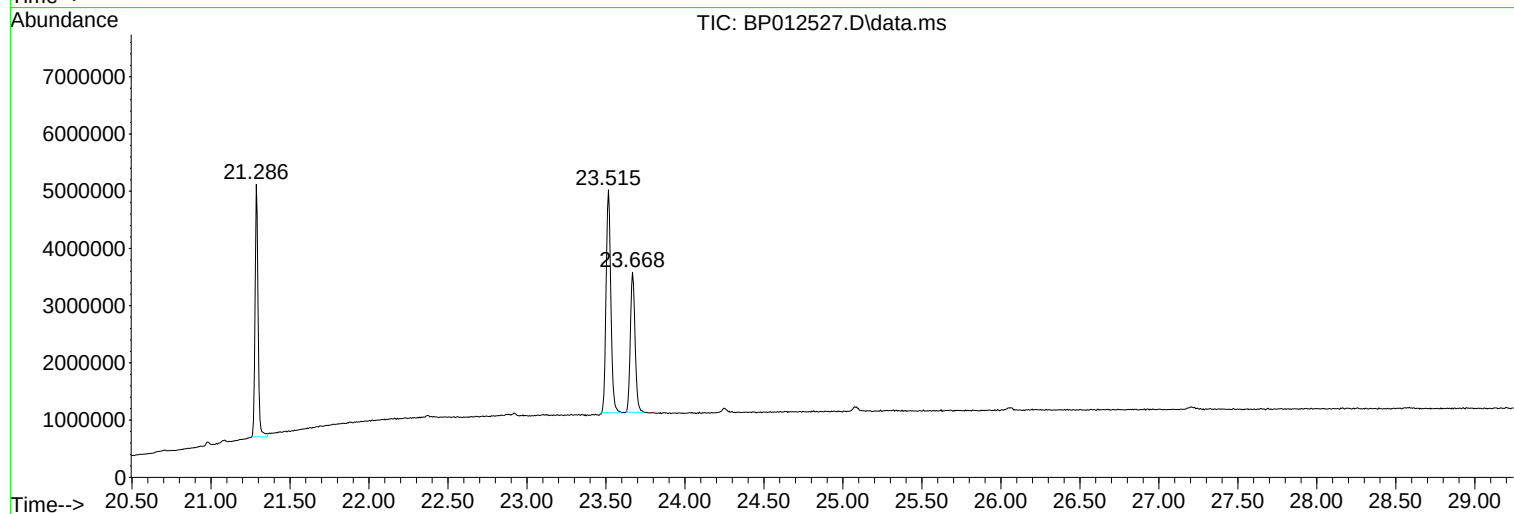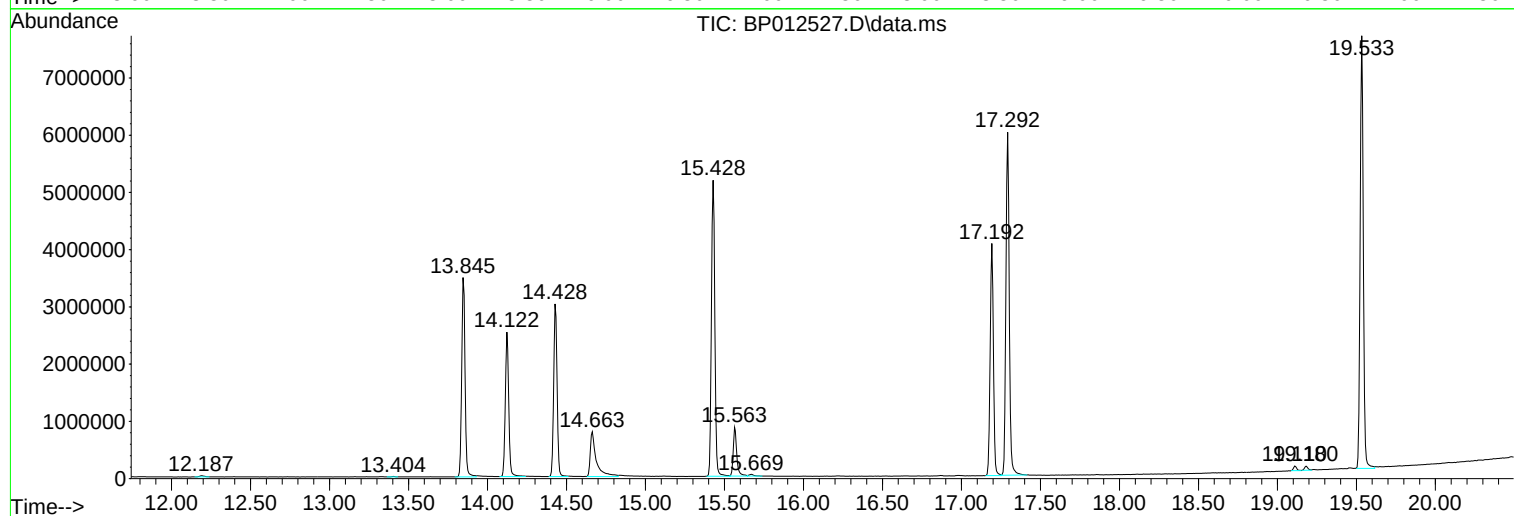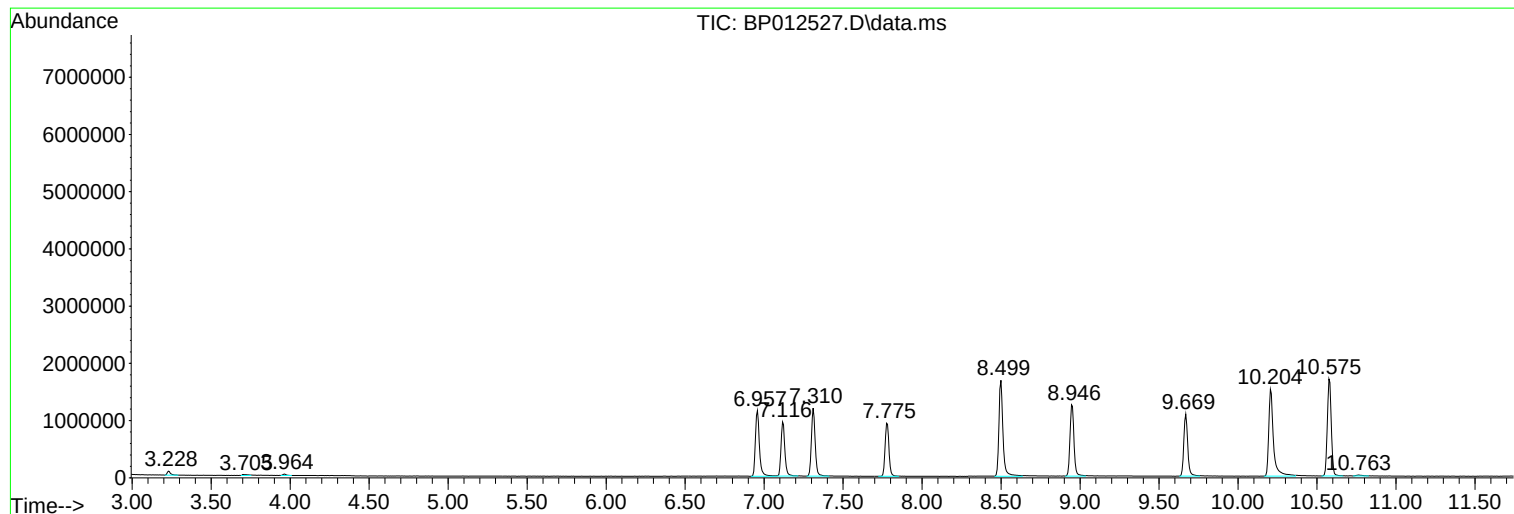

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110722\
Data File : BP012527.D
Acq On : 07 Nov 2022 12:39
Operator : CG/JU
Sample : PB148750BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK750

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110722\
Data File : BP012527.D
Acq On : 07 Nov 2022 12:39
Operator : CG/JU
Sample : PB148750BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK750

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc