

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110722\
 Data File : BP012528.D
 Acq On : 07 Nov 2022 13:15
 Operator : CG/JU
 Sample : N5353-10
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DBWU7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
 Title : SVOA CALIBRATION

Signal : TIC: BP012528.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.234	38	42	54	rVB	61050	106267	0.86%	0.099%
2	3.658	112	114	132	rBV	346941	656275	5.34%	0.610%
3	3.864	145	149	158	rVB2	22861	42713	0.35%	0.040%
4	3.964	162	166	174	rVB	22245	37771	0.31%	0.035%
5	4.487	251	255	264	rVB10	11737	25839	0.21%	0.024%
6	6.893	656	664	670	rBV3	11677	23046	0.19%	0.021%
7	6.958	670	675	688	rBV	287465	542700	4.42%	0.504%
8	7.116	696	702	717	rBV	1230419	2019713	16.43%	1.877%
9	7.310	728	735	744	rBV	1158290	1924922	15.66%	1.789%
10	7.422	750	754	770	rVB3	18753	52723	0.43%	0.049%
11	7.775	807	814	823	rBV	1221751	2054895	16.72%	1.909%
12	8.263	891	897	904	rBV6	9919	20305	0.17%	0.019%
13	8.499	930	937	959	rBV	1016194	1804887	14.69%	1.677%
14	8.946	1006	1013	1029	rBV	1524126	2620064	21.32%	2.434%
15	9.069	1029	1034	1038	rVV7	7840	12656	0.10%	0.012%
16	9.328	1073	1078	1084	rVB	41640	67538	0.55%	0.063%
17	9.669	1127	1136	1152	rBV	1228944	2112585	17.19%	1.963%
18	10.204	1219	1227	1248	rBV	1949108	3641062	29.63%	3.383%
19	10.387	1252	1258	1274	rVB3	36174	125297	1.02%	0.116%
20	10.575	1283	1290	1304	rVB	2025456	3478051	28.30%	3.232%
21	10.734	1306	1317	1347	rVV	1069785	2188316	17.81%	2.033%
22	11.010	1362	1364	1376	rVB	7284	18841	0.15%	0.018%
23	11.416	1427	1433	1441	rVB	6062	16931	0.14%	0.016%
24	11.828	1495	1503	1507	rVB4	13017	25596	0.21%	0.024%
25	12.175	1557	1562	1572	rVB2	33113	67527	0.55%	0.063%
26	13.040	1704	1709	1714	rBV8	7594	15253	0.12%	0.014%
27	13.240	1733	1743	1749	rBV2	34296	62017	0.50%	0.058%
28	13.322	1752	1757	1764	rVV5	16600	32546	0.26%	0.030%
29	13.404	1766	1771	1777	rVB6	8884	16990	0.14%	0.016%
30	13.845	1838	1846	1859	rBV	4117779	5995362	48.78%	5.570%
31	14.122	1886	1893	1911	rBV	4809539	7255114	59.04%	6.741%
32	14.322	1924	1927	1932	rVB5	10407	14858	0.12%	0.014%
33	14.428	1938	1945	1955	rBV	3351740	5075706	41.30%	4.716%
34	14.681	1982	1988	2003	rBV2	93127	285860	2.33%	0.266%
35	14.998	2038	2042	2048	rBV2	22287	40715	0.33%	0.038%
36	15.269	2085	2088	2095	rVB2	30299	42041	0.34%	0.039%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110722\
 Data File : BP012528.D
 Acq On : 07 Nov 2022 13:15
 Operator : CG/JU
 Sample : N5353-10
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DBWU7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
 Title : SVOA CALIBRATION

37	15.428	2108	2115	2132	rBV	6125345	9435066	76.77%	8.766%
38	15.563	2132	2138	2152	rVV	1316843	2005422	16.32%	1.863%
39	15.669	2153	2156	2163	rVB4	33214	52794	0.43%	0.049%
40	16.216	2246	2249	2252	rVB5	9750	12907	0.11%	0.012%
41	16.269	2255	2258	2262	rVB	17581	17985	0.15%	0.017%
42	16.333	2265	2269	2275	rVB4	21965	41224	0.34%	0.038%
43	16.392	2275	2279	2283	rBV4	21286	36345	0.30%	0.034%
44	16.598	2309	2314	2319	rBV6	33360	57169	0.47%	0.053%
45	17.192	2408	2415	2425	rBV	4513214	6385619	51.96%	5.933%
46	17.292	2426	2432	2452	rVB2	6977069	10449783	85.03%	9.709%
47	17.863	2526	2529	2532	rVB3	26143	31123	0.25%	0.029%
48	17.969	2544	2547	2553	rBV4	59138	114083	0.93%	0.106%
49	18.080	2562	2566	2576	rBV	245359	387956	3.16%	0.360%
50	19.110	2738	2741	2746	rVB2	115331	141945	1.16%	0.132%
51	19.180	2749	2753	2760	rBV	103026	196340	1.60%	0.182%
52	19.316	2773	2776	2786	rBV2	145736	222218	1.81%	0.206%
53	19.533	2807	2813	2828	rBV	8798088	12289481	100.00%	11.419%
54	21.010	3060	3064	3070	rBV2	481377	717846	5.84%	0.667%
55	21.286	3107	3111	3121	rBV	4663220	6282092	51.12%	5.837%
56	23.515	3483	3490	3508	rVB2	5009008	10448453	85.02%	9.708%
57	23.668	3510	3516	3529	rVB2	2777691	5778890	47.02%	5.369%




Sum of corrected areas: 107627723

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110722\
Data File : BP012528.D
Acq On : 07 Nov 2022 13:15
Operator : CG/JU
Sample : N5353-10
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DBWU7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

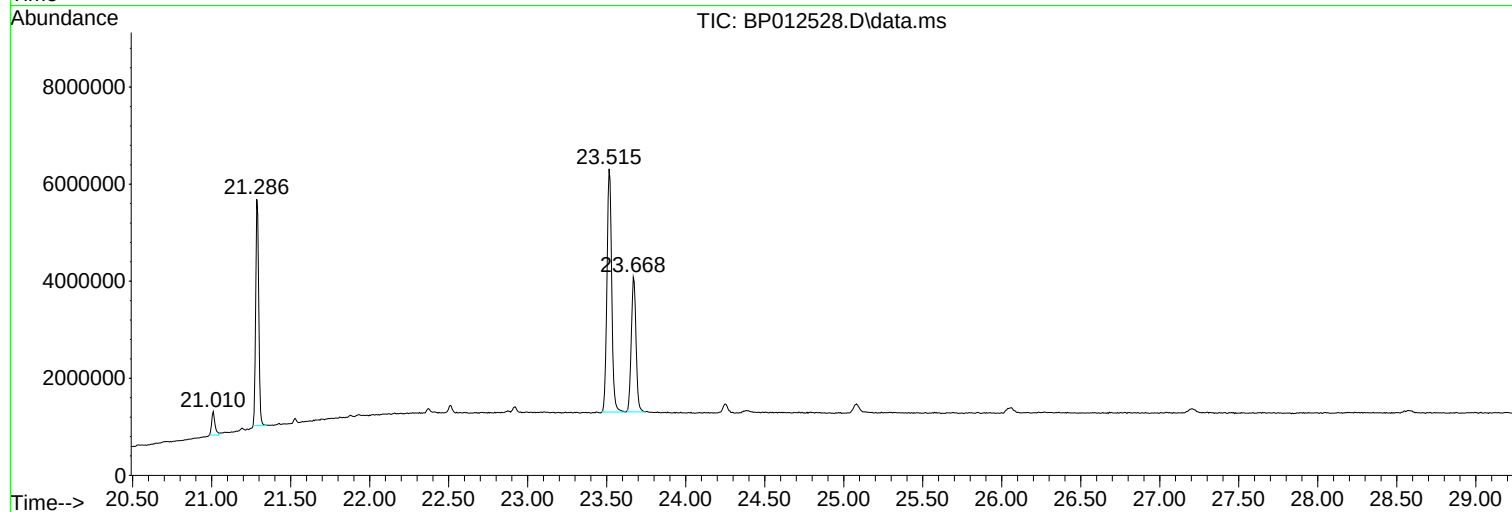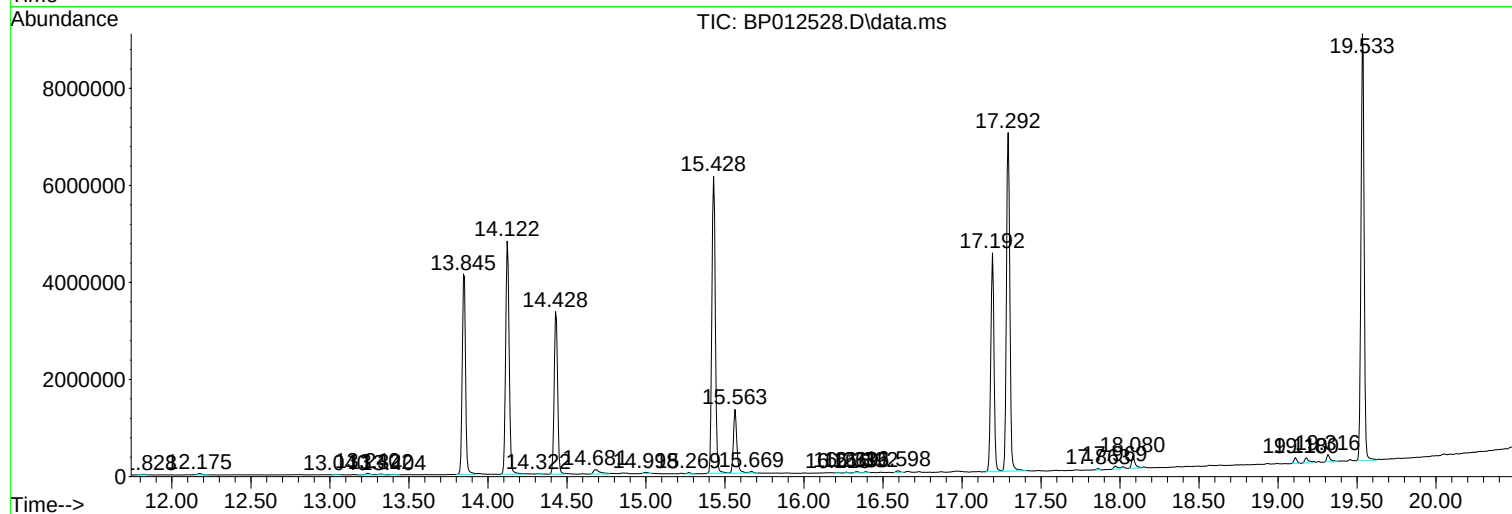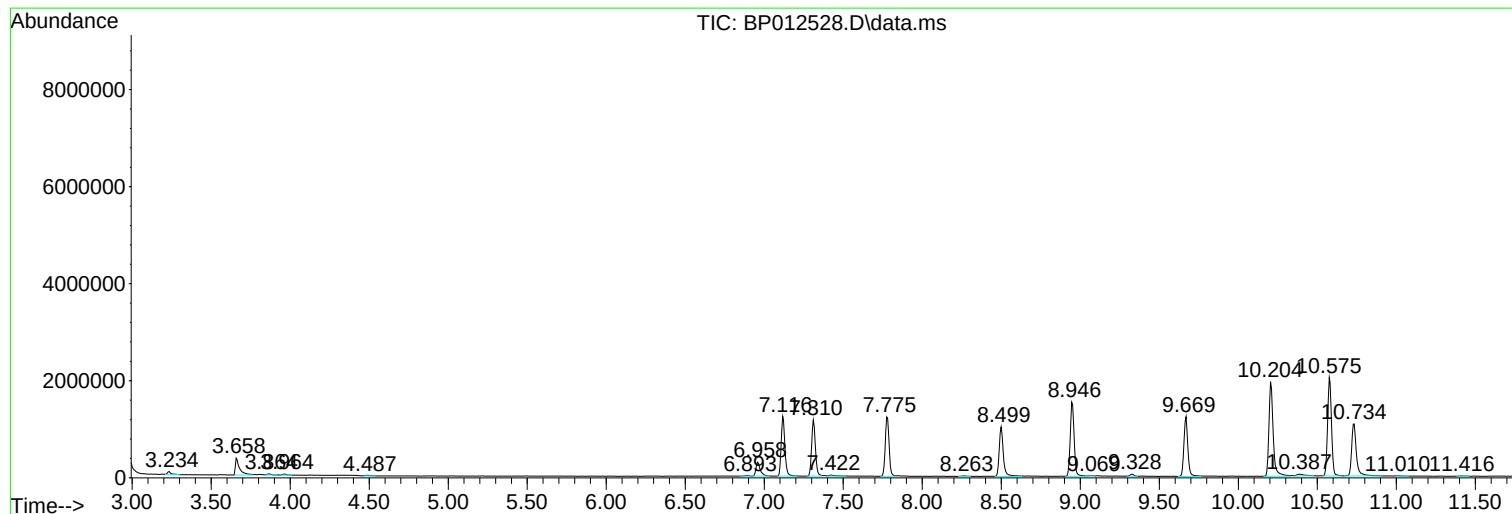

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110722\
Data File : BP012528.D
Acq On : 07 Nov 2022 13:15
Operator : CG/JU
Sample : N5353-10
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DBWU7










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Behenic alcohol Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
21.010	2.29 ng/ul	717846	Chrysene-d12	21.286

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Behenic alcohol	326	C22H46O	000661-19-8	94
2			Trifluoroacetic acid, pentadecyl...	324	C17H31F3O2	959010-23-2	94
3			n-Nonadecanol-1	284	C19H40O	001454-84-8	94
4			n-Tetracosanol-1	354	C24H50O	000506-51-4	91
5			1-Octadecanol	270	C18H38O	000112-92-5	91

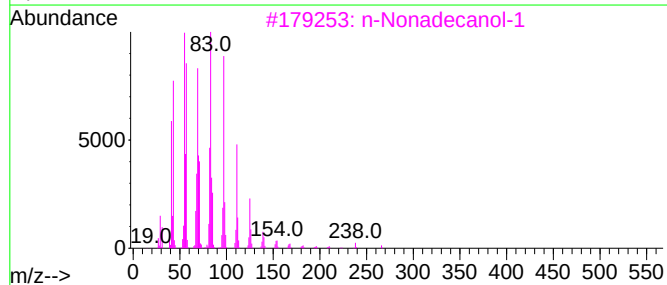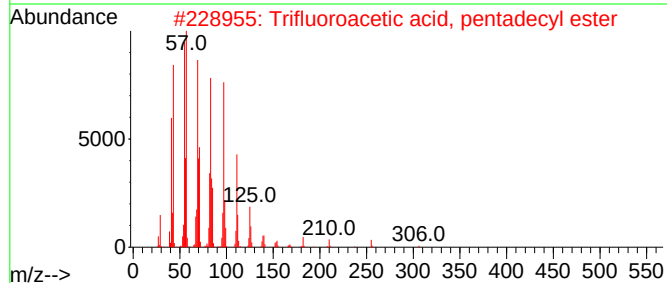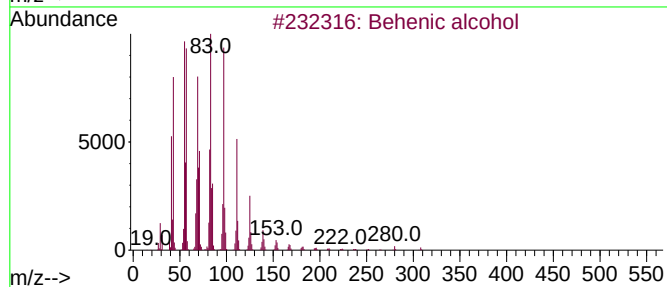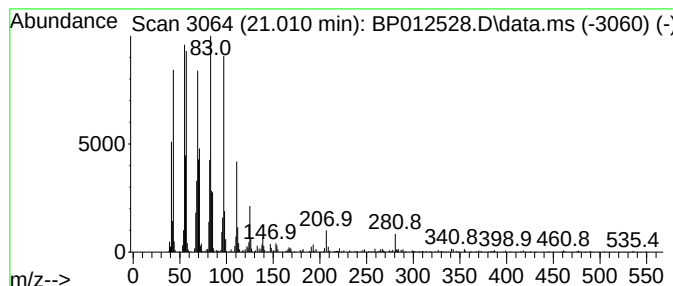

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110722\
Data File : BP012528.D
Acq On : 07 Nov 2022 13:15
Operator : CG/JU
Sample : N5353-10
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DBWU7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Behenic alcohol	21.010	2.3	ng/u1	717846	5	21.286	6282090	20.0