

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110722\
 Data File : BP012532.D
 Acq On : 07 Nov 2022 15:36
 Operator : CG/JU
 Sample : N5353-20
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DBXB3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
 Title : SVOA CALIBRATION

Signal : TIC: BP012532.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.234	38	42	54	rVB	64355	106680	1.05%	0.111%
2	3.658	112	114	132	rBV	312462	555903	5.48%	0.577%
3	3.864	145	149	156	rVB	21967	38251	0.38%	0.040%
4	3.964	162	166	170	rVB	28191	36787	0.36%	0.038%
5	4.270	214	218	222	rVB2	11404	13907	0.14%	0.014%
6	4.981	332	339	347	rBV4	17728	32462	0.32%	0.034%
7	5.093	355	358	365	rVB8	10990	17653	0.17%	0.018%
8	6.958	666	675	691	rBV	249437	461582	4.55%	0.479%
9	7.116	696	702	721	rVV	1136923	1824252	17.98%	1.894%
10	7.311	728	735	750	rBV	975621	1645072	16.21%	1.708%
11	7.775	804	814	824	rBV	1330604	2198178	21.66%	2.282%
12	7.875	829	831	840	rVB9	11904	27685	0.27%	0.029%
13	8.081	856	866	874	rBV2	26990	55754	0.55%	0.058%
14	8.446	918	928	930	rBV6	12369	21333	0.21%	0.022%
15	8.499	930	937	952	rBV	811273	1412890	13.93%	1.467%
16	8.946	1001	1013	1023	rBV	1335950	2321424	22.88%	2.410%
17	9.210	1053	1058	1067	rVB9	12074	27893	0.27%	0.029%
18	9.322	1071	1077	1083	rVB8	11125	23159	0.23%	0.024%
19	9.563	1112	1118	1123	rBV10	4333	10792	0.11%	0.011%
20	9.669	1127	1136	1149	rBV	1014495	1782810	17.57%	1.851%
21	9.775	1150	1154	1160	rVB7	9534	22749	0.22%	0.024%
22	9.963	1180	1186	1187	rBV6	8388	13755	0.14%	0.014%
23	9.993	1187	1191	1198	rVB2	24314	37027	0.36%	0.038%
24	10.146	1211	1217	1220	rBV2	14609	22021	0.22%	0.023%
25	10.205	1220	1227	1248	rVV	1549192	2781913	27.42%	2.888%
26	10.575	1283	1290	1305	rBV	2078161	3613843	35.62%	3.752%
27	10.728	1309	1316	1332	rBV	1384581	2667333	26.29%	2.769%
28	10.952	1349	1354	1364	rVB	26105	51367	0.51%	0.053%
29	11.163	1387	1390	1396	rVB8	5838	11374	0.11%	0.012%
30	11.816	1494	1501	1506	rVB10	8138	17889	0.18%	0.019%
31	11.928	1512	1520	1525	rBV10	4349	12418	0.12%	0.013%
32	11.993	1528	1531	1537	rVB8	8049	14432	0.14%	0.015%
33	12.099	1544	1549	1552	rBV6	5228	10655	0.11%	0.011%
34	12.175	1556	1562	1570	rBV3	27806	51552	0.51%	0.054%
35	12.246	1570	1574	1580	rVB7	17880	33878	0.33%	0.035%
36	12.328	1582	1588	1591	rBV7	10380	19810	0.20%	0.021%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110722\
 Data File : BP012532.D
 Acq On : 07 Nov 2022 15:36
 Operator : CG/JU
 Sample : N5353-20
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DBXB3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
 Title : SVOA CALIBRATION

37	12.716	1648	1654	1659	rBV9	7905	18861	0.19%	0.020%
38	12.775	1661	1664	1670	rVV7	6353	13099	0.13%	0.014%
39	12.893	1678	1684	1688	rBV6	10377	20711	0.20%	0.022%
40	12.969	1693	1697	1705	rVB2	18998	30006	0.30%	0.031%
41	13.157	1725	1729	1732	rBV5	8268	15577	0.15%	0.016%
42	13.204	1732	1737	1740	rBV4	14791	27196	0.27%	0.028%
43	13.322	1750	1757	1764	rVB3	37111	80206	0.79%	0.083%
44	13.410	1765	1772	1777	rBV6	14391	30859	0.30%	0.032%
45	13.845	1840	1846	1858	rBV	3563353	4995094	49.23%	5.186%
46	14.122	1885	1893	1908	rBV2	3822758	5905163	58.20%	6.131%
47	14.428	1939	1945	1957	rBV	3444464	5243291	51.68%	5.443%
48	14.522	1957	1961	1968	rVV6	20018	47196	0.47%	0.049%
49	14.675	1982	1987	1999	rBV	117502	314292	3.10%	0.326%
50	15.228	2078	2081	2083	rBV3	9755	11849	0.12%	0.012%
51	15.269	2084	2088	2095	rVB4	31995	57213	0.56%	0.059%
52	15.428	2107	2115	2132	rBV	5173623	7877297	77.64%	8.178%
53	15.563	2132	2138	2153	rVV	1631211	2383232	23.49%	2.474%
54	15.663	2153	2155	2167	rVB5	39544	83679	0.82%	0.087%
55	15.892	2192	2194	2198	rVB5	15114	20436	0.20%	0.021%
56	16.139	2233	2236	2243	rBV2	33980	52018	0.51%	0.054%
57	16.939	2368	2372	2375	rBV	33859	44225	0.44%	0.046%
58	17.192	2409	2415	2426	rBV	4369034	6334006	62.43%	6.576%
59	17.292	2426	2432	2455	rVB2	5987510	8908806	87.80%	9.249%
60	17.681	2496	2498	2502	rVB2	24157	21623	0.21%	0.022%
61	18.081	2562	2566	2576	rBV2	100394	171780	1.69%	0.178%
62	19.104	2738	2740	2747	rVB2	92405	129096	1.27%	0.134%
63	19.181	2749	2753	2758	rBV	80211	121808	1.20%	0.126%
64	19.316	2773	2776	2784	rBV2	97568	158229	1.56%	0.164%
65	19.533	2807	2813	2819	rBV	7438015	10146290	100.00%	10.534%
66	19.586	2819	2822	2831	rVB	270400	374596	3.69%	0.389%
67	21.286	3106	3111	3124	rBV	4554505	6024387	59.38%	6.254%
68	21.598	3160	3164	3174	rBV	772010	1042196	10.27%	1.082%
69	23.516	3483	3490	3507	rVB2	3907090	8260382	81.41%	8.576%
70	23.668	3510	3516	3534	rVB2	2560904	5360991	52.84%	5.566%




Sum of corrected areas: 96322173

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110722\
Data File : BP012532.D
Acq On : 07 Nov 2022 15:36
Operator : CG/JU
Sample : N5353-20
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DBXB3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

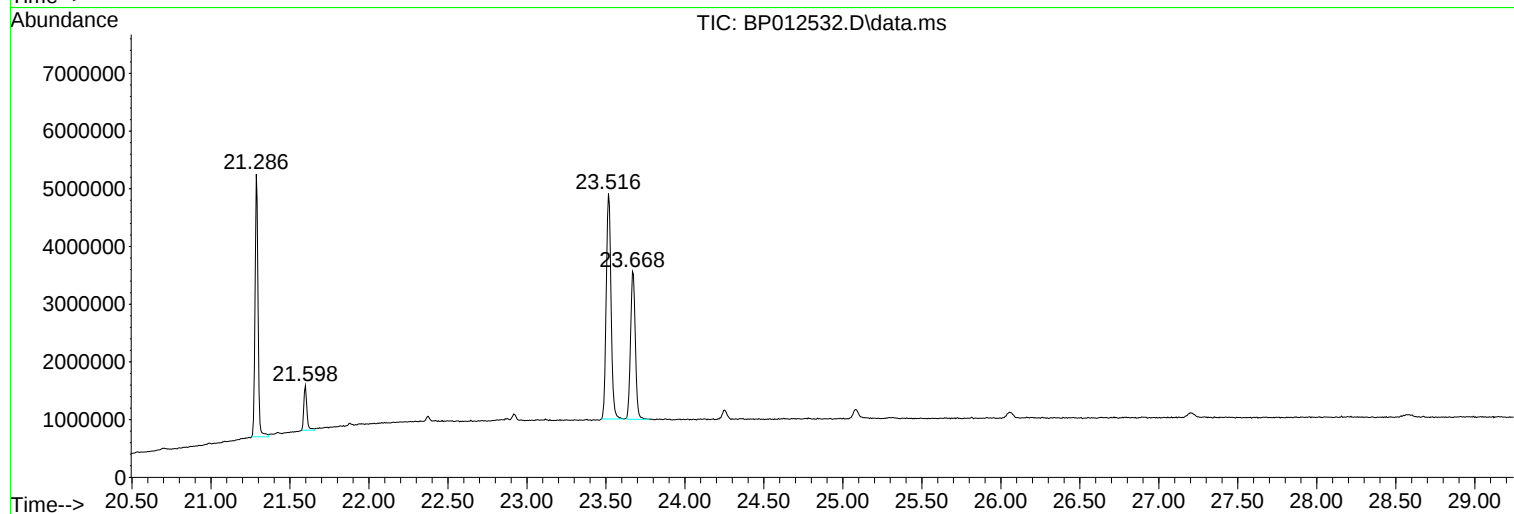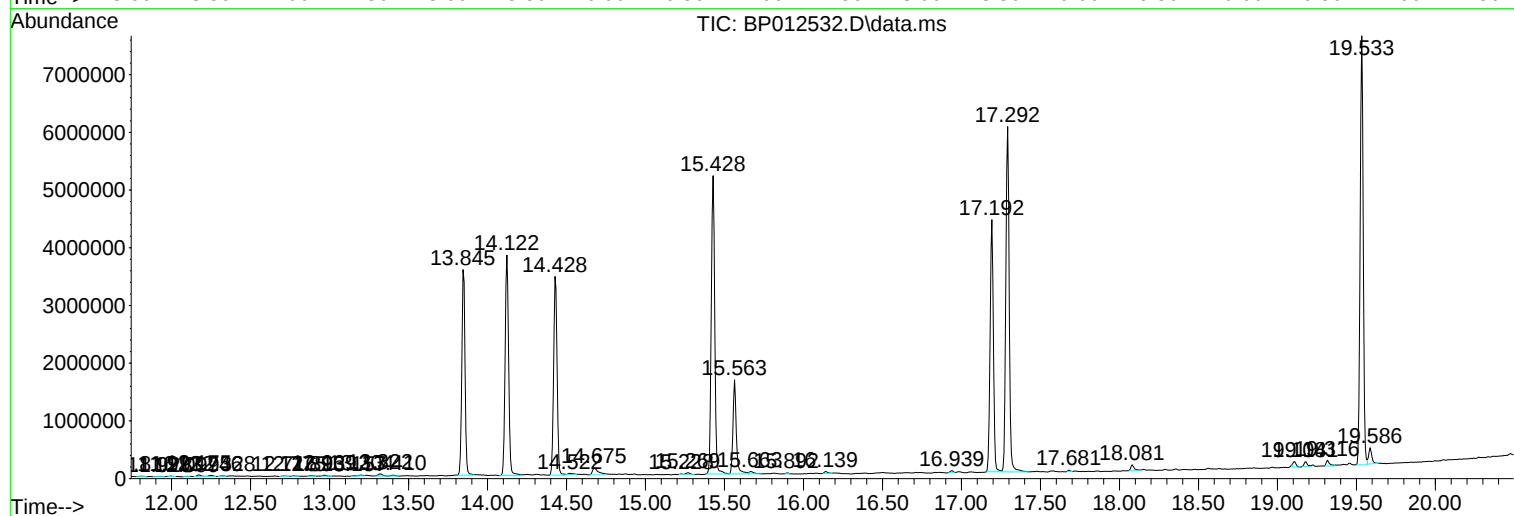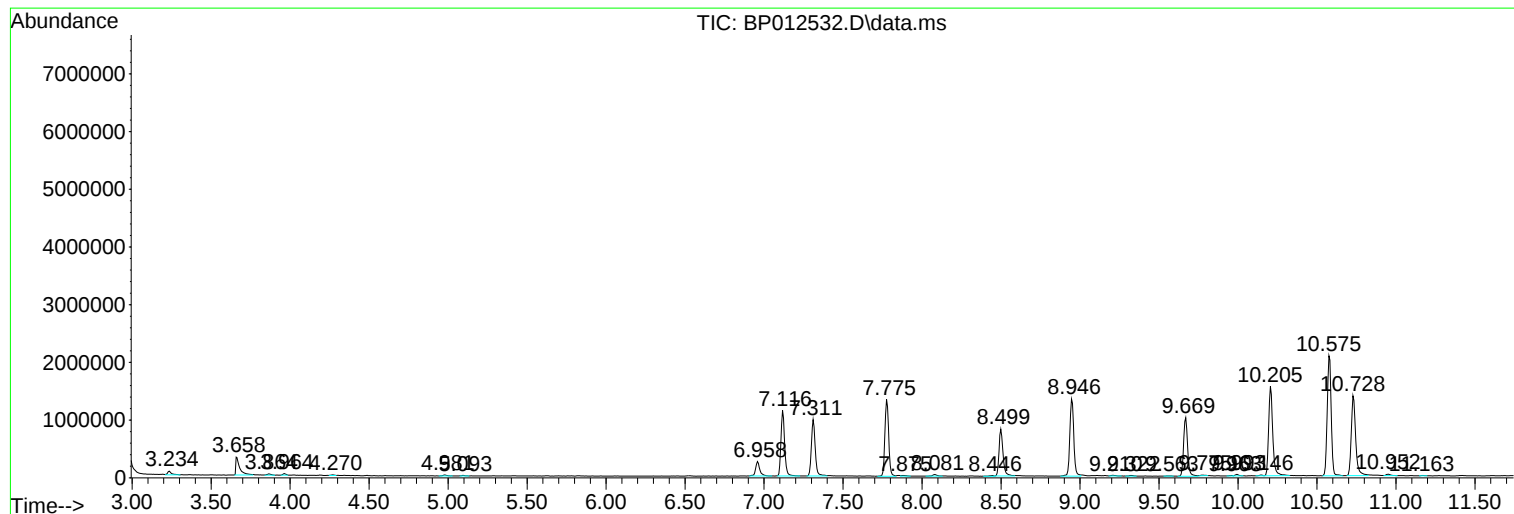

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110722\
Data File : BP012532.D
Acq On : 07 Nov 2022 15:36
Operator : CG/JU
Sample : N5353-20
Misc :
ALS Vial : 9 Sample Multiplier: 1










Instrument :
BNA_P
ClientSampleId :
DBXB3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 2-((2H-benzotriazo)-2-yl)-4... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.	
21.598	3.46 ng/ul	1042200	Chrysene-d12	21.286	
Hit# of 5	Tentative ID	MW	MolForm	CAS#	Qual
1	2-((2H-benzotriazo)-2-yl)-4-(1,1...	323	C20H25N3O	003147-75-9	97
2	5-Methoxyflavone	252	C16H12O3	042079-78-7	87
3	2-((2H-benzotriazo)-2-yl)-4-(1,1...	323	C20H25N3O	003147-75-9	83
4	Benzo[a]pyrene	252	C20H12	000050-32-8	72
5	Benzo[e]pyrene	252	C20H12	000192-97-2	72

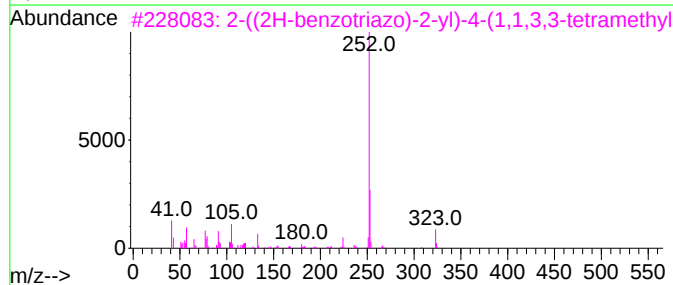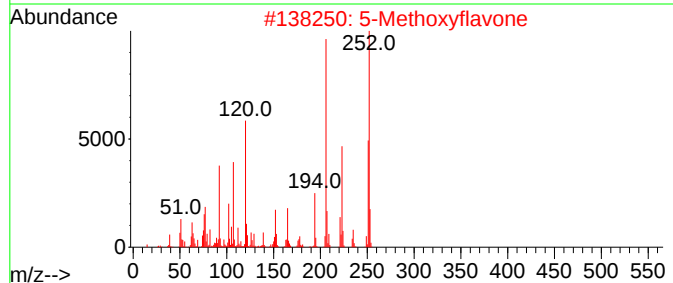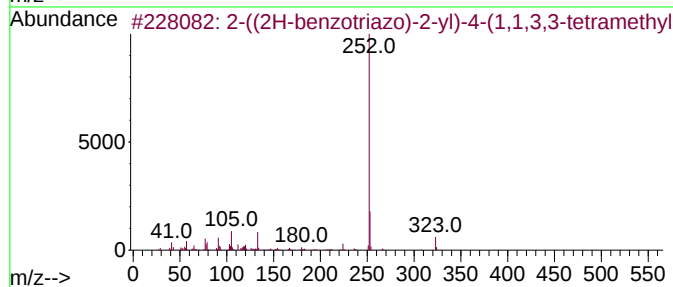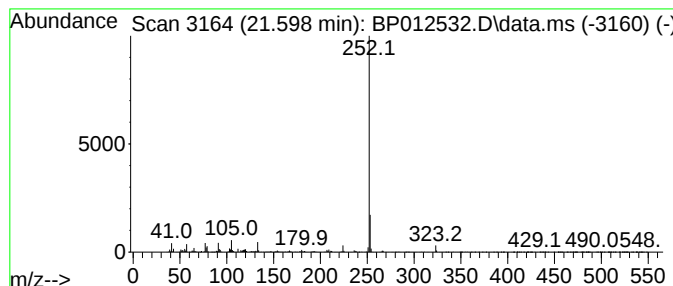

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110722\
Data File : BP012532.D
Acq On : 07 Nov 2022 15:36
Operator : CG/JU
Sample : N5353-20
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DBXB3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
2-((2H-benzotri...	21.598	3.5	ng/u1	1042200	5	21.286	6024390	20.0