

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110722\
 Data File : BP012533.D
 Acq On : 07 Nov 2022 16:11
 Operator : CG/JU
 Sample : N5353-12
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DBVV2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
 Title : SVOA CALIBRATION

Signal : TIC: BP012533.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.193	30	35	57	rVB	2920998	4759947	65.01%	6.208%
2	3.664	112	115	130	rBV	165321	318203	4.35%	0.415%
3	3.864	145	149	155	rVB	19029	32734	0.45%	0.043%
4	3.964	162	166	171	rBV	21832	36580	0.50%	0.048%
5	4.023	172	176	182	rVB	12533	19633	0.27%	0.026%
6	4.122	191	193	199	rVB7	6433	10846	0.15%	0.014%
7	4.487	248	255	266	rVB	266761	424173	5.79%	0.553%
8	6.958	670	675	691	rBV	178177	346635	4.73%	0.452%
9	7.116	694	702	719	rBV	728788	1233378	16.85%	1.609%
10	7.311	729	735	745	rBV	697020	1149434	15.70%	1.499%
11	7.658	791	794	799	rBV7	4655	7814	0.11%	0.010%
12	7.775	807	814	830	rBV	1018349	1707923	23.33%	2.227%
13	7.881	830	832	839	rVB7	8196	12525	0.17%	0.016%
14	8.128	869	874	882	rVB	56934	97553	1.33%	0.127%
15	8.499	930	937	957	rBV	572473	1063509	14.53%	1.387%
16	8.946	1007	1013	1033	rBV	890433	1567436	21.41%	2.044%
17	9.116	1036	1042	1045	rVV7	5546	12157	0.17%	0.016%
18	9.322	1069	1077	1088	rVB3	21337	43390	0.59%	0.057%
19	9.669	1128	1136	1151	rBV	716161	1248326	17.05%	1.628%
20	10.205	1218	1227	1244	rBV	1025452	1983487	27.09%	2.587%
21	10.393	1252	1259	1279	rVB2	31327	115433	1.58%	0.151%
22	10.575	1283	1290	1306	rVB	1656078	2858097	39.04%	3.728%
23	10.728	1309	1316	1329	rBV	954394	1868994	25.53%	2.438%
24	11.422	1425	1434	1436	rBV9	6319	13855	0.19%	0.018%
25	11.828	1497	1503	1505	rBV5	5468	9528	0.13%	0.012%
26	12.175	1557	1562	1569	rBV4	15999	33420	0.46%	0.044%
27	12.257	1572	1576	1582	rVB9	7367	14280	0.20%	0.019%
28	12.328	1582	1588	1593	rBV9	4768	11084	0.15%	0.014%
29	12.781	1661	1665	1668	rBV6	5493	9316	0.13%	0.012%
30	13.040	1705	1709	1715	rBV8	5772	11421	0.16%	0.015%
31	13.240	1739	1743	1748	rVB5	6634	10481	0.14%	0.014%
32	13.322	1752	1757	1762	rVB3	14379	23417	0.32%	0.031%
33	13.398	1766	1770	1776	rBV7	6725	12246	0.17%	0.016%
34	13.681	1811	1818	1821	rBV9	6649	12885	0.18%	0.017%
35	13.846	1837	1846	1860	rBV	2322926	3388340	46.28%	4.419%
36	14.122	1886	1893	1909	rBV	2723980	4075724	55.67%	5.316%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110722\
 Data File : BP012533.D
 Acq On : 07 Nov 2022 16:11
 Operator : CG/JU
 Sample : N5353-12
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DBWV2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
 Title : SVOA CALIBRATION

37	14.428	1938	1945	1960	rBV	2821872	4225503	57.72%	5.511%
38	14.687	1983	1989	2007	rBV3	63976	222192	3.03%	0.290%
39	15.263	2084	2087	2094	rVB7	9352	15397	0.21%	0.020%
40	15.428	2108	2115	2133	rBV	3640310	5407696	73.86%	7.053%
41	15.563	2133	2138	2151	rVV	988766	1484910	20.28%	1.937%
42	15.663	2153	2155	2164	rVB5	24929	46792	0.64%	0.061%
43	17.192	2408	2415	2425	rBV	3608206	5331155	72.82%	6.953%
44	17.292	2426	2432	2451	rVB2	3980610	6199832	84.68%	8.086%
45	17.863	2525	2529	2534	rBV	56163	72051	0.98%	0.094%
46	18.081	2562	2566	2573	rBV	130894	205732	2.81%	0.268%
47	18.998	2718	2722	2725	rBV	84462	98027	1.34%	0.128%
48	19.110	2738	2741	2747	rVB3	66298	85582	1.17%	0.112%
49	19.181	2749	2753	2756	rBV	64802	90984	1.24%	0.119%
50	19.316	2773	2776	2786	rBV2	131862	225694	3.08%	0.294%
51	19.533	2807	2813	2819	rBV	5401016	7321323	100.00%	9.549%
52	19.586	2819	2822	2829	rVB	264140	368549	5.03%	0.481%
53	21.286	3106	3111	3124	rBV	4293997	5603892	76.54%	7.309%
54	23.516	3483	3490	3506	rBV2	3061768	6332099	86.49%	8.258%
55	23.669	3510	3516	3526	rVB2	2294046	4793054	65.47%	6.251%




Sum of corrected areas: 76674668

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110722\
Data File : BP012533.D
Acq On : 07 Nov 2022 16:11
Operator : CG/JU
Sample : N5353-12
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DBWV2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

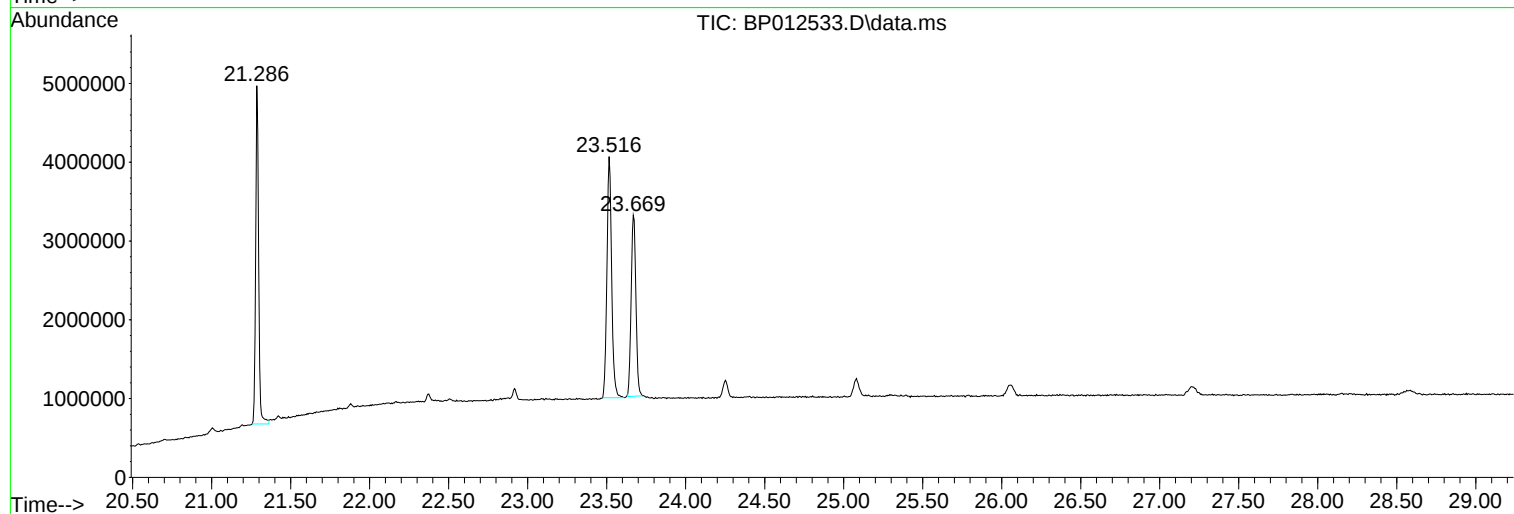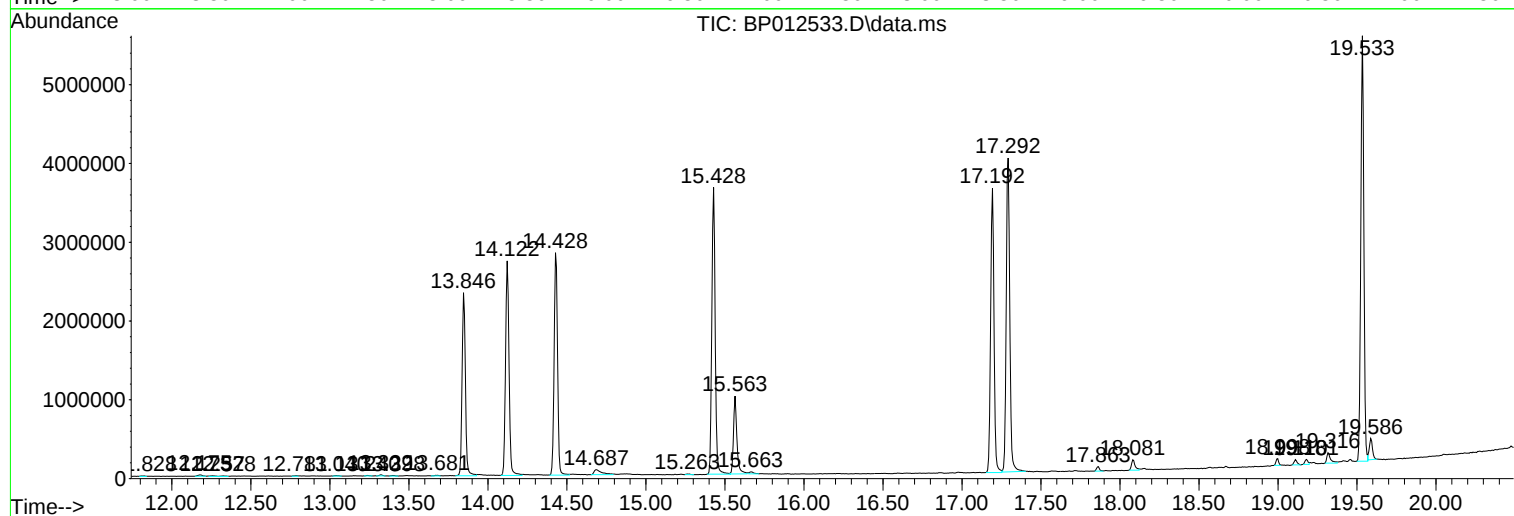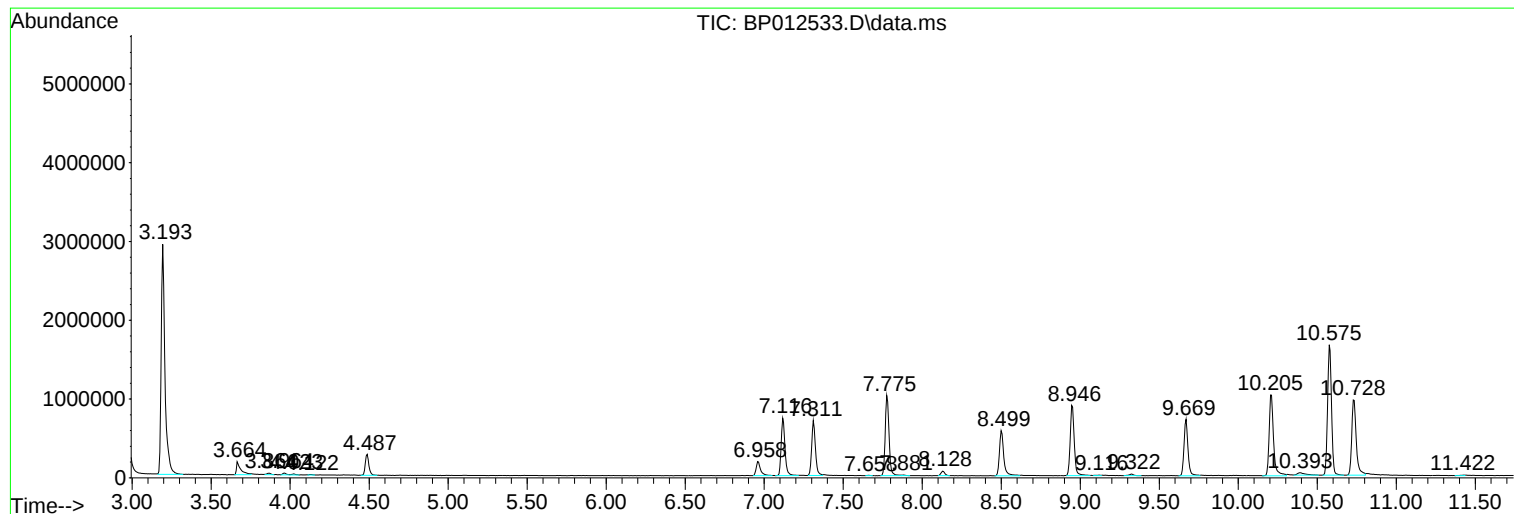

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110722\
Data File : BP012533.D
Acq On : 07 Nov 2022 16:11
Operator : CG/JU
Sample : N5353-12
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DBVV2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110722\
Data File : BP012533.D
Acq On : 07 Nov 2022 16:11
Operator : CG/JU
Sample : N5353-12
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DBVV2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------