

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110722\
 Data File : BP012537.D
 Acq On : 07 Nov 2022 18:32
 Operator : CG/JU
 Sample : N5353-09
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DBWR9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
 Title : SVOA CALIBRATION

Signal : TIC: BP012537.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.228	37	41	54	rVB	42736	76721	0.98%	0.106%
2	3.664	113	115	139	rBV	124061	281127	3.57%	0.388%
3	3.864	145	149	154	rVB3	14572	23752	0.30%	0.033%
4	3.958	162	165	175	rVB	19169	30124	0.38%	0.042%
5	5.093	350	358	366	rBV	65509	117673	1.50%	0.163%
6	6.881	657	662	669	rBV7	5066	10127	0.13%	0.014%
7	6.958	669	675	686	rBV	150639	316005	4.02%	0.436%
8	7.116	696	702	721	rBV	731891	1226807	15.60%	1.694%
9	7.311	728	735	752	rBV	642011	1105392	14.05%	1.527%
10	7.775	805	814	825	rBV	1017204	1694523	21.54%	2.340%
11	8.134	868	875	882	rBV4	13151	27148	0.35%	0.037%
12	8.499	927	937	960	rBV	519072	990373	12.59%	1.368%
13	8.669	962	966	975	rVB	4500	14189	0.18%	0.020%
14	8.946	1006	1013	1028	rBV	901240	1569991	19.96%	2.168%
15	9.046	1028	1030	1035	rVB6	5749	8763	0.11%	0.012%
16	9.157	1046	1049	1054	rVB7	10399	16666	0.21%	0.023%
17	9.293	1067	1072	1074	rBV5	13305	21251	0.27%	0.029%
18	9.322	1074	1077	1088	rVB2	18740	37186	0.47%	0.051%
19	9.510	1103	1109	1115	rBV2	4124	8913	0.11%	0.012%
20	9.604	1120	1125	1129	rBV5	9151	16360	0.21%	0.023%
21	9.663	1129	1135	1150	rVV	656993	1188516	15.11%	1.641%
22	9.946	1178	1183	1187	rBV8	6420	11942	0.15%	0.016%
23	10.204	1220	1227	1247	rBV	1024856	1992254	25.33%	2.752%
24	10.434	1260	1266	1272	rVB	7935	20051	0.25%	0.028%
25	10.575	1282	1290	1308	rBV	1629900	2821161	35.87%	3.896%
26	10.728	1308	1316	1330	rBV	929763	1791739	22.78%	2.475%
27	10.840	1330	1335	1346	rVB	40995	94024	1.20%	0.130%
28	11.451	1434	1439	1441	rBV5	5569	8165	0.10%	0.011%
29	11.528	1446	1452	1458	rVB5	6818	14131	0.18%	0.020%
30	11.616	1463	1467	1470	rVV6	6859	12102	0.15%	0.017%
31	11.646	1470	1472	1478	rVB7	5555	9387	0.12%	0.013%
32	11.834	1495	1504	1510	rVB	43013	80022	1.02%	0.111%
33	12.034	1533	1538	1543	rVB2	9643	14772	0.19%	0.020%
34	12.175	1554	1562	1568	rBV3	15046	37226	0.47%	0.051%
35	12.251	1571	1575	1583	rVV7	14369	30302	0.39%	0.042%
36	12.334	1583	1589	1594	rVB9	10354	17791	0.23%	0.025%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110722\
 Data File : BP012537.D
 Acq On : 07 Nov 2022 18:32
 Operator : CG/JU
 Sample : N5353-09
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DBWR9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
 Title : SVOA CALIBRATION

37	12.498	1608	1617	1626	rBV6	16396	43104	0.55%	0.060%
38	12.598	1629	1634	1639	rBV8	10539	18137	0.23%	0.025%
39	12.669	1639	1646	1651	rVB10	8282	15514	0.20%	0.021%
40	12.781	1661	1665	1667	rBV5	6084	9623	0.12%	0.013%
41	12.951	1689	1694	1699	rBV2	22731	37911	0.48%	0.052%
42	13.151	1725	1728	1732	rBV5	6222	8094	0.10%	0.011%
43	13.234	1739	1742	1748	rBV3	12324	17079	0.22%	0.024%
44	13.322	1752	1757	1763	rBV5	10216	15987	0.20%	0.022%
45	13.393	1765	1769	1772	rBV5	9871	19466	0.25%	0.027%
46	13.434	1772	1776	1781	rVB5	15307	25107	0.32%	0.035%
47	13.845	1837	1846	1857	rBV	2371345	3453136	43.90%	4.769%
48	14.045	1878	1880	1885	rVB6	6277	9426	0.12%	0.013%
49	14.122	1886	1893	1911	rBV	2588024	4021511	51.13%	5.554%
50	14.428	1938	1945	1960	rBV	2748647	4180540	53.15%	5.774%
51	14.692	1984	1990	2002	rBV4	55853	189120	2.40%	0.261%
52	14.792	2003	2007	2014	rVB	33847	61007	0.78%	0.084%
53	14.969	2033	2037	2045	rVB6	32204	54129	0.69%	0.075%
54	15.040	2045	2049	2055	rBV9	13915	24522	0.31%	0.034%
55	15.275	2084	2089	2095	rVB7	13389	25001	0.32%	0.035%
56	15.428	2108	2115	2132	rBV	3530921	5410304	68.79%	7.472%
57	15.563	2132	2138	2151	rBV	959411	1454477	18.49%	2.009%
58	15.881	2189	2192	2200	rVB4	19774	30294	0.39%	0.042%
59	16.586	2308	2312	2319	rBV10	18755	49781	0.63%	0.069%
60	16.975	2375	2378	2384	rVB6	23300	35814	0.46%	0.049%
61	17.192	2408	2415	2425	rBV	3548925	5349401	68.01%	7.388%
62	17.292	2425	2432	2454	rVB	4175802	6497846	82.61%	8.974%
63	18.081	2562	2566	2575	rBV2	193634	328430	4.18%	0.454%
64	19.110	2737	2741	2744	rBV2	63179	87412	1.11%	0.121%
65	19.180	2749	2753	2756	rBV	66048	102029	1.30%	0.141%
66	19.316	2772	2776	2783	rBV	146425	231024	2.94%	0.319%
67	19.533	2807	2813	2824	rBV	5629185	7865448	100.00%	10.863%
68	21.286	3106	3111	3122	rBV	4335366	5539107	70.42%	7.650%
69	23.510	3483	3489	3502	rVB2	3048497	6591879	83.81%	9.104%
70	23.668	3509	3516	3526	rVB2	2361050	4866854	61.88%	6.722%




Sum of corrected areas: 72405190

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110722\
Data File : BP012537.D
Acq On : 07 Nov 2022 18:32
Operator : CG/JU
Sample : N5353-09
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DBWR9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

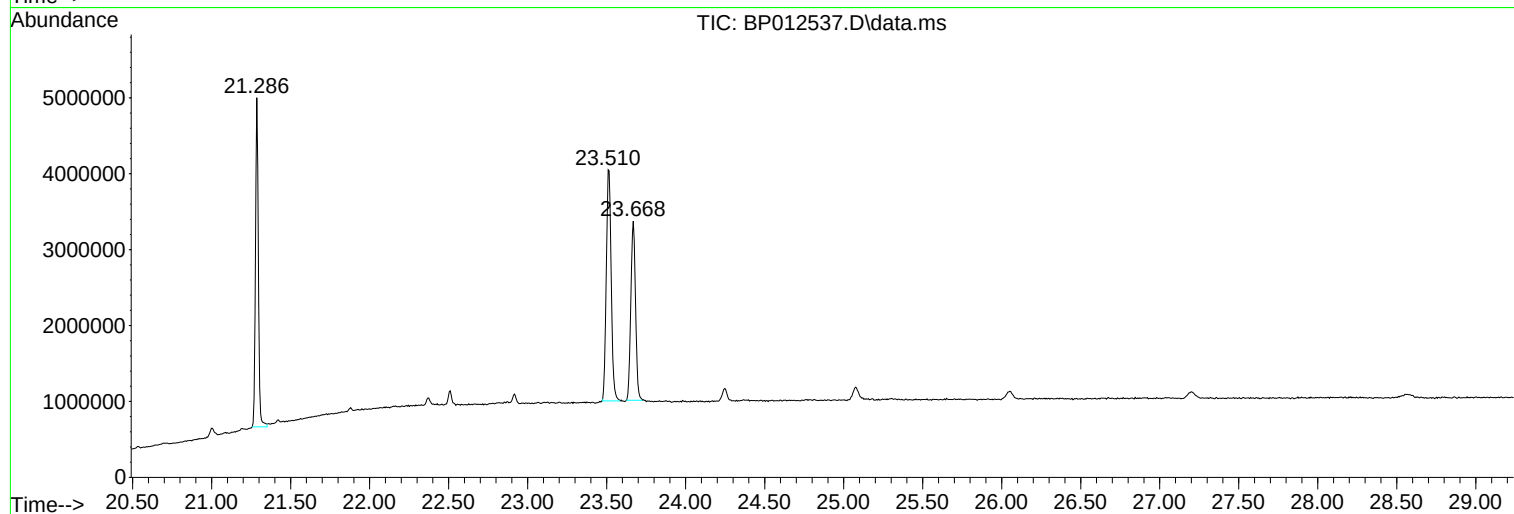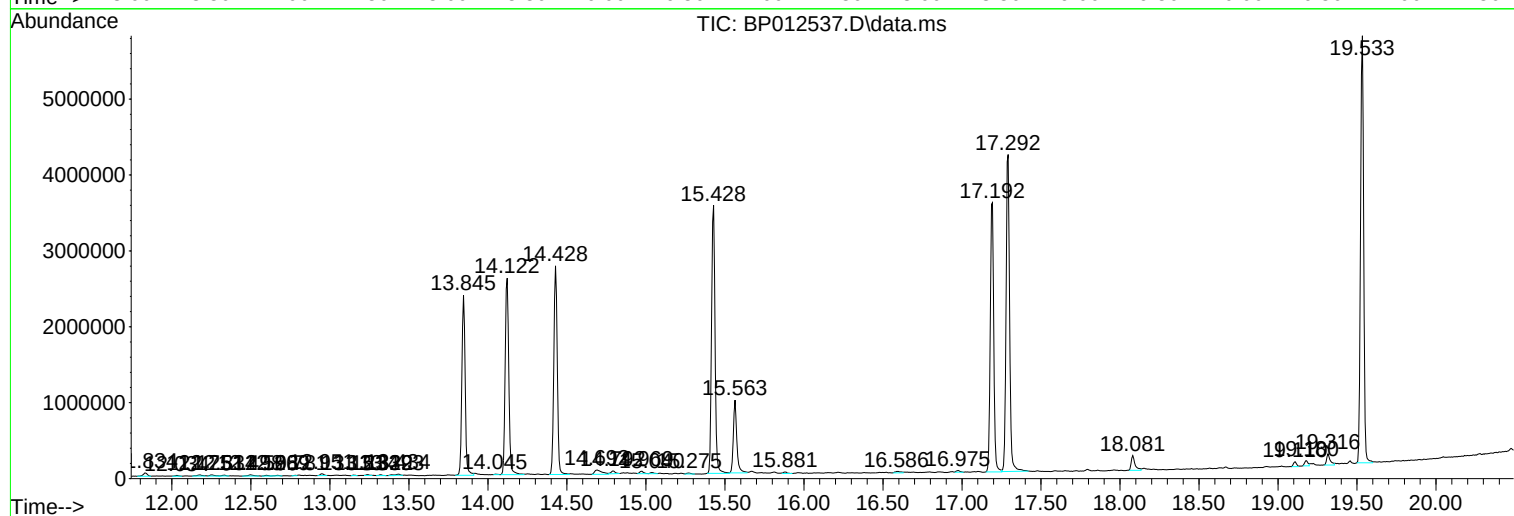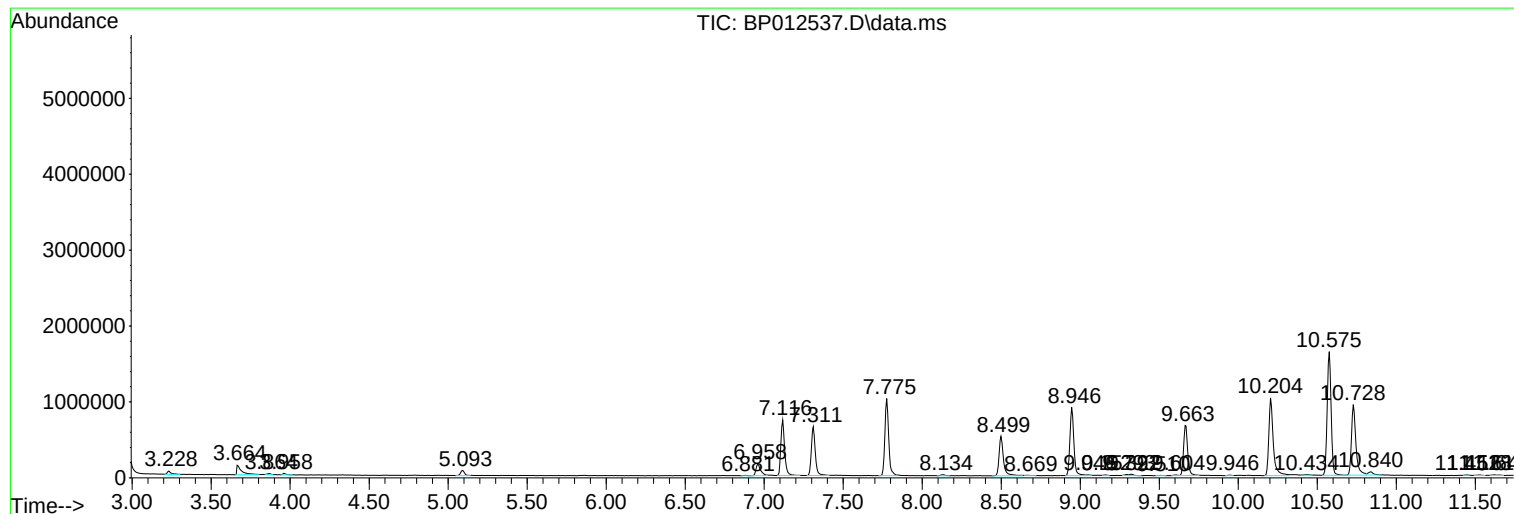

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110722\
Data File : BP012537.D
Acq On : 07 Nov 2022 18:32
Operator : CG/JU
Sample : N5353-09
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DBWR9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110722\
Data File : BP012537.D
Acq On : 07 Nov 2022 18:32
Operator : CG/JU
Sample : N5353-09
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DBWR9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc