
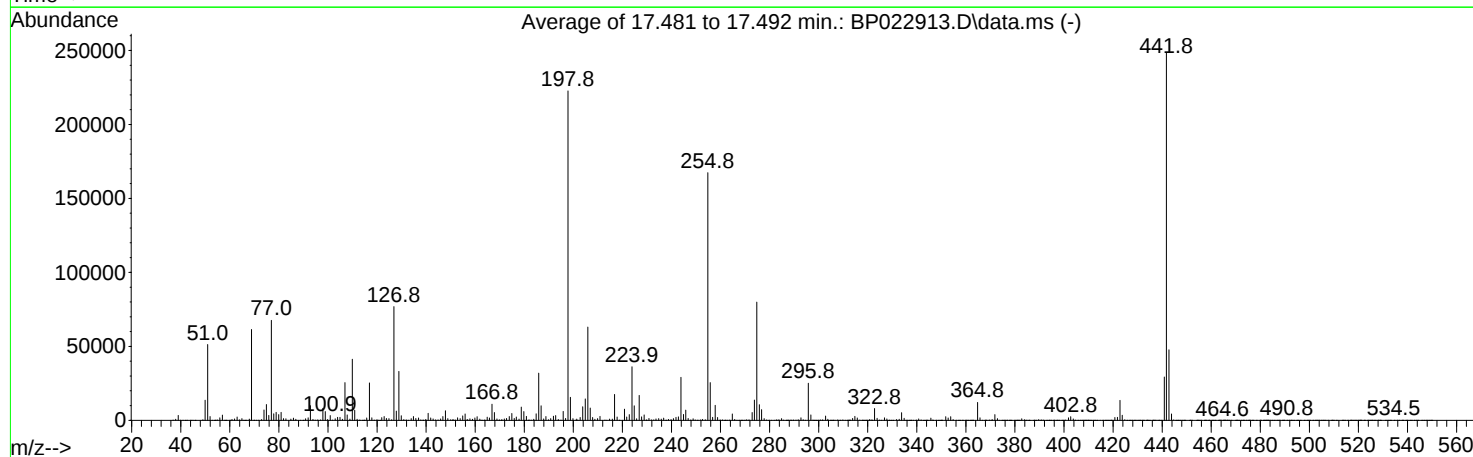


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110724\
Data File : BP022913.D
Acq On : 07 Nov 2024 11:06
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP110724.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Nov 07 23:36:11 2024

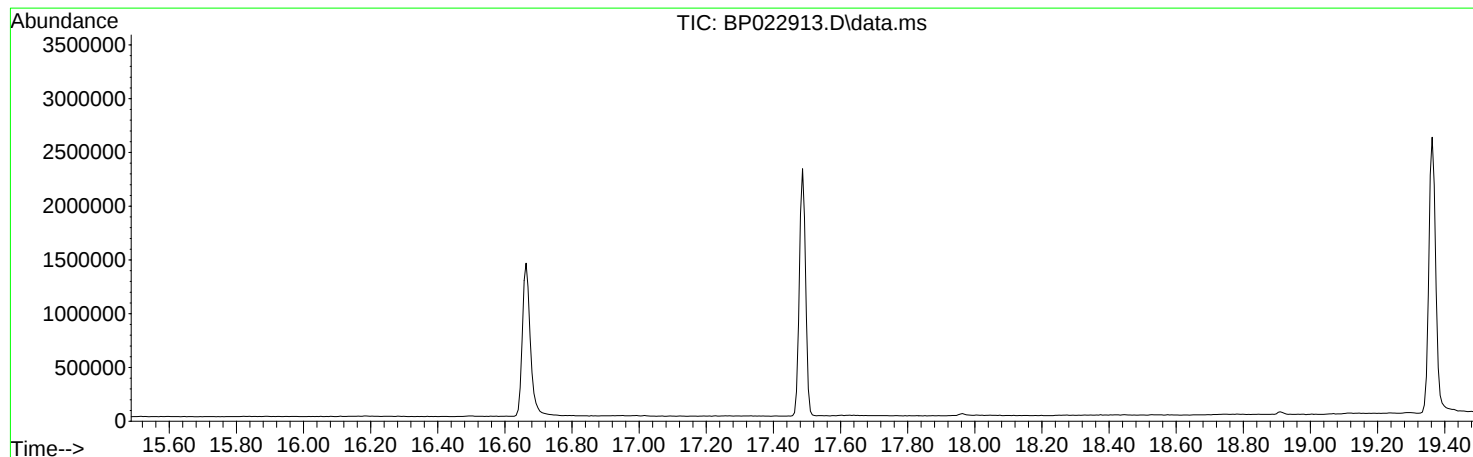




AutoFind: Scans 2464, 2465, 2466; Background Corrected with Scan 2455

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	23.0	51279	PASS
68	69	0.00	2	1.4	866	PASS
69	198	0.00	100	27.6	61439	PASS
70	69	0.00	2	0.3	162	PASS
127	198	10	80	34.5	76868	PASS
197	198	0.00	2	0.6	1341	PASS
198	198	100	100	100.0	222635	PASS
199	198	5	9	7.0	15627	PASS
275	198	10	60	35.9	79909	PASS
365	198	1	100	5.5	12171	PASS
441	198	0.01	100	13.2	29320	PASS
442	442	100	100	100.0	248617	PASS
443	442	15	24	19.2	47659	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110724\
Data File : BP022913.D
Acq On : 07 Nov 2024 11:06
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Nov 08 02:41:03 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP110724.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 07 23:36:11 2024
Response via : Initial Calibration

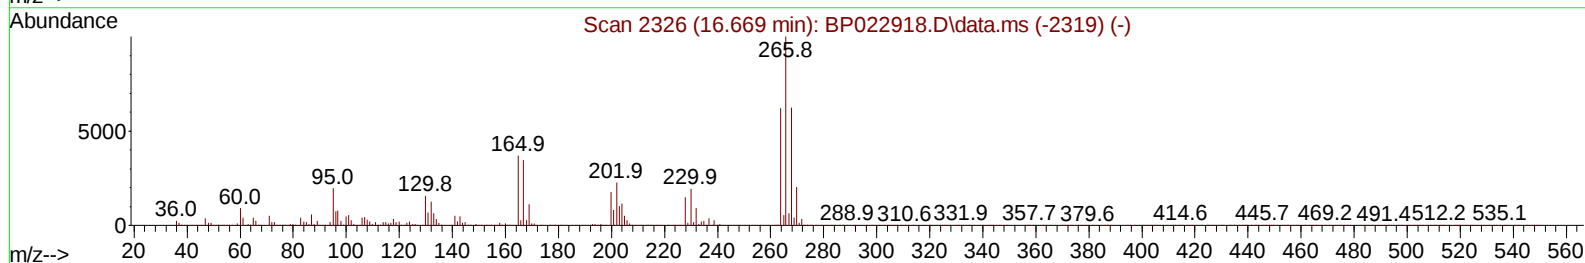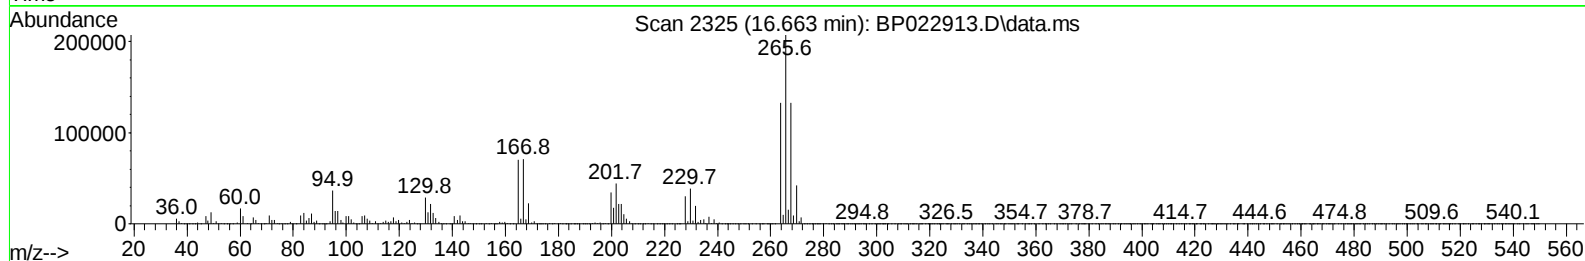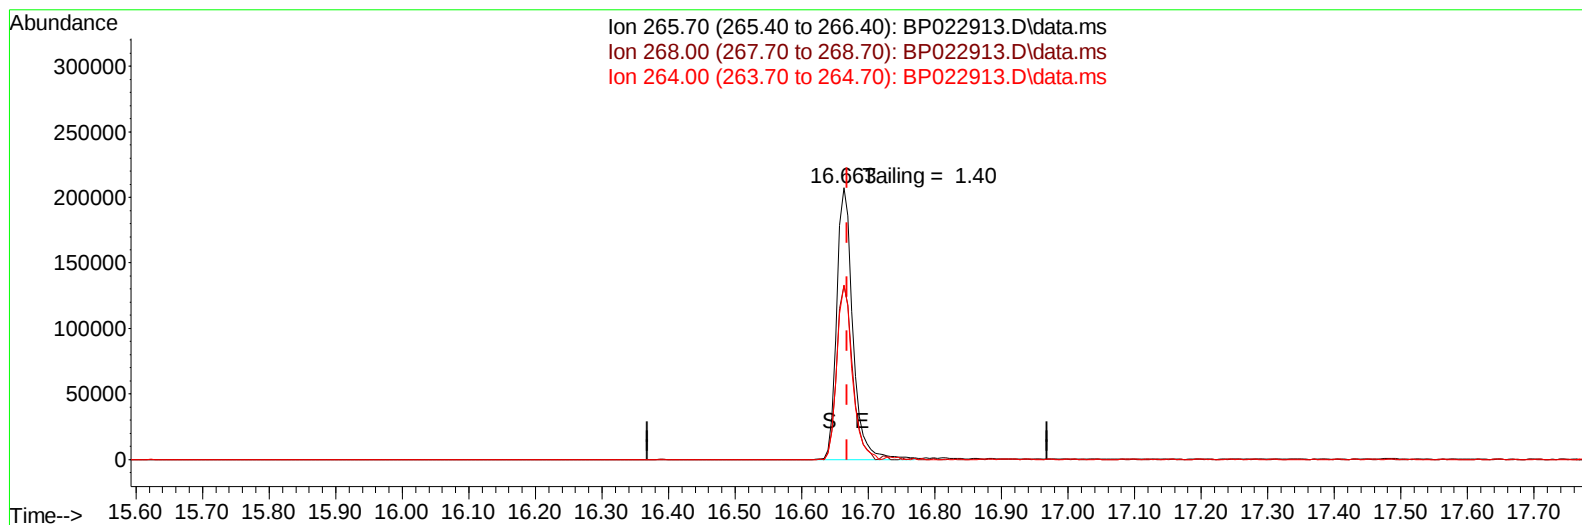

TIC: BP022913.D\data.ms

(70) Pentachlorophenol (C)

16.663min (-0.006) 1173465.20 ng




response 345390

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.40	68.49
264.00	62.10	68.98
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110724\
Data File : BP022913.D
Acq On : 07 Nov 2024 11:06
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Nov 08 02:41:03 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP110724.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 07 23:36:11 2024
Response via : Initial Calibration

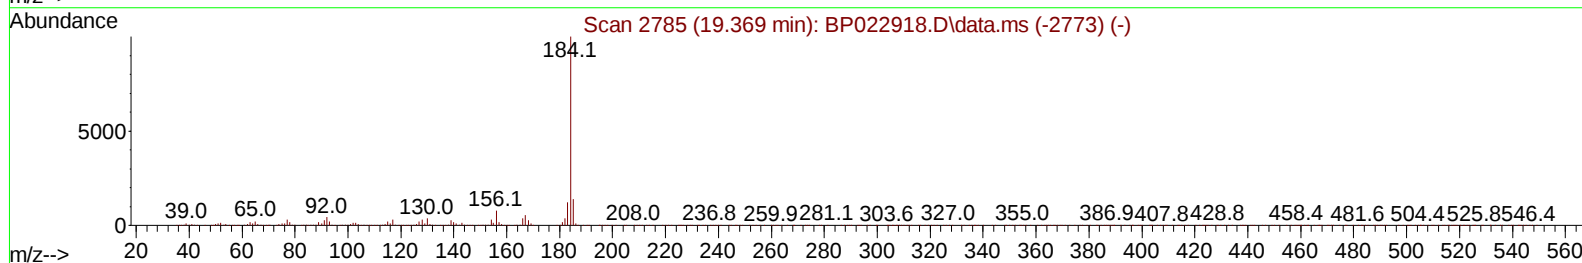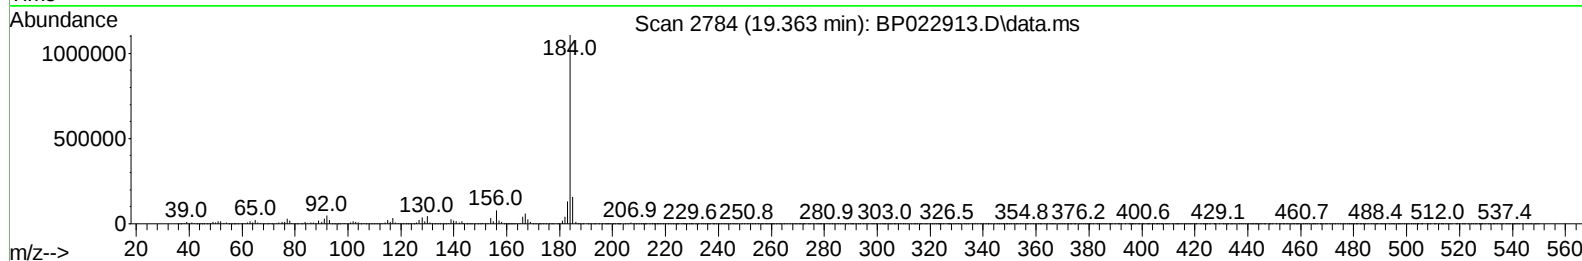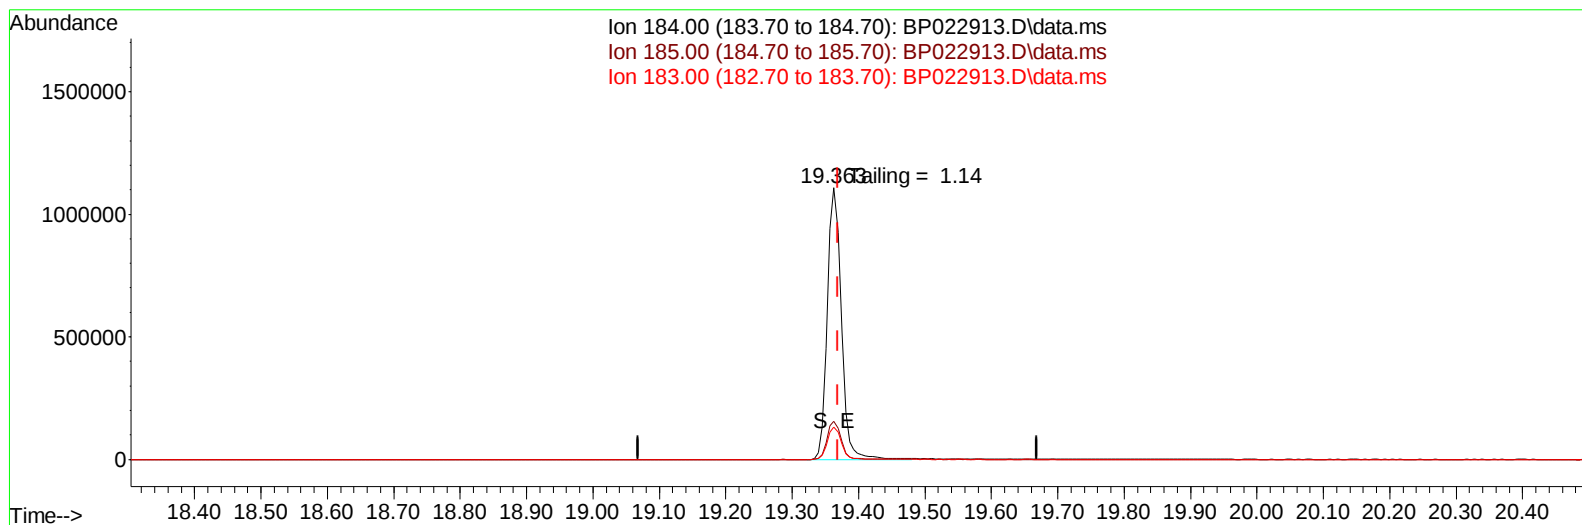

TIC: BP022913.D\data.ms

(77) Benzidine

19.363min (-0.006) 990982.71 ng

response 1605571

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.10	14.09
183.00	12.10	11.97
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
11/7/2024	BNA_P	<u>BP022913.D</u>
Compound Name	Response	Retention Time
DDT	872211	20.657
DDD	22121	20.198
DDE	1008	19.657
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
23129	895340	2.58

Instrument :
BNA_P
ClientSampleId :
DFTPP