




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110822\
 Data File : BP012549.D
 Acq On : 08 Nov 2022 12:56
 Operator : CG/JU
 Sample : N5407-06
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EW4Y6

Manual IntegrationsAPPROVED

Quant Time: Nov 08 21:41:17 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Nov 04 02:53:36 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 11/09/2022
 Supervised By :mohammad ahmed 11/14/2022

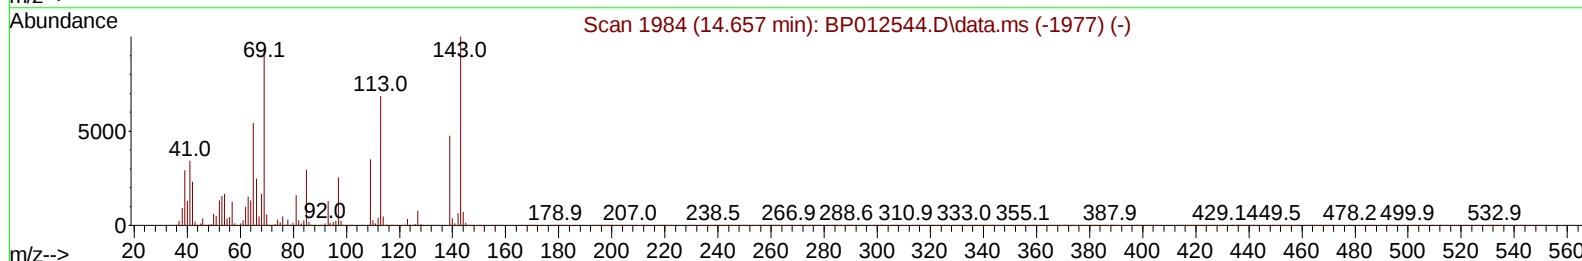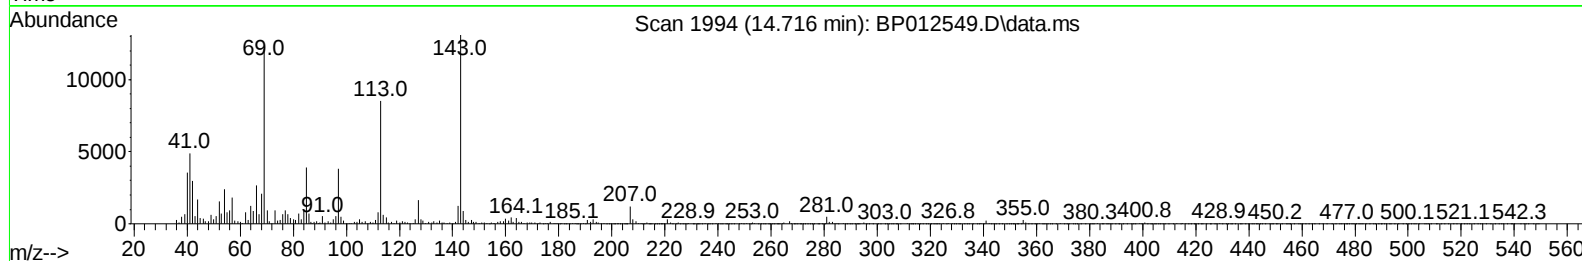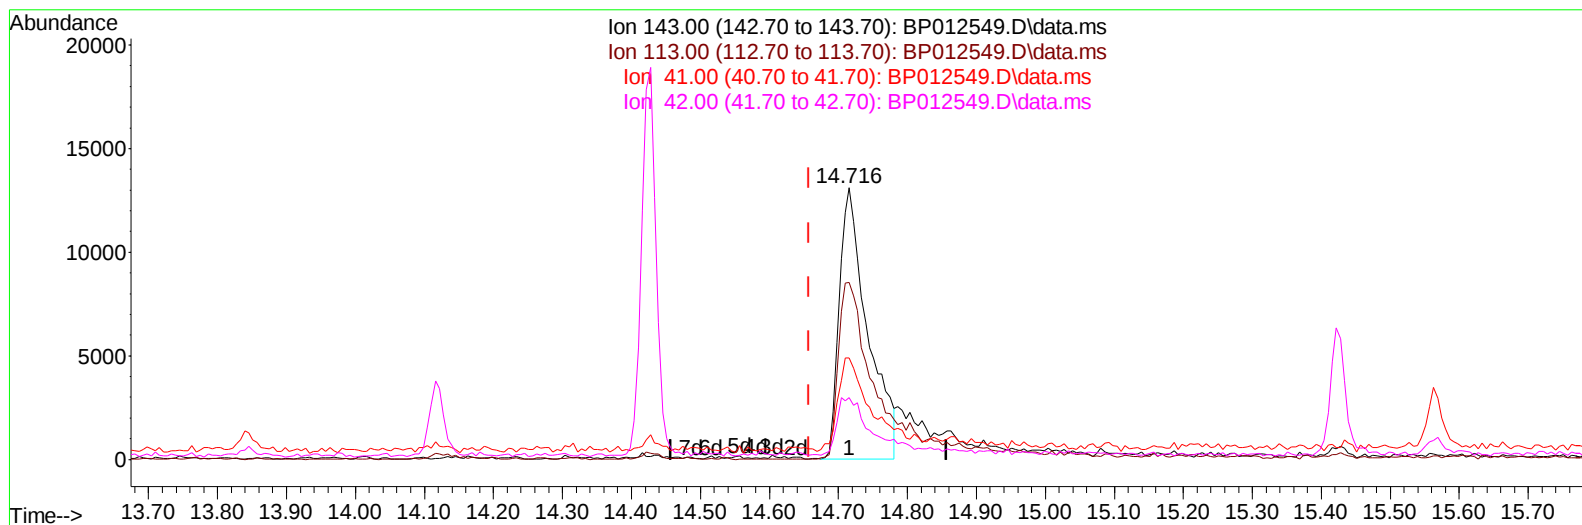

TIC: BP012549.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.716min (+ 0.059) 2.43 ng/u1

response 37314

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	65.10	65.21
41.00	34.50	37.40
42.00	23.60	22.83




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110822\
 Data File : BP012549.D
 Acq On : 08 Nov 2022 12:56
 Operator : CG/JU
 Sample : N5407-06
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EW4Y6

Manual IntegrationsAPPROVED

Quant Time: Nov 08 21:41:17 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Nov 04 02:53:36 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 11/09/2022
 Supervised By :mohammad ahmed 11/14/2022

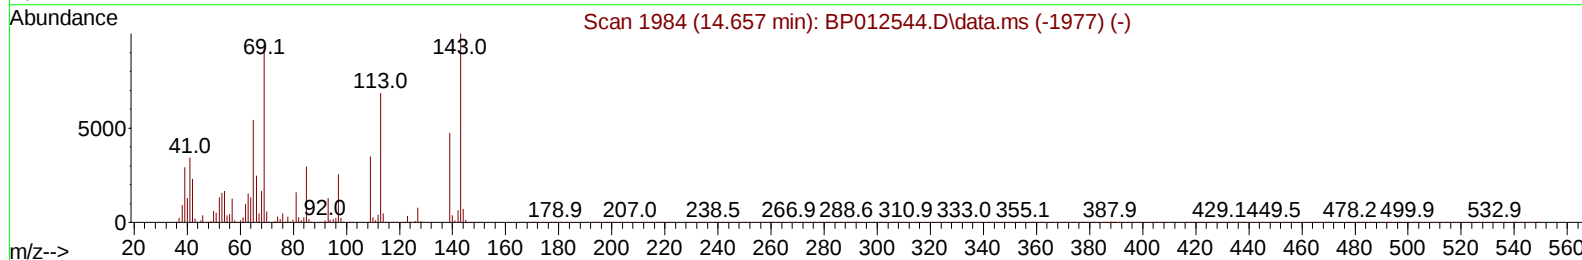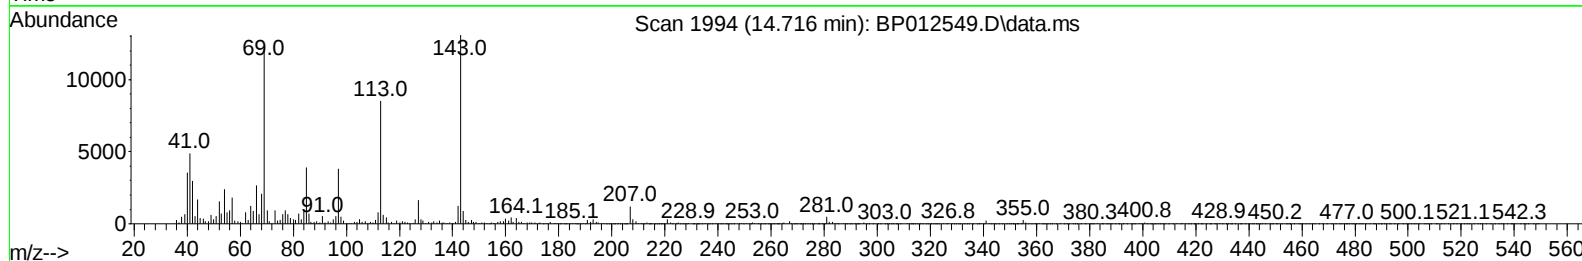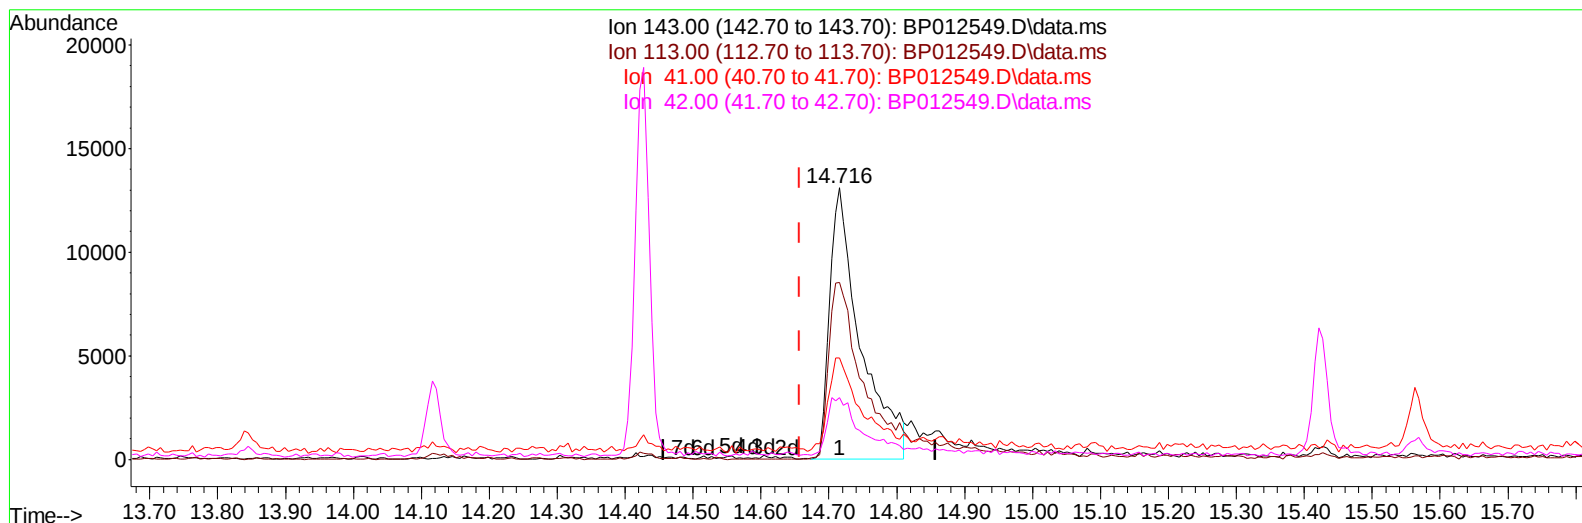

TIC: BP012549.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.716min (+ 0.059) 2.69 ng/ul m

response 41241

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	65.10	65.21
41.00	34.50	37.40
42.00	23.60	22.83

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110822\
 Data File : BP012549.D
 Acq On : 08 Nov 2022 12:56
 Operator : CG/JU
 Sample : N5407-06
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EW4Y6

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 11/09/2022
 Supervised By :mohammad ahmed 11/14/2022

Quant Time: Nov 08 21:41:17 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Nov 04 02:53:36 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.775	152	327934	20.000	ng/ul	0.00
20) Naphthalene-d8	10.575	136	1628398	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.428	164	1185280	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.192	188	2674284	20.000	ng/ul	0.00
79) Chrysene-d12	21.286	240	2532452	20.000	ng/ul	0.00
88) Perylene-d12	23.668	264	2335755	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.228	96	19176	2.355	ng/uL	0.00
4) Pyridine-d5	3.663	84	81909	3.501	ng/ul	0.01
7) Phenol-d5	6.969	99	136486	4.640	ng/ul	0.01
9) Bis-(2-Chloroethyl)eth...	7.116	67	90411	5.149	ng/ul	0.00
11) 2-Chlorophenol-d4	7.310	132	117058	5.450	ng/ul	0.00
15) 4-Methylphenol-d8	8.510	113	120355	5.174	ng/ul	0.01
21) Nitrobenzene-d5	8.945	128	66307	6.279	ng/ul	0.00
24) 2-Nitrophenol-d4	9.669	143	70494	6.432	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.216	165	130105	5.477	ng/ul	0.01
31) 4-Chloroaniline-d4	10.728	131	180317	5.098	ng/ul	0.00
46) Dimethylphthalate-d6	13.845	166	483671	5.961	ng/ul	0.00
49) Acenaphthylene-d8	14.122	160	530157	5.718	ng/ul	0.00
54) 4-Nitrophenol-d4	14.716	143	41241m	2.686	ng/ul	0.06
60) Fluorene-d10	15.422	176	446871	6.433	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.563	200	59062	4.242	ng/ul	0.00
73) Anthracene-d10	17.286	188	795235	6.901	ng/ul	0.00
81) Pyrene-d10	19.533	212	940310	7.396	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.509	264	770600	6.752	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110822\
Data File : BP012549.D
Acq On : 08 Nov 2022 12:56
Operator : CG/JU
Sample : N5407-06
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EW4Y6

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 11/09/2022
Supervised By :mohammad ahmed 11/14/2022

Quant Time: Nov 08 21:41:17 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Nov 04 02:53:36 2022
Response via : Initial Calibration

