




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110822\
 Data File : BP012568.D
 Acq On : 09 Nov 2022 00:57
 Operator : CG/JU
 Sample : N5407-18
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EW4Z5

Manual IntegrationsAPPROVED

Quant Time: Nov 09 02:25:50 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Nov 08 22:40:23 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 11/09/2022
 Supervised By :mohammad ahmed 11/14/2022

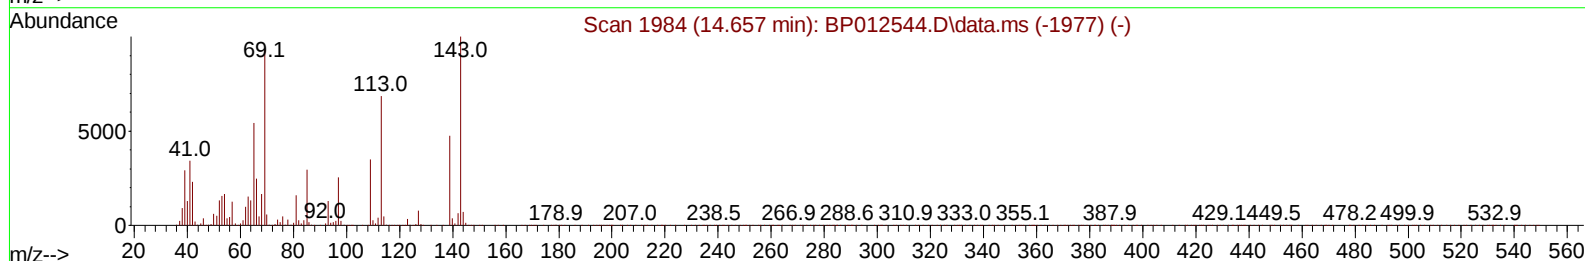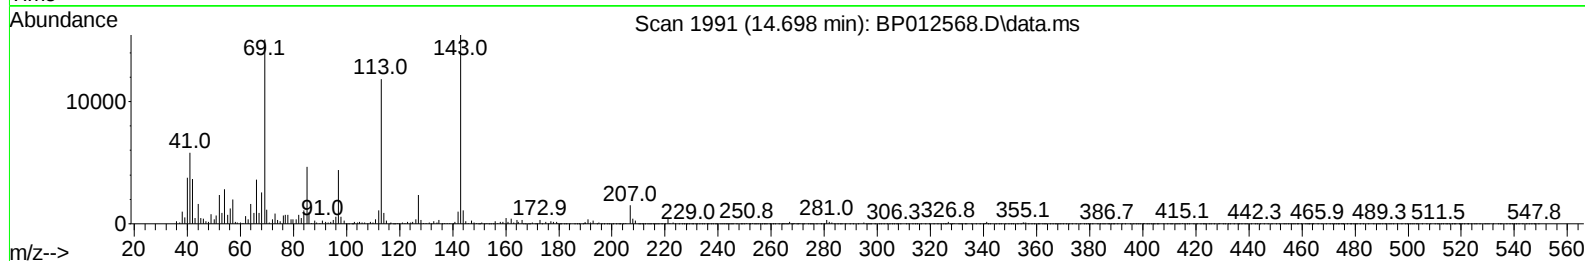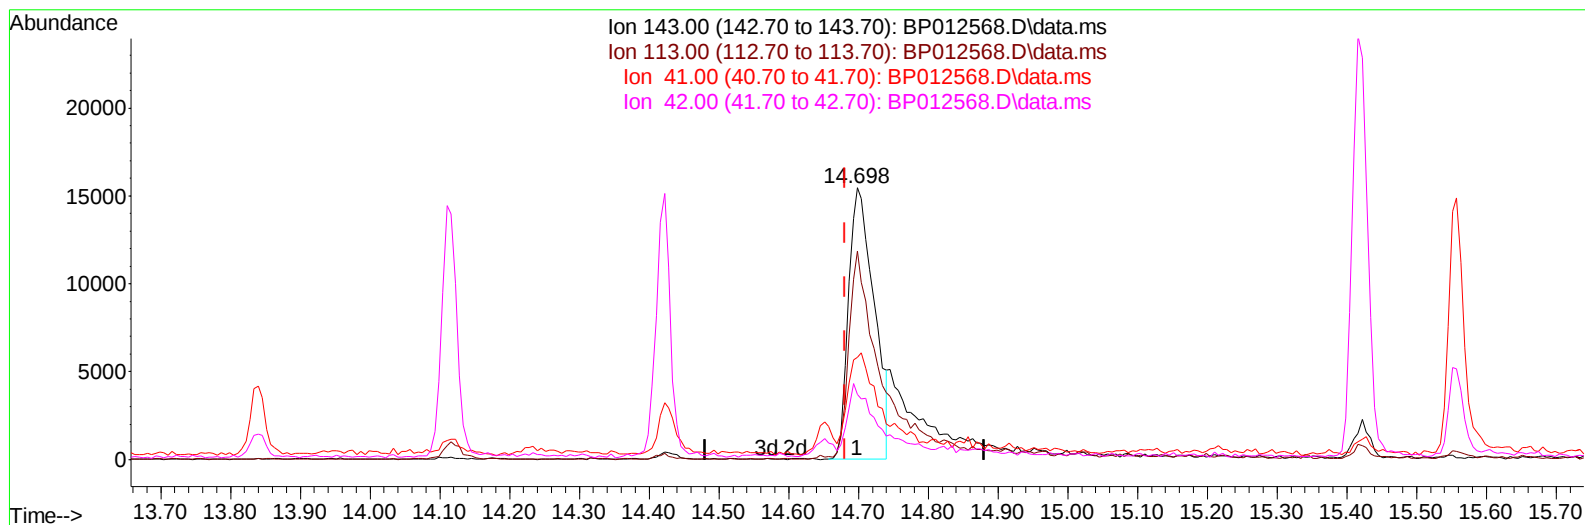

TIC: BP012568.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.698min (+ 0.018) 3.57 ng/u1

response 39286

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	65.10	76.78
41.00	34.50	37.62
42.00	23.60	23.85




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110822\
Data File : BP012568.D
Acq On : 09 Nov 2022 00:57
Operator : CG/JU
Sample : N5407-18
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EW4Z5

Manual IntegrationsAPPROVED

Quant Time: Nov 09 02:25:50 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Nov 08 22:40:23 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 11/09/2022
Supervised By :mohammad ahmed 11/14/2022

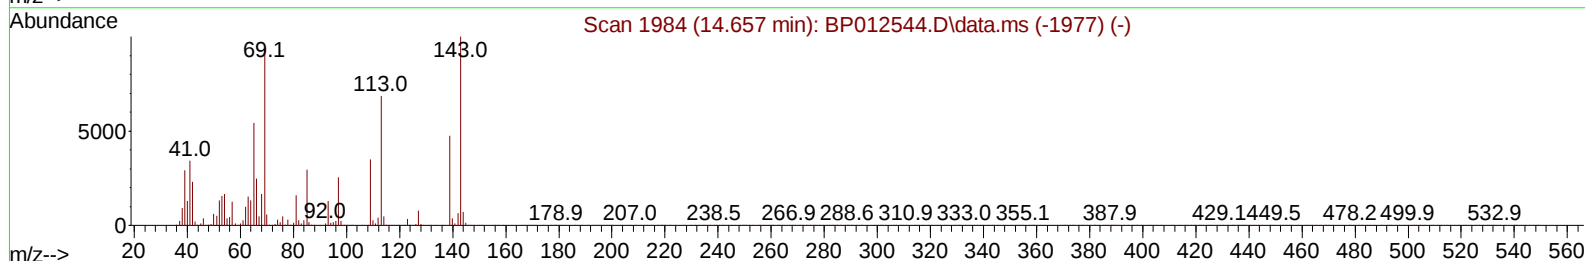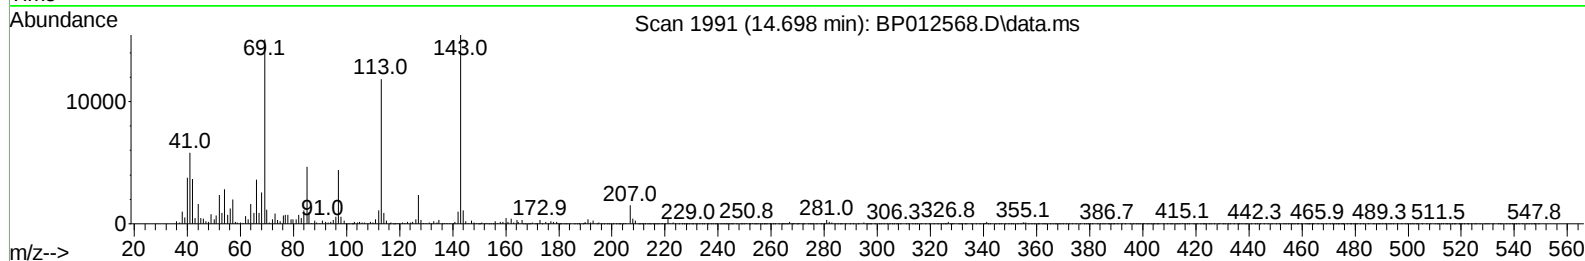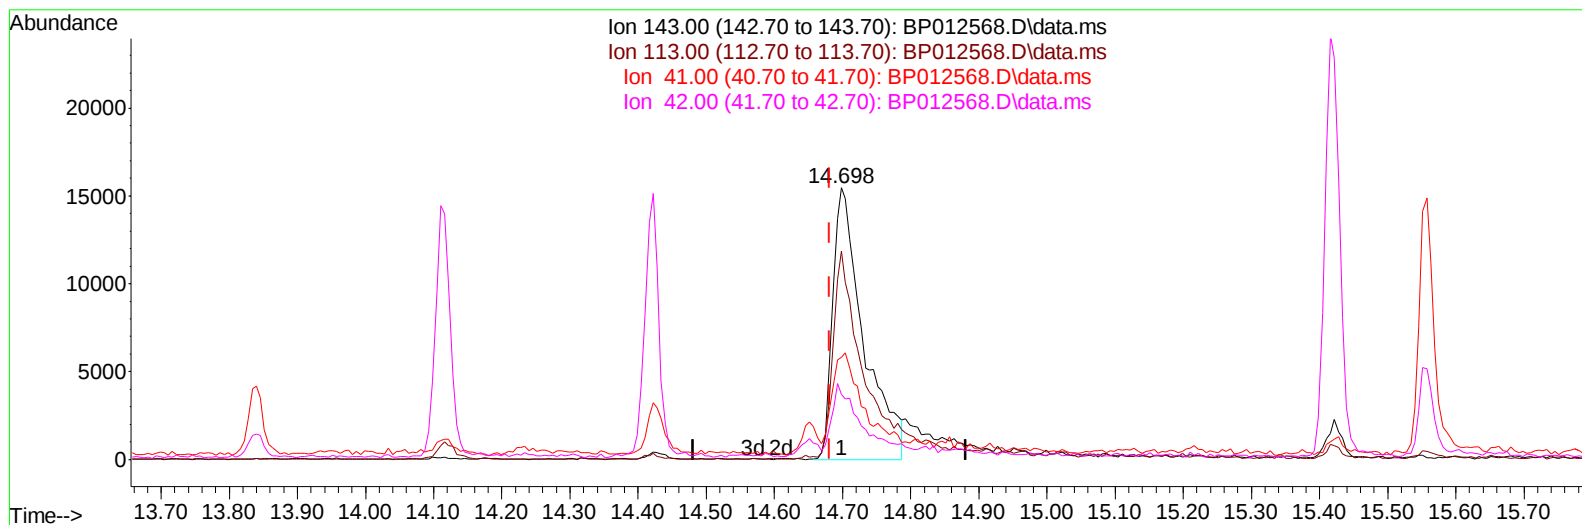

TIC: BP012568.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.698min (+ 0.018) 4.43 ng/ul m

response 48735

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	65.10	76.78
41.00	34.50	37.62
42.00	23.60	23.85

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110822\
 Data File : BP012568.D
 Acq On : 09 Nov 2022 00:57
 Operator : CG/JU
 Sample : N5407-18
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EW4Z5

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 11/09/2022
 Supervised By :mohammad ahmed 11/14/2022

Quant Time: Nov 09 02:25:50 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Nov 08 22:40:23 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.769	152	235430	20.000	ng/ul	0.00
20) Naphthalene-d8	10.569	136	1171920	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.422	164	848743	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.187	188	1906108	20.000	ng/ul	0.00
79) Chrysene-d12	21.280	240	1726484	20.000	ng/ul	0.00
88) Perylene-d12	23.657	264	1562520	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.228	96	20778	3.554	ng/uL	0.00
4) Pyridine-d5	3.658	84	96816	5.764	ng/ul	0.00
7) Phenol-d5	6.964	99	151914	7.194	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.111	67	368549	29.237	ng/ul	0.00
11) 2-Chlorophenol-d4	7.305	132	340463	22.079	ng/ul	0.00
15) 4-Methylphenol-d8	8.499	113	269595	16.142	ng/ul	0.00
21) Nitrobenzene-d5	8.940	128	266639	35.086	ng/ul	0.00
24) 2-Nitrophenol-d4	9.658	143	250591	31.769	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.205	165	450212	26.337	ng/ul	0.00
31) 4-Chloroaniline-d4	10.722	131	533649	20.966	ng/ul	0.00
46) Dimethylphthalate-d6	13.840	166	1982145	34.115	ng/ul	0.00
49) Acenaphthylene-d8	14.116	160	2098512	31.606	ng/ul	0.00
54) 4-Nitrophenol-d4	14.698	143	48735m	4.432	ng/ul	0.02
60) Fluorene-d10	15.422	176	1757977	35.340	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.557	200	292223	29.446	ng/ul	0.00
73) Anthracene-d10	17.287	188	3095869	37.695	ng/ul	0.00
81) Pyrene-d10	19.528	212	3537136	40.806	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.504	264	2953296	38.683	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110822\
Data File : BP012568.D
Acq On : 09 Nov 2022 00:57
Operator : CG/JU
Sample : N5407-18
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EW4Z5

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 11/09/2022
Supervised By :mohammad ahmed 11/14/2022

Quant Time: Nov 09 02:25:50 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Nov 08 22:40:23 2022
Response via : Initial Calibration

