




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110822\
 Data File : BP012572.D
 Acq On : 09 Nov 2022 03:13
 Operator : CG/JU
 Sample : N5455-02
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BFZ12

Manual IntegrationsAPPROVED

Quant Time: Nov 09 04:01:23 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Nov 08 22:40:23 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 11/09/2022
 Supervised By :mohammad ahmed 11/14/2022

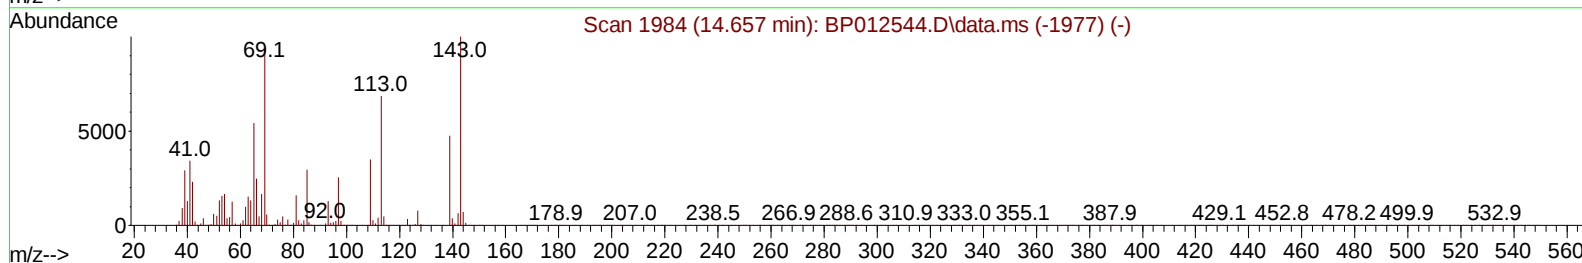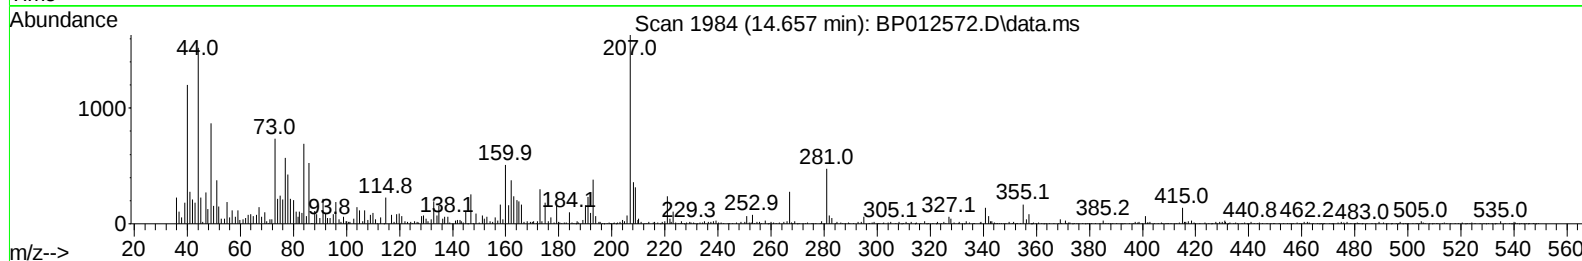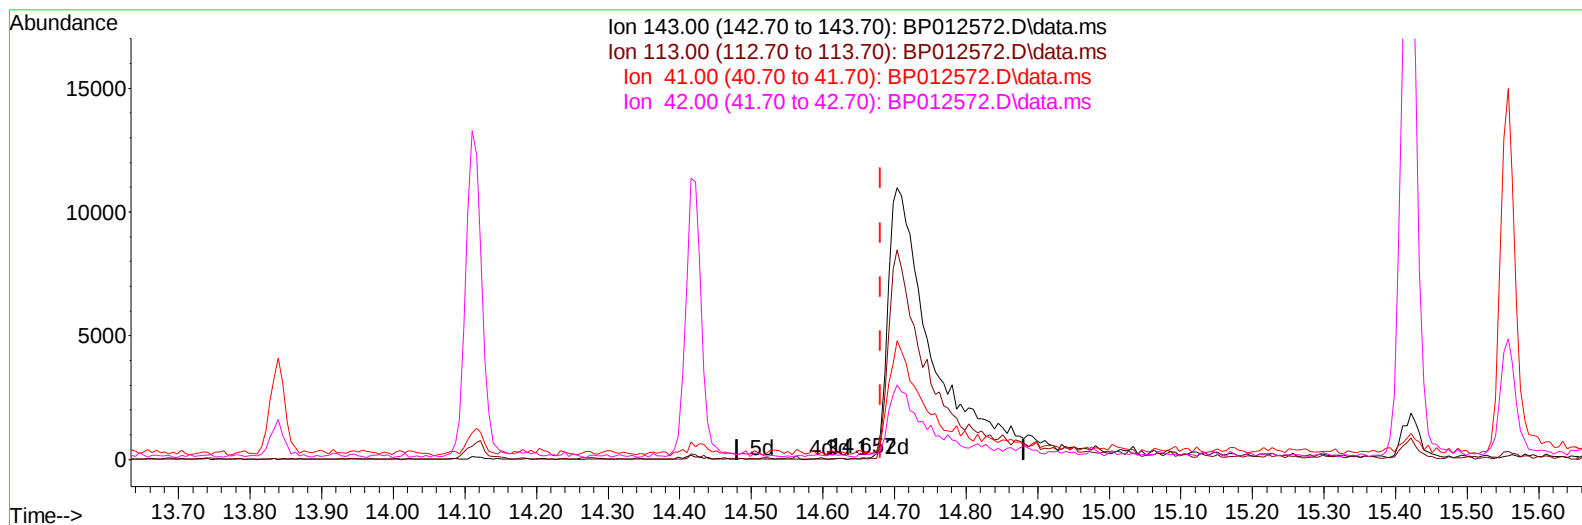

TIC: BP012572.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.657min (-0.024) 0.00 ng/u1

response 41

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	65.10	98.18#
41.00	34.50	503.64#
42.00	23.60	387.27#




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110822\
 Data File : BP012572.D
 Acq On : 09 Nov 2022 03:13
 Operator : CG/JU
 Sample : N5455-02
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BFZ12

Manual IntegrationsAPPROVED

Quant Time: Nov 09 04:01:23 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Nov 08 22:40:23 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 11/09/2022
 Supervised By :mohammad ahmed 11/14/2022

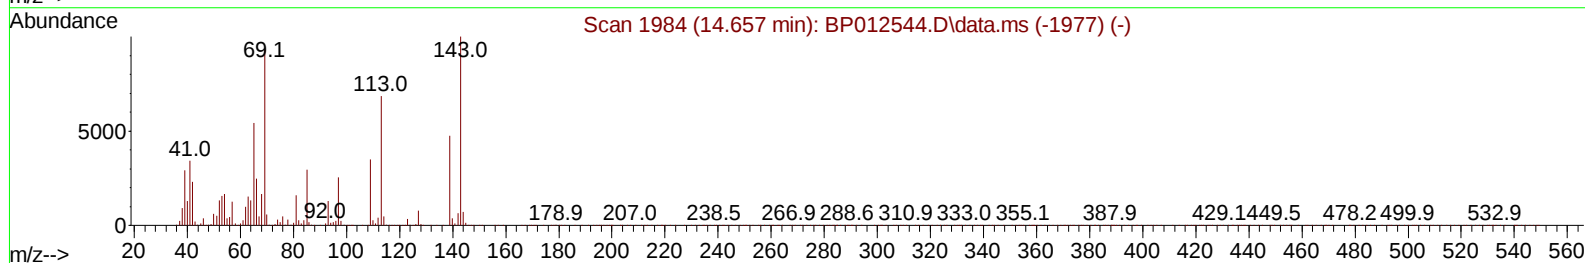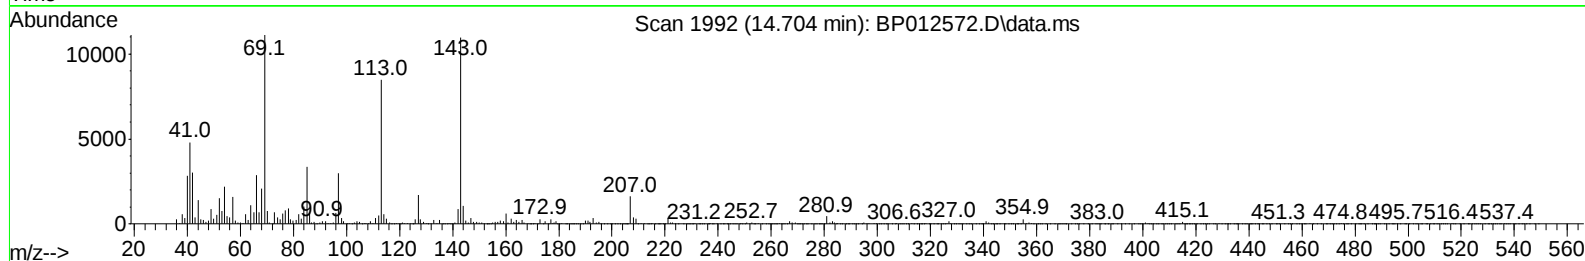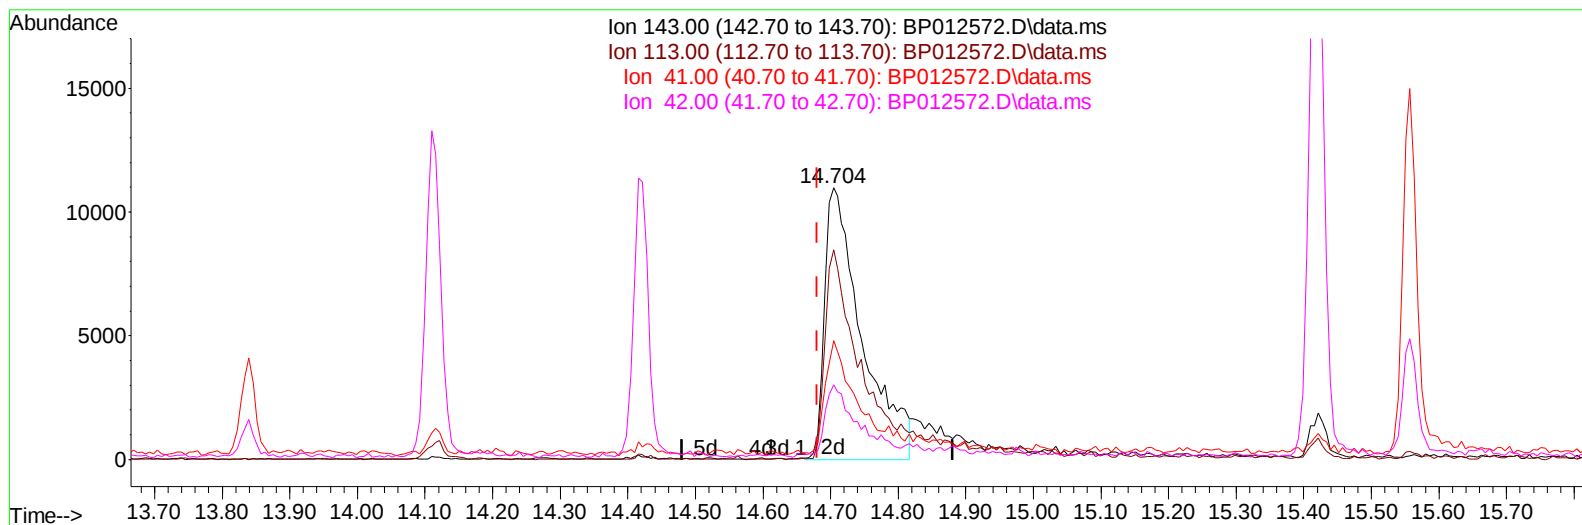

TIC: BP012572.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.704min (+ 0.023) 4.86 ng/ul m

response 42124

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	65.10	77.21
41.00	34.50	43.71#
42.00	23.60	27.56

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110822\
 Data File : BP012572.D
 Acq On : 09 Nov 2022 03:13
 Operator : CG/JU
 Sample : N5455-02
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BFZ12

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 11/09/2022
 Supervised By :mohammad ahmed 11/14/2022

Quant Time: Nov 09 04:01:23 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Nov 08 22:40:23 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.769	152	184644	20.000	ng/ul	0.00
20) Naphthalene-d8	10.563	136	923831	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.422	164	668342	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.186	188	1510581	20.000	ng/ul	0.00
79) Chrysene-d12	21.280	240	1393443	20.000	ng/ul	0.00
88) Perylene-d12	23.657	264	1247734	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.222	96	20634	4.500	ng/uL	0.00
4) Pyridine-d5	3.669	84	42913	3.258	ng/ul	0.02
7) Phenol-d5	6.963	99	225651	13.625	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.105	67	355692	35.978	ng/ul	0.00
11) 2-Chlorophenol-d4	7.305	132	426626	35.276	ng/ul	0.00
15) 4-Methylphenol-d8	8.499	113	374907	28.622	ng/ul	0.00
21) Nitrobenzene-d5	8.940	128	254867	42.543	ng/ul	0.00
24) 2-Nitrophenol-d4	9.657	143	282063	45.362	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.204	165	518688	38.491	ng/ul	0.00
31) 4-Chloroaniline-d4	10.728	131	98418	4.905	ng/ul	0.00
46) Dimethylphthalate-d6	13.839	166	1952320	42.672	ng/ul	0.00
49) Acenaphthylene-d8	14.110	160	2043023	39.075	ng/ul	0.00
54) 4-Nitrophenol-d4	14.704	143	42124m	4.865	ng/ul	0.02
60) Fluorene-d10	15.422	176	1726685	44.080	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.557	200	285440	36.294	ng/ul	0.00
73) Anthracene-d10	17.286	188	2953389	45.376	ng/ul	0.00
81) Pyrene-d10	19.527	212	3370205	48.173	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.504	264	2802798	45.973	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110822\
Data File : BP012572.D
Acq On : 09 Nov 2022 03:13
Operator : CG/JU
Sample : N5455-02
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BFZ12

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 11/09/2022
Supervised By :mohammad ahmed 11/14/2022

Quant Time: Nov 09 04:01:23 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Nov 08 22:40:23 2022
Response via : Initial Calibration

