

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110822\
 Data File : BP012545.D
 Acq On : 08 Nov 2022 10:38
 Operator : CG/JU
 Sample : PB148823BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK823

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
 Title : SVOA CALIBRATION

Signal : TIC: BP012545.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.228	37	41	51	rVB	78327	113047	1.08%	0.114%
2	3.963	161	166	174	rVB	29975	50649	0.48%	0.051%
3	6.952	667	674	693	rBV	1357264	2360123	22.56%	2.388%
4	7.110	695	701	718	rVV	1132470	1866305	17.84%	1.888%
5	7.304	727	734	753	rBV	1392291	2284343	21.83%	2.311%
6	7.769	805	813	828	rBV	1181640	1988855	19.01%	2.012%
7	8.493	927	936	959	rBV	1801723	3138552	30.00%	3.176%
8	8.940	1005	1012	1029	rBV	1386635	2386606	22.81%	2.415%
9	9.663	1125	1135	1152	rBV	1172767	2030929	19.41%	2.055%
10	10.198	1218	1226	1268	rBV	1601158	3362147	32.14%	3.402%
11	10.569	1282	1289	1306	rBV	1894383	3359537	32.11%	3.399%
12	10.763	1316	1322	1331	rBV4	8970	21494	0.21%	0.022%
13	12.187	1558	1564	1572	rBV2	20569	47494	0.45%	0.048%
14	13.316	1752	1756	1764	rVB3	15178	27549	0.26%	0.028%
15	13.398	1766	1770	1775	rBV5	7552	10962	0.10%	0.011%
16	13.845	1839	1846	1859	rBV	3647811	5284829	50.51%	5.347%
17	14.116	1885	1892	1910	rBV	2492363	3793239	36.26%	3.838%
18	14.428	1938	1945	1964	rBV	3276461	5047958	48.25%	5.108%
19	14.657	1977	1984	2013	rBV	930014	2313153	22.11%	2.341%
20	15.422	2108	2114	2132	rBV	5046680	7911973	75.62%	8.006%
21	15.563	2132	2138	2150	rVV	1252662	1980962	18.93%	2.004%
22	15.663	2152	2155	2170	rVB	34468	70608	0.67%	0.071%
23	16.869	2356	2360	2365	rVB7	8181	14407	0.14%	0.015%
24	16.980	2374	2379	2383	rBV2	10749	17166	0.16%	0.017%
25	17.186	2407	2414	2425	rBV	4262642	6380427	60.98%	6.456%
26	17.286	2425	2431	2454	rVB	5771498	8848753	84.58%	8.953%
27	19.104	2736	2740	2747	rBV3	84973	129753	1.24%	0.131%
28	19.174	2749	2752	2757	rVB	66813	94002	0.90%	0.095%
29	19.533	2807	2813	2825	rBV	7140126	10271997	98.18%	10.394%
30	21.286	3106	3111	3120	rBV	5004442	6237565	59.62%	6.311%
31	23.445	3476	3478	3479	rBV	189959	139469	1.33%	0.141%
32	23.510	3482	3489	3503	rVV	4916534	10462383	100.00%	10.586%
33	23.662	3509	3515	3531	rVB2	3188264	6783019	64.83%	6.863%




Sum of corrected areas: 98830255

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110822\
Data File : BP012545.D
Acq On : 08 Nov 2022 10:38
Operator : CG/JU
Sample : PB148823BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK823

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

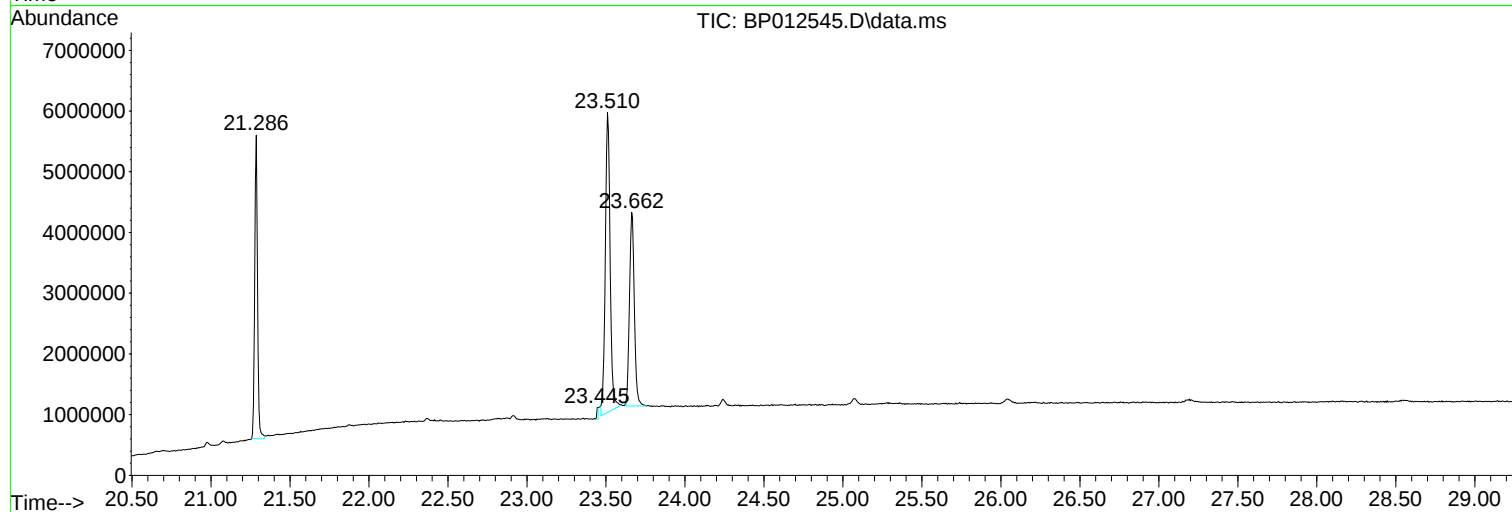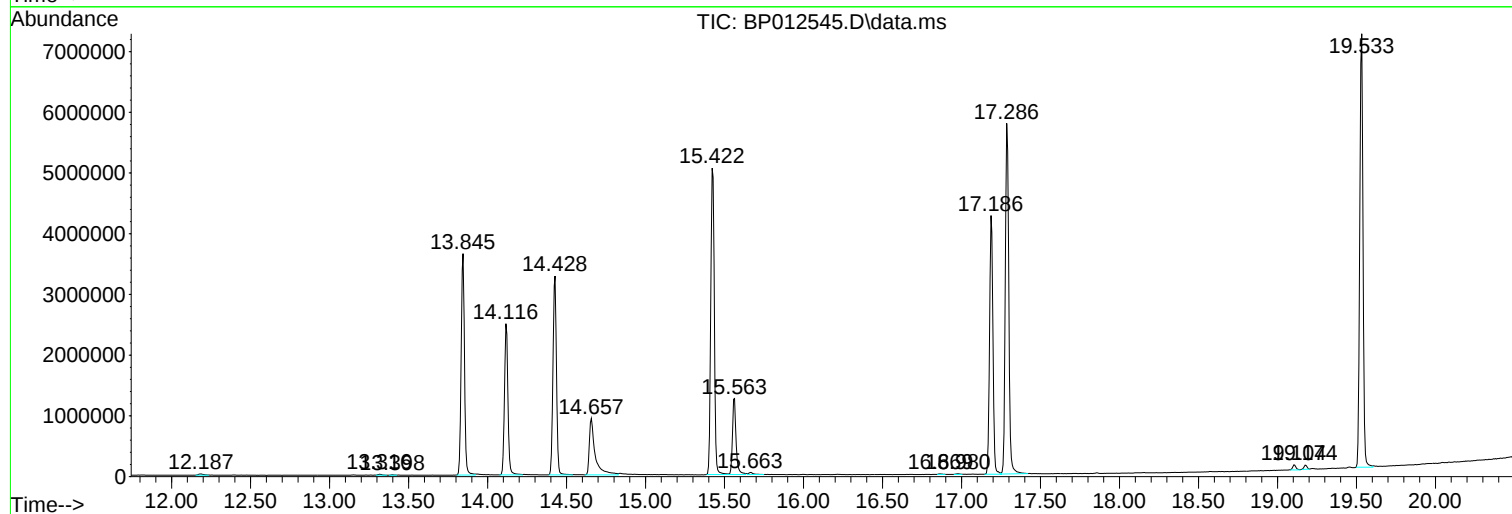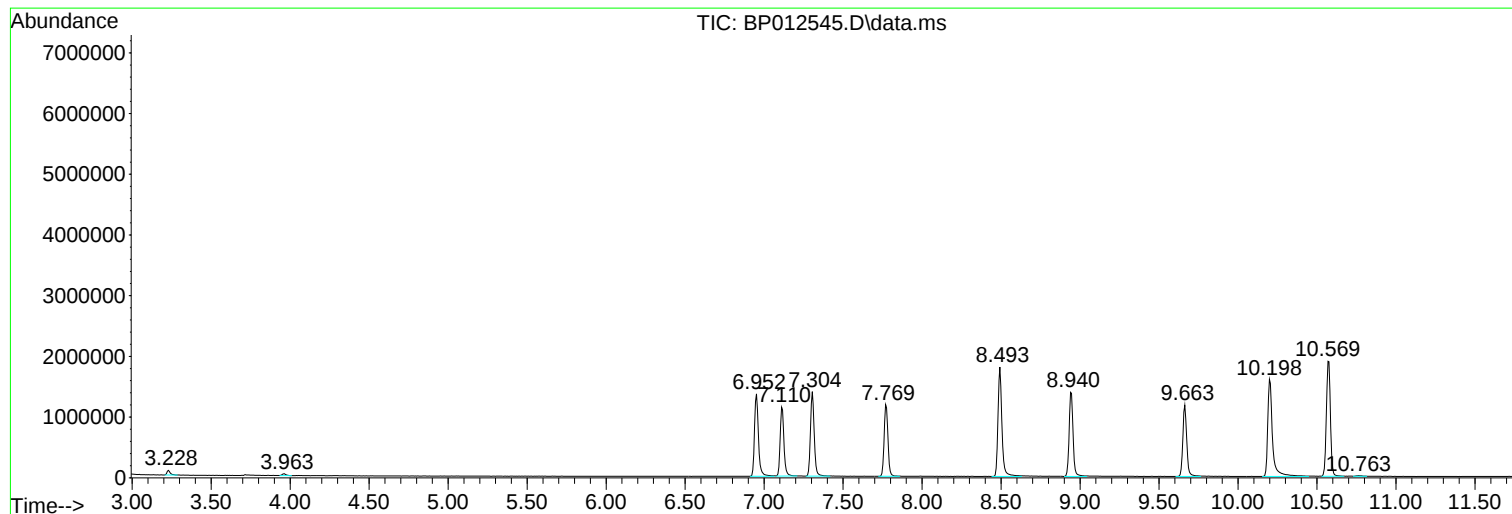

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110822\
Data File : BP012545.D
Acq On : 08 Nov 2022 10:38
Operator : CG/JU
Sample : PB148823BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK823

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110822\
Data File : BP012545.D
Acq On : 08 Nov 2022 10:38
Operator : CG/JU
Sample : PB148823BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK823

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc