

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110822\
 Data File : BP012549.D
 Acq On : 08 Nov 2022 12:56
 Operator : CG/JU
 Sample : N5407-06
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EW4Y6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
 Title : SVOA CALIBRATION

Signal : TIC: BP012549.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.228	37	41	47	rBV	33029	39887	0.59%	0.089%
2	3.663	113	115	125	rBV	117084	224441	3.34%	0.499%
3	3.957	161	165	171	rVB	16053	25342	0.38%	0.056%
4	6.969	671	677	690	rBV	192049	355353	5.29%	0.790%
5	7.116	696	702	714	rBV	184951	312052	4.65%	0.694%
6	7.310	728	735	751	rBV	226369	391776	5.84%	0.871%
7	7.775	807	814	829	rBV	1113325	1880155	28.01%	4.180%
8	8.510	932	939	952	rBV	263325	517871	7.72%	1.151%
9	8.945	1006	1013	1029	rBV	241818	428255	6.38%	0.952%
10	9.663	1125	1135	1150	rBV	188011	357484	5.33%	0.795%
11	10.216	1222	1229	1244	rBV	267764	570912	8.51%	1.269%
12	10.575	1281	1290	1309	rBV	1828063	3263414	48.62%	7.255%
13	10.728	1309	1316	1331	rBV	259019	548521	8.17%	1.219%
14	11.934	1515	1521	1527	rBV2	9585	19676	0.29%	0.044%
15	12.175	1555	1562	1567	rBV9	5168	12249	0.18%	0.027%
16	13.145	1725	1727	1734	rVB8	6018	7948	0.12%	0.018%
17	13.316	1752	1756	1764	rBV8	6077	10302	0.15%	0.023%
18	13.845	1839	1846	1857	rBV	657470	989393	14.74%	2.199%
19	14.122	1884	1893	1908	rBV	752009	1206353	17.97%	2.682%
20	14.428	1938	1945	1966	rBV	3411710	5084986	75.76%	11.304%
21	14.716	1987	1994	2014	rBV2	78013	276407	4.12%	0.614%
22	15.427	2108	2115	2125	rBV	1042890	1638452	24.41%	3.642%
23	15.563	2132	2138	2149	rBV	239685	389637	5.81%	0.866%
24	17.192	2408	2415	2426	rBV	4285996	6401140	95.37%	14.230%
25	17.286	2426	2431	2447	rVB	1319828	1966594	29.30%	4.372%
26	17.857	2525	2528	2531	rBV5	12659	15535	0.23%	0.035%
27	18.080	2562	2566	2574	rBV	73125	124436	1.85%	0.277%
28	19.451	2795	2799	2804	rBV	336762	388029	5.78%	0.863%
29	19.533	2807	2813	2822	rVV	1745348	2419913	36.06%	5.379%
30	21.286	3106	3111	3119	rBV	5214727	6711607	100.00%	14.920%
31	23.515	3484	3490	3501	rVB2	991760	2321780	34.59%	5.161%
32	23.668	3509	3516	3530	rVB2	2975461	6084388	90.65%	13.526%




Sum of corrected areas: 44984288

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110822\
Data File : BP012549.D
Acq On : 08 Nov 2022 12:56
Operator : CG/JU
Sample : N5407-06
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EW4Y6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

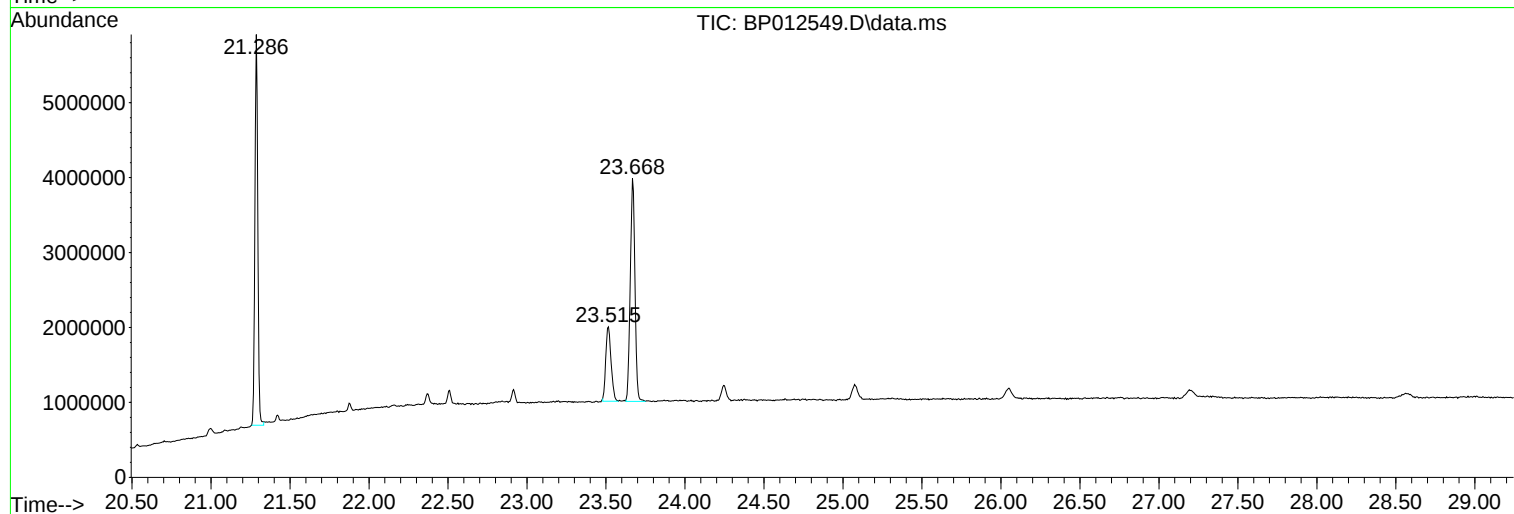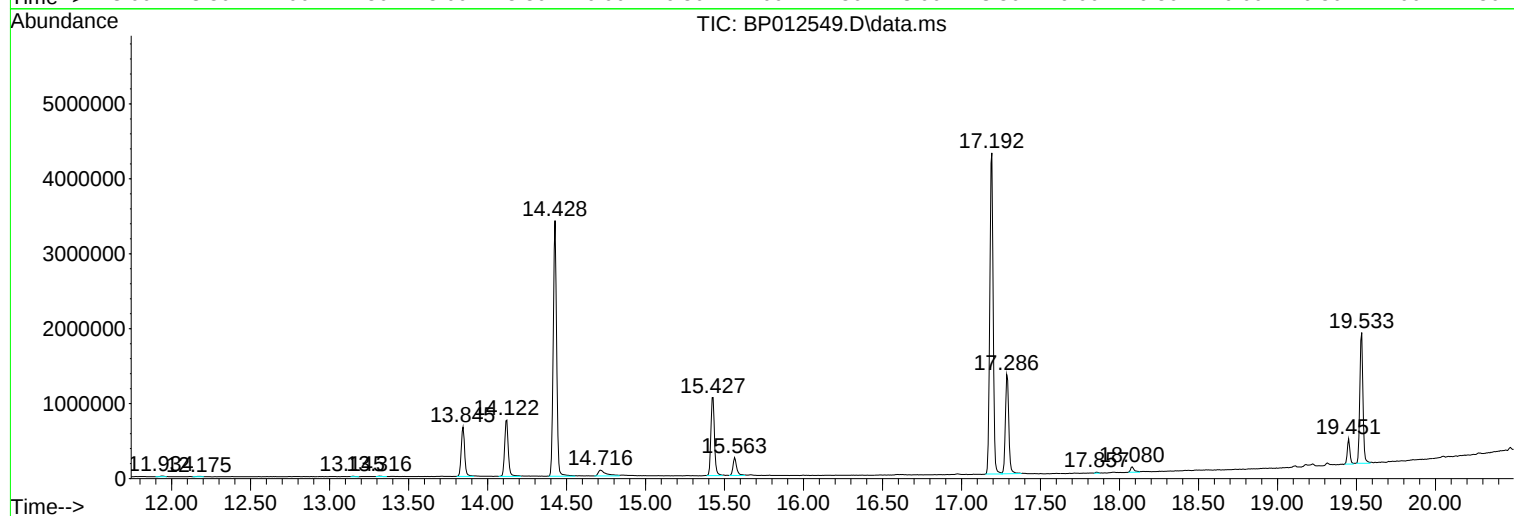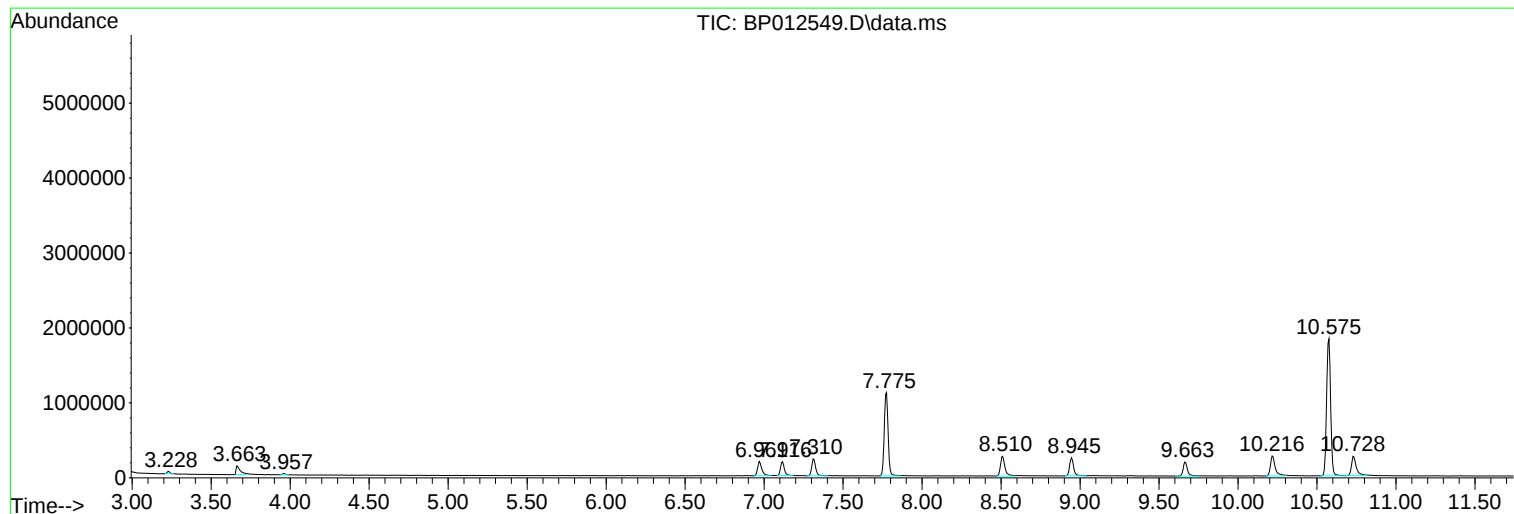

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110822\
Data File : BP012549.D
Acq On : 08 Nov 2022 12:56
Operator : CG/JU
Sample : N5407-06
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EW4Y6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110822\
Data File : BP012549.D
Acq On : 08 Nov 2022 12:56
Operator : CG/JU
Sample : N5407-06
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EW4Y6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc