

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110822\
 Data File : BP012553.D
 Acq On : 08 Nov 2022 15:14
 Operator : CG/JU
 Sample : N5407-11
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EW4Z0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
 Title : SVOA CALIBRATION

Signal : TIC: BP012553.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.228	37	41	52	rVB	54034	80567	0.71%	0.086%
2	3.658	111	114	136	rBV	286672	543608	4.77%	0.577%
3	3.858	144	148	159	rVB	19822	36604	0.32%	0.039%
4	3.958	161	165	169	rBV	15274	20220	0.18%	0.021%
5	6.969	669	677	692	rBV	365826	669489	5.87%	0.711%
6	7.111	695	701	716	rVV	1024862	1723706	15.12%	1.831%
7	7.311	728	735	750	rBV	1134270	1848599	16.21%	1.963%
8	7.769	806	813	825	rBV	871360	1436666	12.60%	1.526%
9	8.505	931	938	961	rBV	1083070	1913112	16.78%	2.032%
10	8.946	1005	1013	1030	rBV	1361686	2340752	20.53%	2.486%
11	9.316	1071	1076	1081	rBV4	7020	12672	0.11%	0.013%
12	9.663	1127	1135	1154	rBV	1140735	1945463	17.06%	2.066%
13	10.210	1220	1228	1250	rBV	1709080	3171864	27.82%	3.369%
14	10.575	1282	1290	1304	rBV	1425453	2469548	21.66%	2.623%
15	10.728	1308	1316	1341	rBV	1465990	2860502	25.09%	3.038%
16	11.940	1513	1522	1529	rBV2	26498	52844	0.46%	0.056%
17	12.169	1555	1561	1567	rBV2	26131	46515	0.41%	0.049%
18	13.046	1704	1710	1716	rVB5	6861	14538	0.13%	0.015%
19	13.316	1751	1756	1764	rVB4	12873	23656	0.21%	0.025%
20	13.393	1764	1769	1775	rBV4	9004	18370	0.16%	0.020%
21	13.845	1837	1846	1858	rBV	3753505	5327932	46.73%	5.659%
22	14.122	1884	1893	1910	rBV	4107081	6168296	54.10%	6.552%
23	14.428	1937	1945	1957	rBV	2442454	3706474	32.51%	3.937%
24	14.698	1985	1991	2011	rBV	224276	600493	5.27%	0.638%
25	14.869	2018	2020	2028	rVB7	19254	32296	0.28%	0.034%
26	15.428	2108	2115	2131	rBV	5303151	8221385	72.10%	8.732%
27	15.563	2131	2138	2151	rVV	1976943	2929719	25.69%	3.112%
28	15.663	2152	2155	2161	rVB	30714	45872	0.40%	0.049%
29	16.004	2208	2213	2217	rBV6	7696	12213	0.11%	0.013%
30	16.857	2354	2358	2364	rBV8	8392	16245	0.14%	0.017%
31	16.981	2375	2379	2383	rVB4	7707	11429	0.10%	0.012%
32	17.186	2408	2414	2424	rBV	3270643	4746619	41.63%	5.042%
33	17.292	2425	2432	2457	rVB	6487435	9702976	85.10%	10.306%
34	17.851	2525	2527	2533	rBV7	8594	12273	0.11%	0.013%
35	18.081	2561	2566	2575	rBV	162021	270482	2.37%	0.287%
36	19.110	2737	2741	2747	rVB	96965	126637	1.11%	0.135%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110822\
Data File : BP012553.D
Acq On : 08 Nov 2022 15:14
Operator : CG/JU
Sample : N5407-11
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EW4Z0

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
Title : SVOA CALIBRATION

37	19.175	2748	2752	2757	rBV	101338	149706	1.31%	0.159%
38	19.316	2772	2776	2782	rBV2	153437	227325	1.99%	0.241%
39	19.533	2807	2813	2828	rBV	8285420	11402127	100.00%	12.111%
40	21.286	3106	3111	3119	rBV	4007462	5020695	44.03%	5.333%
41	23.516	3483	3490	3506	rVB2	4947816	9840449	86.30%	10.452%
42	23.668	3510	3516	3528	rVB2	2179548	4349427	38.15%	4.620%




Sum of corrected areas: 94150365

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110822\
Data File : BP012553.D
Acq On : 08 Nov 2022 15:14
Operator : CG/JU
Sample : N5407-11
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EW4Z0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

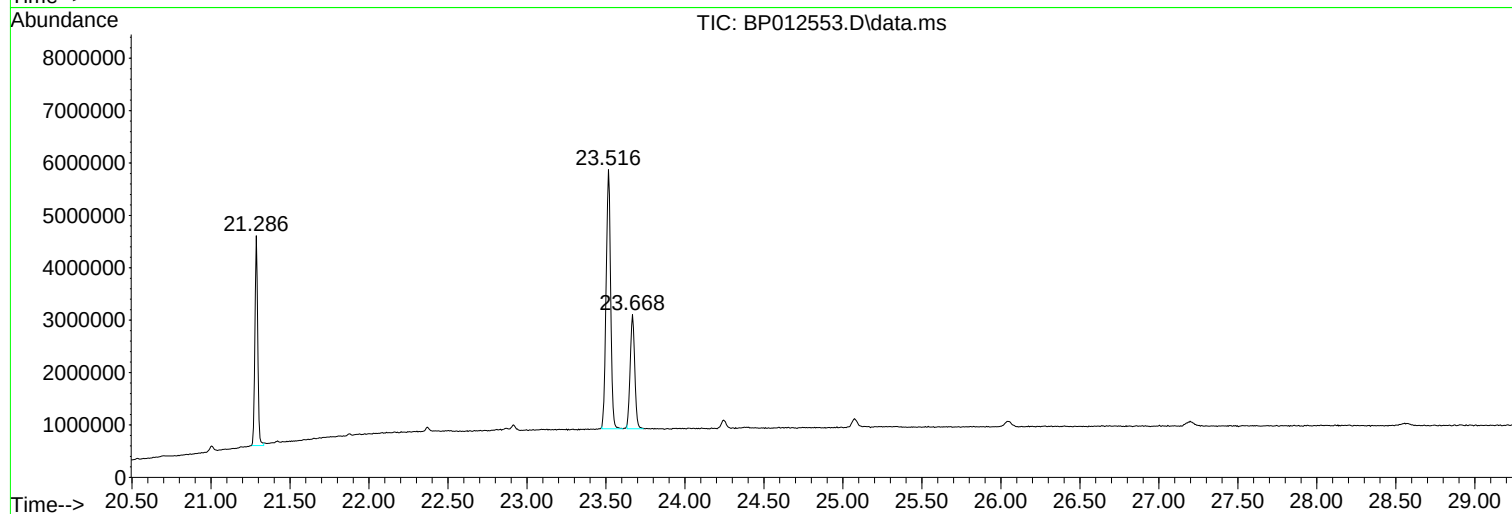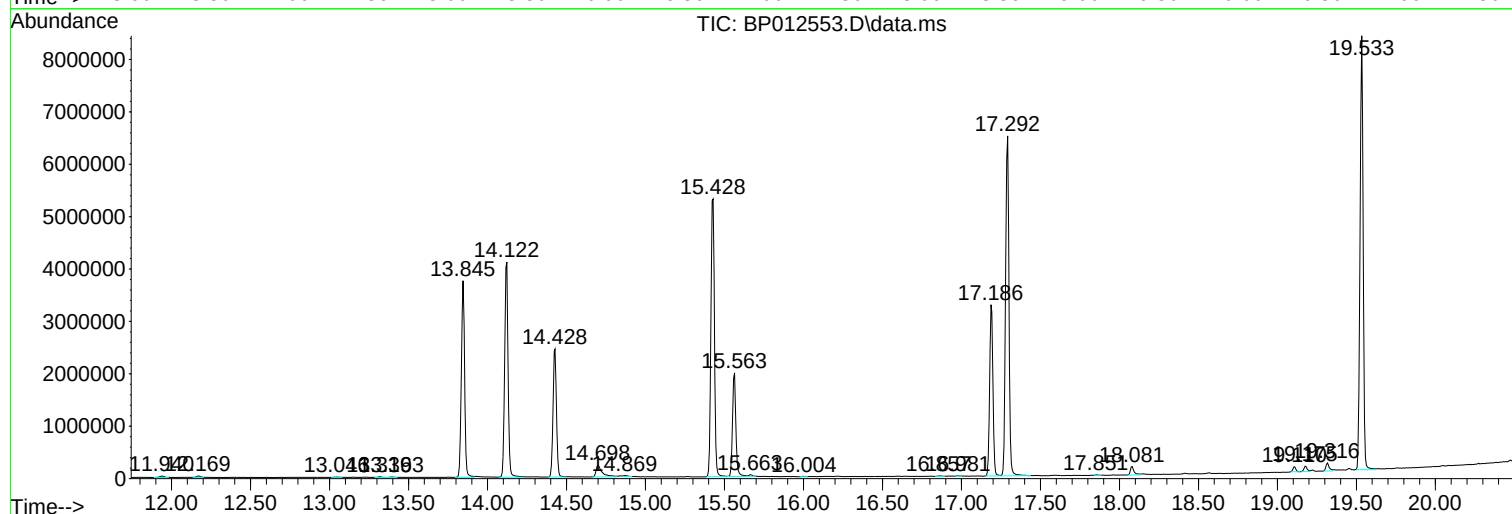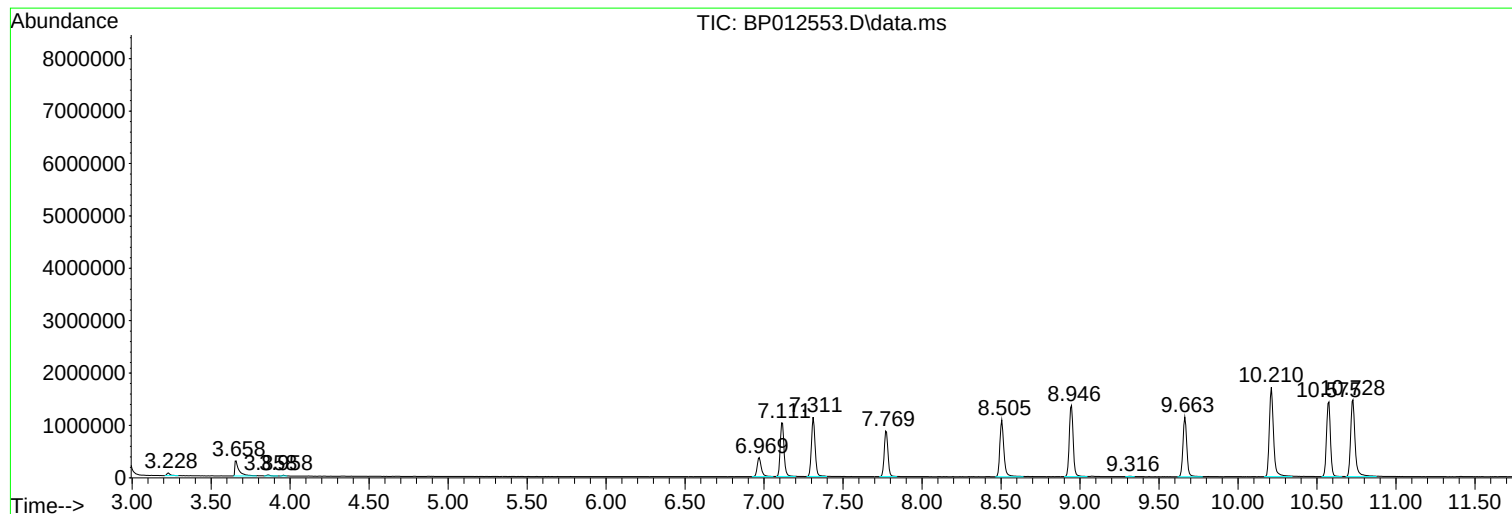

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110822\
Data File : BP012553.D
Acq On : 08 Nov 2022 15:14
Operator : CG/JU
Sample : N5407-11
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EW4Z0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110822\
Data File : BP012553.D
Acq On : 08 Nov 2022 15:14
Operator : CG/JU
Sample : N5407-11
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EW4Z0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc
