

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110822\
 Data File : BP012554.D
 Acq On : 08 Nov 2022 15:49
 Operator : CG/JU
 Sample : N5407-03
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EW4Y3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
 Title : SVOA CALIBRATION

Signal : TIC: BP012554.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.229	37	41	55	rVB	50018	81637	0.81%	0.099%
2	3.658	111	114	136	rBV	263027	497531	4.91%	0.603%
3	3.864	144	149	157	rVV	19523	35513	0.35%	0.043%
4	3.958	161	165	171	rVB	16828	25895	0.26%	0.031%
5	6.969	671	677	689	rBV	232073	430611	4.25%	0.522%
6	7.111	695	701	722	rVB	927838	1577289	15.55%	1.913%
7	7.311	728	735	751	rBV	667161	1094188	10.79%	1.327%
8	7.769	805	813	824	rBV	906090	1520658	15.00%	1.844%
9	8.505	931	938	963	rBV	615652	1118664	11.03%	1.357%
10	8.946	1005	1013	1026	rBV	1228760	2133286	21.04%	2.587%
11	9.322	1071	1077	1084	rVB4	6675	12439	0.12%	0.015%
12	9.663	1124	1135	1147	rBV	722481	1223175	12.06%	1.484%
13	10.211	1221	1228	1254	rBV	993793	1900051	18.74%	2.305%
14	10.575	1281	1290	1303	rBV	1477584	2615490	25.79%	3.172%
15	10.728	1308	1316	1335	rBV	1432037	2689161	26.52%	3.262%
16	12.175	1555	1562	1570	rVB2	23528	45181	0.45%	0.055%
17	13.028	1702	1707	1710	rBV3	8241	12680	0.13%	0.015%
18	13.322	1752	1757	1764	rBV3	14263	22419	0.22%	0.027%
19	13.399	1764	1770	1775	rVB6	5899	10857	0.11%	0.013%
20	13.846	1836	1846	1858	rBV	3041639	4295214	42.36%	5.210%
21	14.122	1885	1893	1909	rBV	3621611	5526249	54.50%	6.703%
22	14.428	1938	1945	1959	rBV	2640879	3939684	38.85%	4.778%
23	14.710	1987	1993	2004	rBV	102312	284276	2.80%	0.345%
24	15.222	2077	2080	2084	rVB3	8677	10332	0.10%	0.013%
25	15.428	2108	2115	2132	rBV	4963972	7533673	74.29%	9.137%
26	15.563	2132	2138	2152	rVV	1192312	1747208	17.23%	2.119%
27	15.663	2152	2155	2161	rVB2	27962	47173	0.47%	0.057%
28	16.593	2310	2313	2319	rBV8	8969	18106	0.18%	0.022%
29	16.863	2357	2359	2364	rVB5	8968	11220	0.11%	0.014%
30	17.192	2408	2415	2425	rBV	3334104	5010240	49.41%	6.077%
31	17.292	2425	2432	2457	rVB	5982943	8955296	88.31%	10.862%
32	17.857	2525	2528	2533	rVB6	20126	26527	0.26%	0.032%
33	18.081	2561	2566	2574	rBV	169390	264285	2.61%	0.321%
34	19.110	2737	2741	2746	rBV	87260	120098	1.18%	0.146%
35	19.175	2749	2752	2758	rBV	91311	151843	1.50%	0.184%
36	19.316	2772	2776	2783	rBV	131186	212787	2.10%	0.258%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110822\
Data File : BP012554.D
Acq On : 08 Nov 2022 15:49
Operator : CG/JU
Sample : N5407-03
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EW4Y3

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
Title : SVOA CALIBRATION

37	19.534	2807	2813	2826	rBV	7283801	10140532	100.00%	12.299%
38	21.286	3106	3111	3121	rBV	3797809	4935913	48.68%	5.987%
39	23.516	3483	3490	3501	rVB2	3953735	7922766	78.13%	9.609%
40	23.669	3510	3516	3529	rVB2	2162788	4249095	41.90%	5.154%




Sum of corrected areas: 82449242

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110822\
Data File : BP012554.D
Acq On : 08 Nov 2022 15:49
Operator : CG/JU
Sample : N5407-03
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EW4Y3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

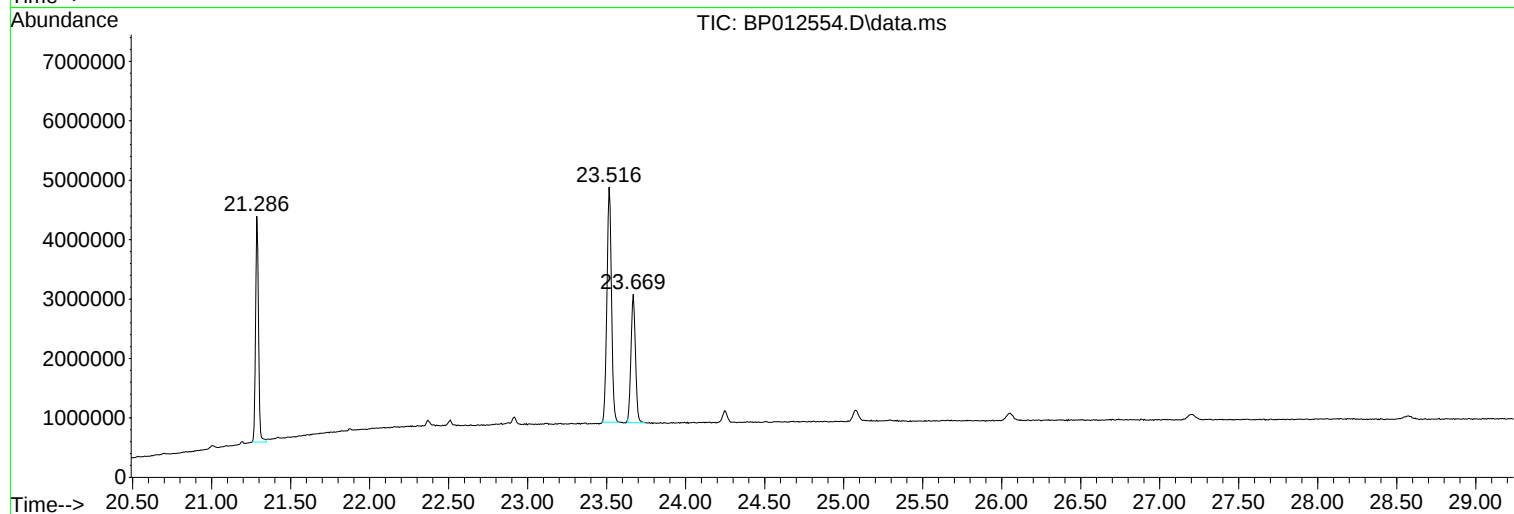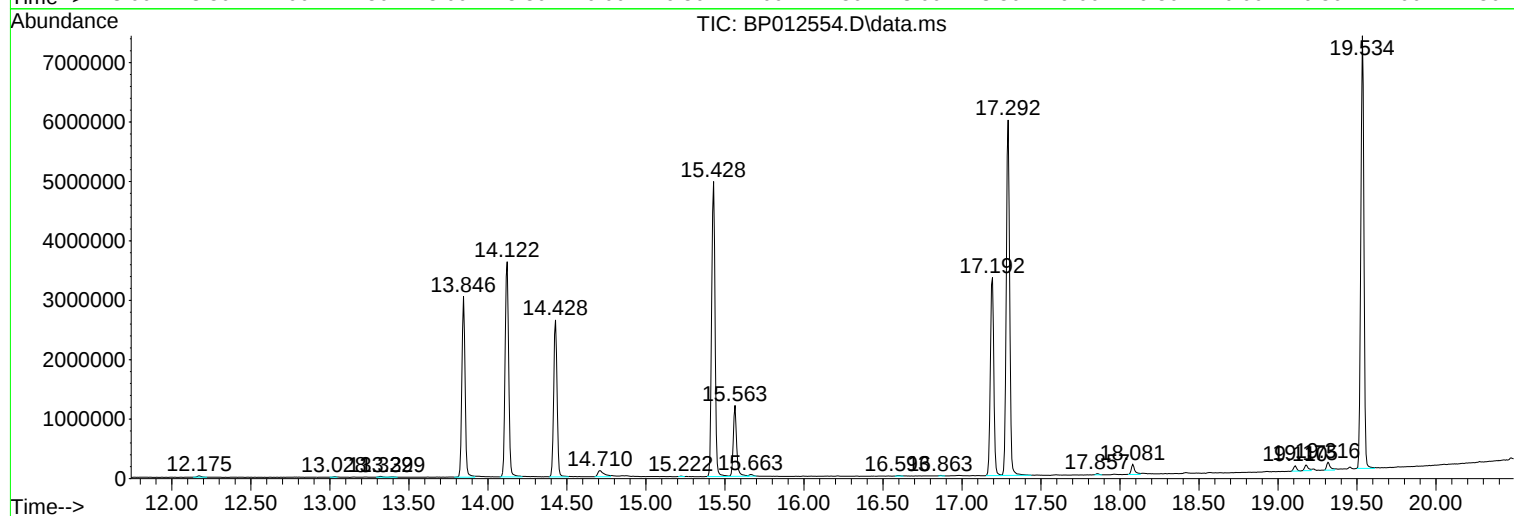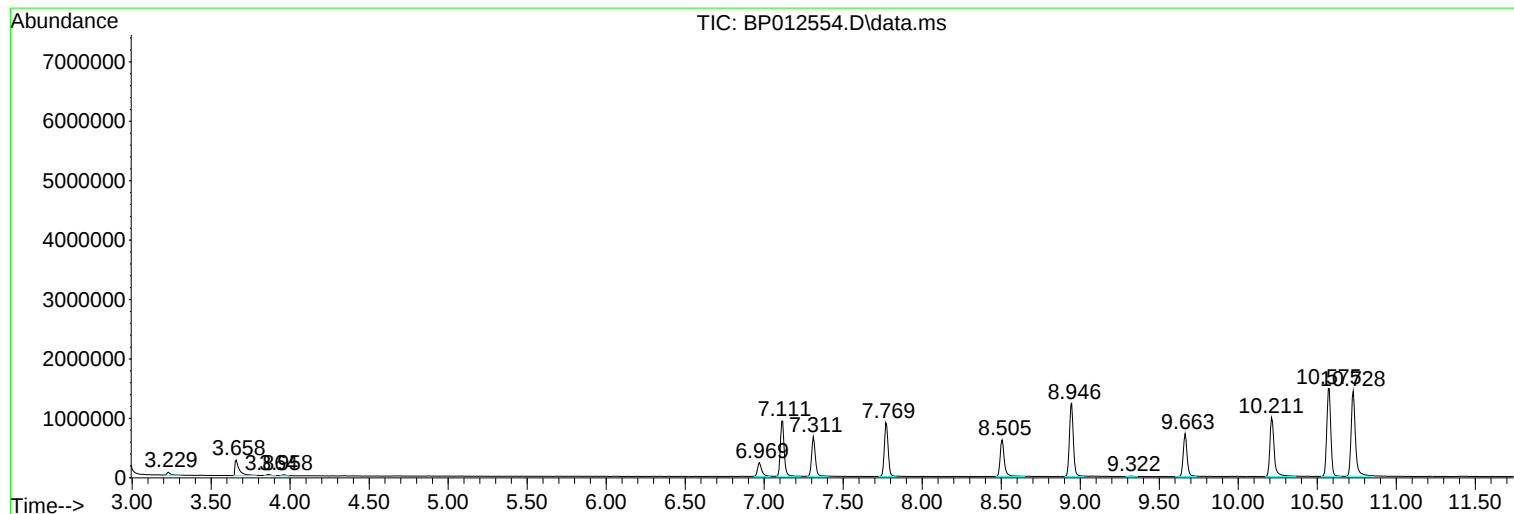

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110822\
Data File : BP012554.D
Acq On : 08 Nov 2022 15:49
Operator : CG/JU
Sample : N5407-03
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EW4Y3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110822\
Data File : BP012554.D
Acq On : 08 Nov 2022 15:49
Operator : CG/JU
Sample : N5407-03
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EW4Y3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc