

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110822\
 Data File : BP012556.D
 Acq On : 08 Nov 2022 18:08
 Operator : CG/JU
 Sample : PB148832BL
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK832

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
 Title : SVOA CALIBRATION

Signal : TIC: BP012556.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.228	37	41	49	rVB	60253	83834	1.12%	0.121%
2	3.646	109	112	139	rBV	686602	1282091	17.12%	1.853%
3	3.952	161	164	173	rVB3	10343	18051	0.24%	0.026%
4	6.963	669	676	695	rBV	1029813	1829073	24.42%	2.643%
5	7.111	695	701	717	rVB	816079	1323229	17.67%	1.912%
6	7.311	727	735	751	rBV	1005973	1713509	22.88%	2.476%
7	7.769	806	813	825	rBV	580524	959599	12.81%	1.387%
8	8.499	930	937	955	rBV2	1336323	2413138	32.22%	3.487%
9	8.940	1005	1012	1028	rBV	1015800	1739330	23.22%	2.513%
10	9.663	1127	1135	1153	rBV	830902	1486808	19.85%	2.148%
11	10.204	1219	1227	1260	rBV	1274461	2570851	34.33%	3.715%
12	10.569	1281	1289	1299	rBV	960193	1644157	21.95%	2.376%
13	10.722	1307	1315	1341	rBV	1292420	2547626	34.02%	3.681%
14	12.175	1557	1562	1572	rBV2	18851	40147	0.54%	0.058%
15	13.316	1752	1756	1762	rBV3	12897	21489	0.29%	0.031%
16	13.393	1765	1769	1775	rBV6	4741	9512	0.13%	0.014%
17	13.840	1836	1845	1860	rBV	2532569	3752439	50.10%	5.422%
18	14.116	1884	1892	1910	rBV	3032516	4578847	61.14%	6.616%
19	14.422	1937	1944	1955	rBV	1648504	2539596	33.91%	3.670%
20	14.687	1982	1989	2012	rBV	627852	1655340	22.10%	2.392%
21	15.422	2107	2114	2131	rBV	3937209	5905983	78.86%	8.534%
22	15.557	2131	2137	2151	rVV	1199706	1793323	23.95%	2.591%
23	15.663	2152	2155	2162	rVB3	23325	38386	0.51%	0.055%
24	16.969	2373	2377	2382	rBV5	5996	12865	0.17%	0.019%
25	17.186	2408	2414	2424	rBV	2222804	3219890	42.99%	4.653%
26	17.286	2425	2431	2450	rVB2	4306616	6585547	87.93%	9.516%
27	19.104	2737	2740	2745	rVB3	57200	75571	1.01%	0.109%
28	19.175	2748	2752	2758	rBV	52943	84540	1.13%	0.122%
29	19.533	2807	2813	2822	rBV	5271548	7489169	100.00%	10.822%
30	21.286	3106	3111	3122	rBV	2291526	3139139	41.92%	4.536%
31	23.510	3483	3489	3505	rVB2	2946633	6024435	80.44%	8.705%
32	23.663	3510	3515	3527	rVB2	1292569	2627975	35.09%	3.797%




Sum of corrected areas: 69205489

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110822\
Data File : BP012556.D
Acq On : 08 Nov 2022 18:08
Operator : CG/JU
Sample : PB148832BL
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK832

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

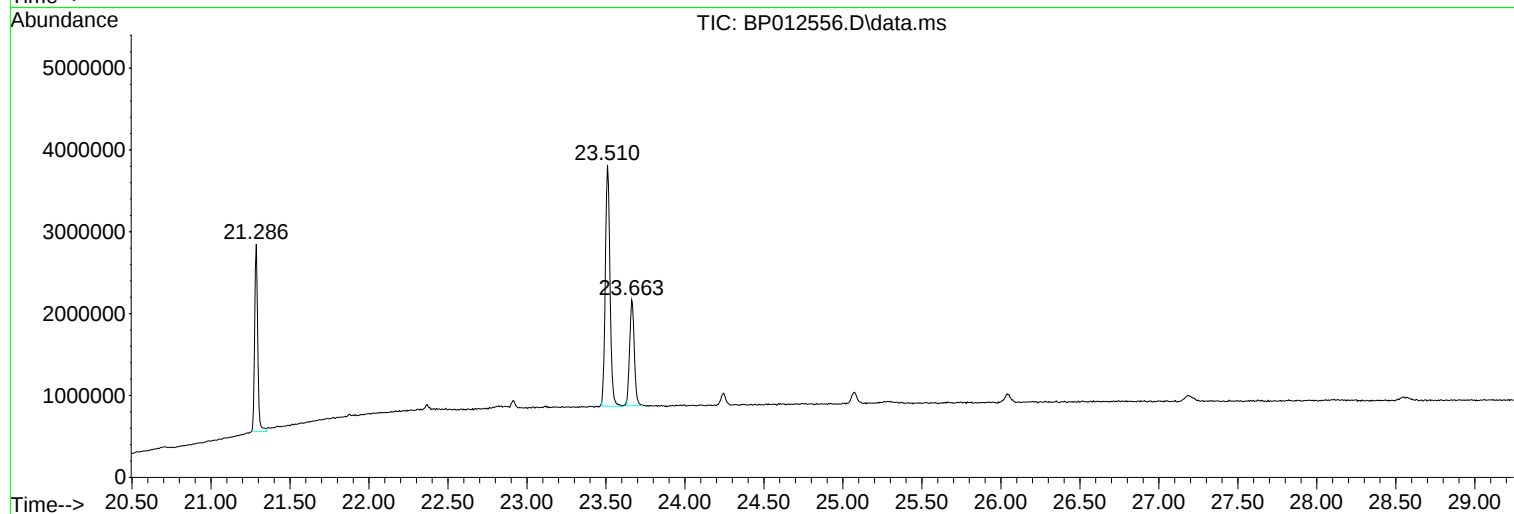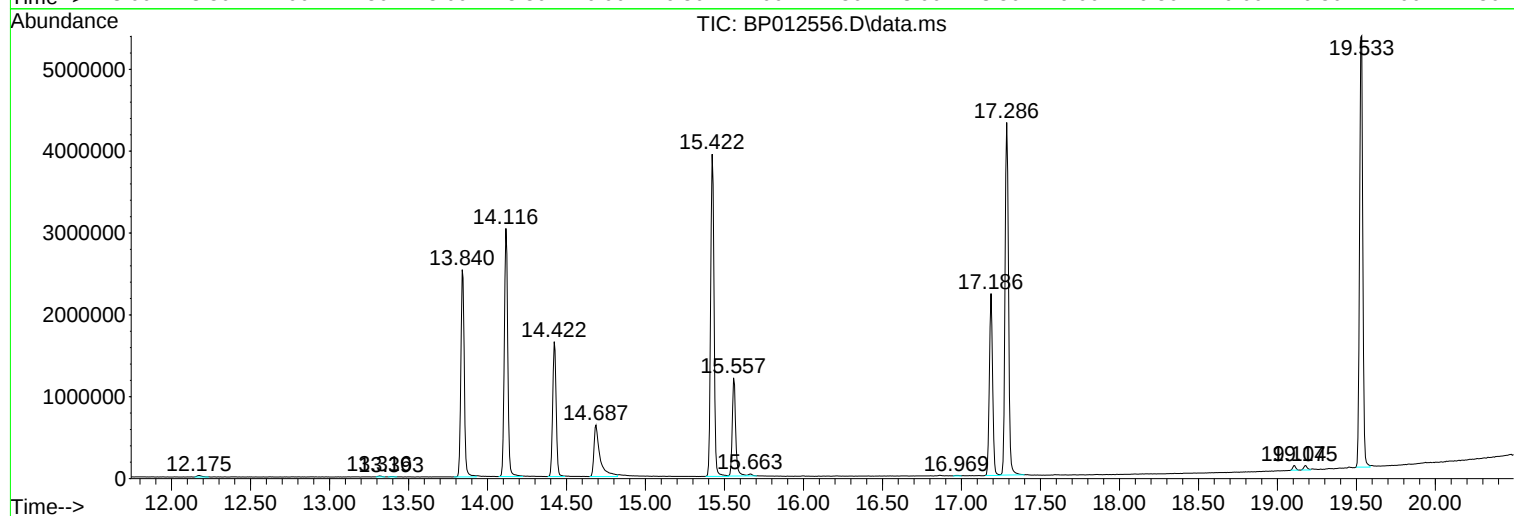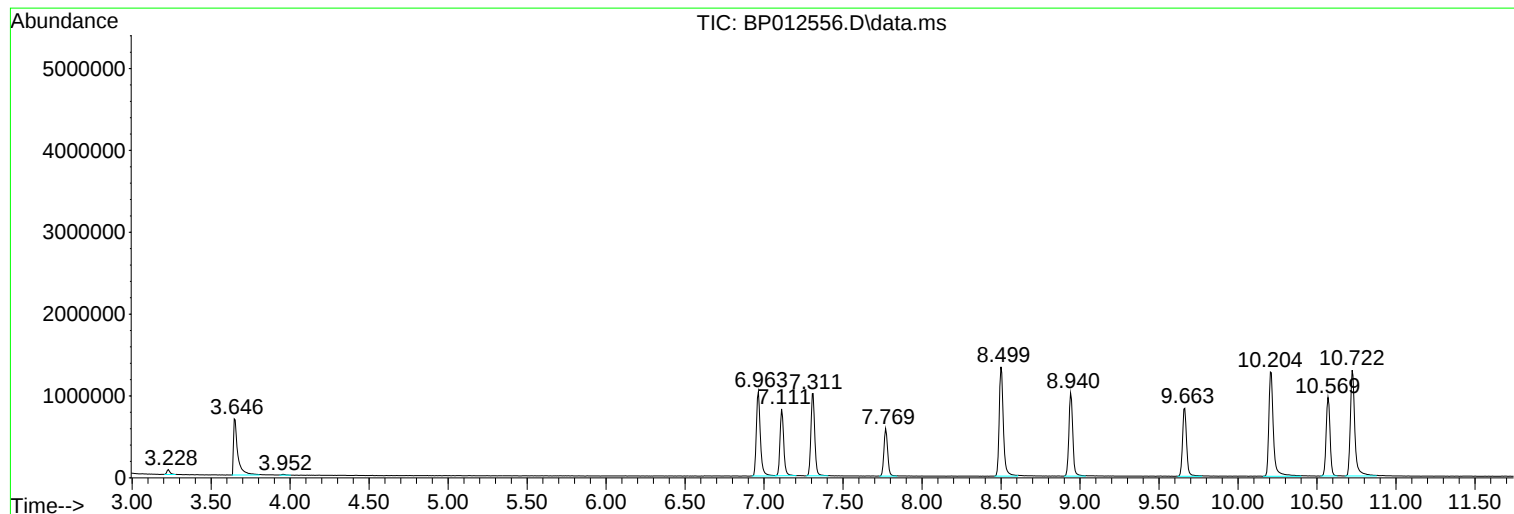

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110822\
Data File : BP012556.D
Acq On : 08 Nov 2022 18:08
Operator : CG/JU
Sample : PB148832BL
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK832

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110822\
Data File : BP012556.D
Acq On : 08 Nov 2022 18:08
Operator : CG/JU
Sample : PB148832BL
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK832

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc