

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110822\
 Data File : BP012557.D
 Acq On : 08 Nov 2022 18:42
 Operator : CG/JU
 Sample : PB148835BL
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK835

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
 Title : SVOA CALIBRATION

Signal : TIC: BP012557.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.228	37	41	53	rVB	68128	100433	1.19%	0.143%
2	3.658	111	114	137	rBV	211783	420613	4.98%	0.597%
3	3.958	162	165	171	rVB	11502	16257	0.19%	0.023%
4	6.963	669	676	694	rBV	1168910	2038538	24.14%	2.894%
5	7.110	695	701	717	rVB	901191	1468827	17.39%	2.085%
6	7.305	728	734	749	rBV	1126537	1891421	22.39%	2.685%
7	7.769	806	813	829	rBV	509923	835985	9.90%	1.187%
8	8.499	929	937	953	rBV	1543402	2680564	31.74%	3.805%
9	8.940	1005	1012	1032	rBV	1129983	1932828	22.88%	2.744%
10	9.663	1127	1135	1151	rBV	925704	1654647	19.59%	2.349%
11	10.204	1218	1227	1255	rBV	1359950	2827003	33.47%	4.013%
12	10.569	1282	1289	1301	rBV	863472	1440554	17.06%	2.045%
13	10.734	1310	1317	1334	rBV	89428	227466	2.69%	0.323%
14	12.175	1558	1562	1570	rBV	20951	41039	0.49%	0.058%
15	13.316	1752	1756	1761	rVV6	6992	10691	0.13%	0.015%
16	13.398	1765	1770	1775	rVB7	4544	8816	0.10%	0.013%
17	13.845	1836	1846	1859	rBV	2828382	4212348	49.87%	5.979%
18	14.116	1885	1892	1908	rBV	3364699	4987914	59.06%	7.080%
19	14.428	1937	1945	1963	rBV	1445513	2212662	26.20%	3.141%
20	14.681	1982	1988	2012	rBV	753132	1929211	22.84%	2.739%
21	15.422	2107	2114	2129	rBV	4361781	6576130	77.86%	9.335%
22	15.557	2131	2137	2151	rVV	1404254	2114088	25.03%	3.001%
23	15.663	2151	2155	2163	rVB	26392	51071	0.60%	0.072%
24	15.939	2197	2202	2207	rVB2	13939	20680	0.24%	0.029%
25	16.863	2355	2359	2363	rBV7	6121	8634	0.10%	0.012%
26	17.186	2407	2414	2424	rBV	1957253	2805337	33.21%	3.982%
27	17.286	2425	2431	2454	rVB2	4896700	7481697	88.58%	10.620%
28	19.104	2736	2740	2746	rBV	71406	117399	1.39%	0.167%
29	19.180	2749	2753	2757	rVV	55001	81048	0.96%	0.115%
30	19.533	2807	2813	2823	rBV	6031162	8446144	100.00%	11.989%
31	21.286	3106	3111	3123	rBV	2005378	2734894	32.38%	3.882%
32	23.510	3482	3489	3503	rBV2	3213263	6795136	80.45%	9.646%
33	23.663	3510	3515	3528	rVB2	1084642	2277397	26.96%	3.233%




Sum of corrected areas: 70447472

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110822\
Data File : BP012557.D
Acq On : 08 Nov 2022 18:42
Operator : CG/JU
Sample : PB148835BL
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK835

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

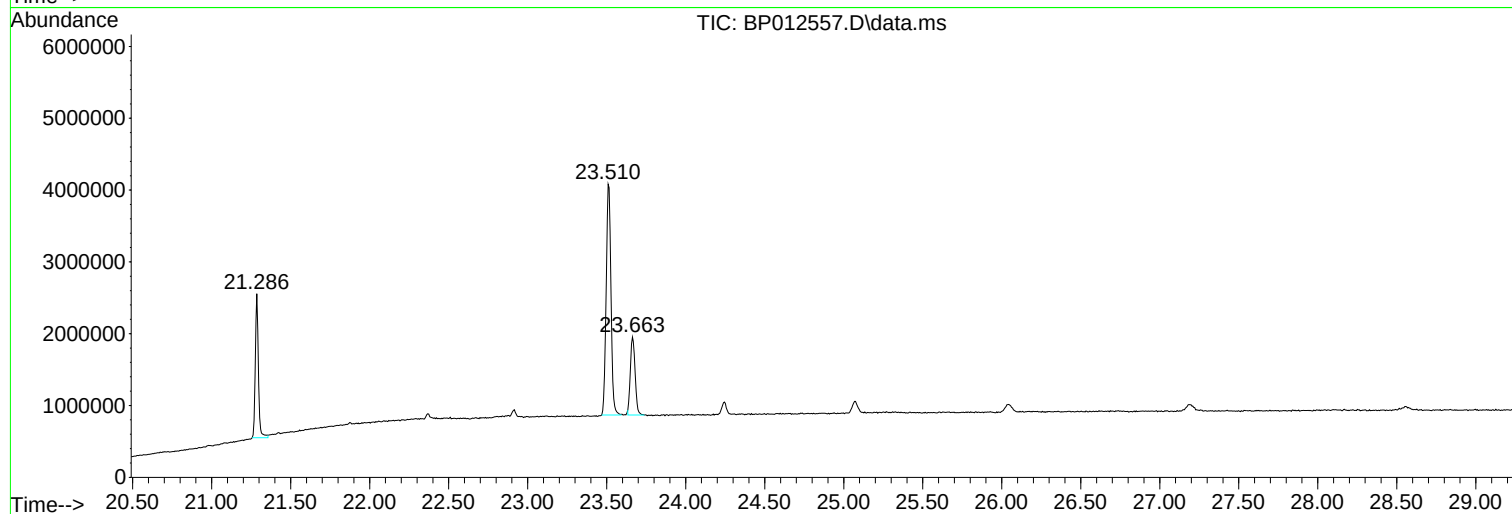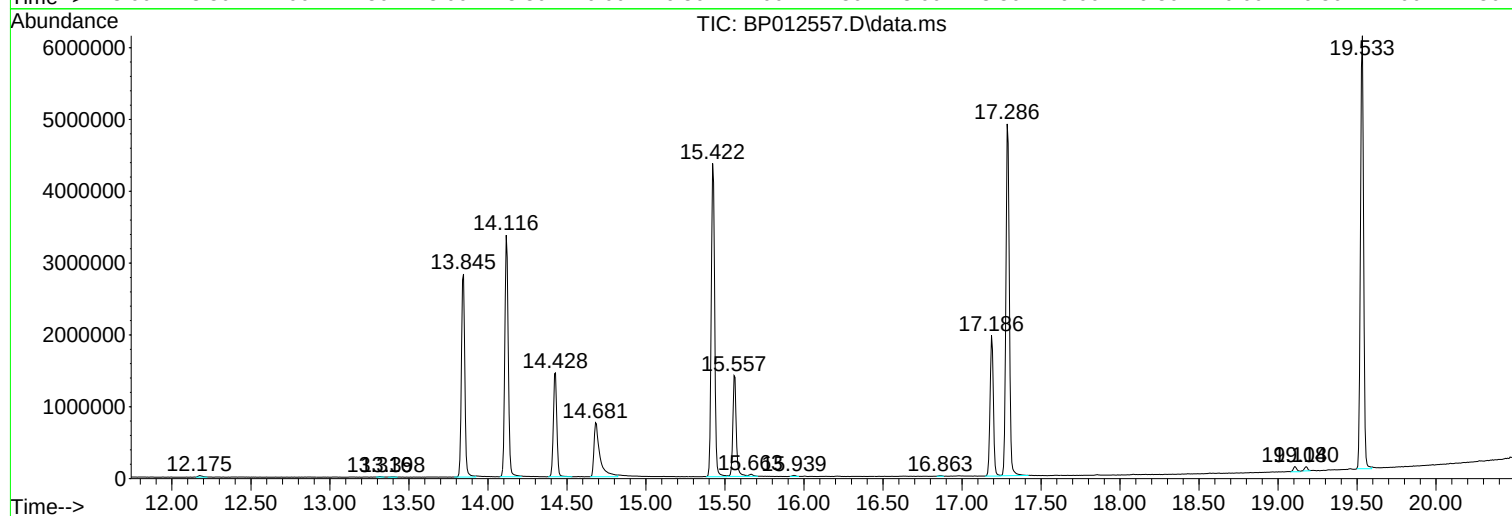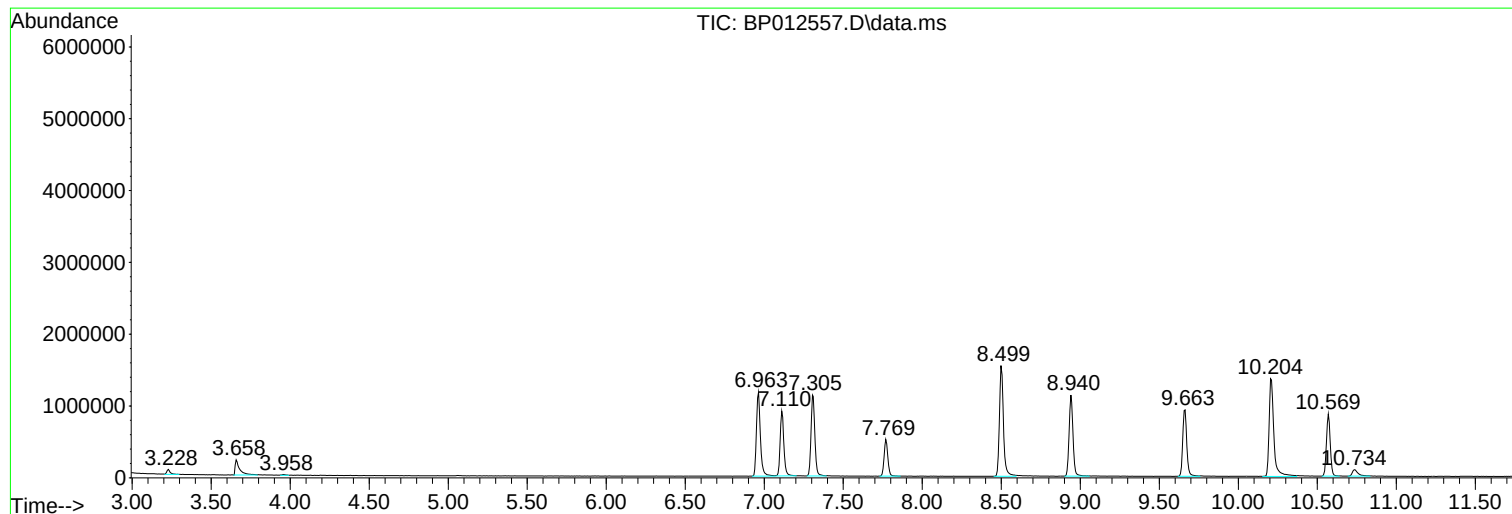

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110822\
Data File : BP012557.D
Acq On : 08 Nov 2022 18:42
Operator : CG/JU
Sample : PB148835BL
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK835

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110822\
Data File : BP012557.D
Acq On : 08 Nov 2022 18:42
Operator : CG/JU
Sample : PB148835BL
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK835

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc