

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110822\
 Data File : BP012560.D
 Acq On : 08 Nov 2022 20:25
 Operator : CG/JU
 Sample : N5407-04
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EW4Y4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
 Title : SVOA CALIBRATION

Signal : TIC: BP012560.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.228	37	41	52	rVB	48168	73169	0.70%	0.078%
2	3.652	111	113	133	rBV	263971	495738	4.77%	0.526%
3	3.864	144	149	154	rVB	20265	30726	0.30%	0.033%
4	3.958	161	165	172	rVB	17527	27729	0.27%	0.029%
5	6.963	669	676	690	rBV	245737	469140	4.51%	0.497%
6	7.110	694	701	716	rBV	974597	1577222	15.18%	1.672%
7	7.305	727	734	750	rBV	749829	1281117	12.33%	1.358%
8	7.769	806	813	821	rBV	953947	1565017	15.06%	1.659%
9	7.840	821	825	842	rVB	47778	102466	0.99%	0.109%
10	8.499	929	937	953	rBV	696406	1247344	12.00%	1.322%
11	8.940	1005	1012	1028	rBV	1213741	2094394	20.15%	2.220%
12	9.316	1072	1076	1082	rBV5	7994	12847	0.12%	0.014%
13	9.657	1126	1134	1146	rBV	842987	1506330	14.49%	1.597%
14	9.899	1167	1175	1177	rBV8	7954	16380	0.16%	0.017%
15	10.204	1220	1227	1248	rBV	1163358	2248050	21.63%	2.383%
16	10.569	1281	1289	1308	rBV	1591281	2758677	26.55%	2.924%
17	10.722	1308	1315	1337	rBV	1202780	2367836	22.78%	2.510%
18	11.404	1423	1431	1442	rBV6	16142	45087	0.43%	0.048%
19	12.169	1555	1561	1565	rBV2	23133	40565	0.39%	0.043%
20	13.028	1701	1707	1713	rBV10	5756	13097	0.13%	0.014%
21	13.393	1763	1769	1774	rVB6	6312	11927	0.11%	0.013%
22	13.640	1806	1811	1817	rBV	26522	46935	0.45%	0.050%
23	13.840	1835	1845	1858	rBV	3079094	4557055	43.85%	4.831%
24	14.116	1884	1892	1909	rBV2	3581093	5445115	52.40%	5.772%
25	14.422	1937	1944	1956	rBV	2718510	4193802	40.36%	4.446%
26	14.698	1985	1991	2004	rBV2	120758	320331	3.08%	0.340%
27	14.851	2012	2017	2028	rVB2	18005	51700	0.50%	0.055%
28	14.998	2037	2042	2043	rBV	21138	27065	0.26%	0.029%
29	15.257	2082	2086	2095	rVB2	39445	63647	0.61%	0.067%
30	15.422	2107	2114	2131	rBV	4866713	7103651	68.36%	7.530%
31	15.557	2131	2137	2150	rVV	1453452	2108673	20.29%	2.235%
32	15.663	2151	2155	2162	rVB3	30093	51341	0.49%	0.054%
33	16.134	2232	2235	2239	rBV4	11121	17395	0.17%	0.018%
34	16.592	2309	2313	2318	rBV8	15100	27500	0.26%	0.029%
35	16.933	2368	2371	2375	rBV4	10351	17329	0.17%	0.018%
36	17.186	2407	2414	2424	rBV	3607397	5205485	50.09%	5.518%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110822\
 Data File : BP012560.D
 Acq On : 08 Nov 2022 20:25
 Operator : CG/JU
 Sample : N5407-04
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EW4Y4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
 Title : SVOA CALIBRATION

37	17.286	2424	2431	2448	rVV	5734461	8359645	80.44%	8.862%
38	17.681	2494	2498	2501	rBV6	12364	20985	0.20%	0.022%
39	17.851	2524	2527	2532	rBV2	44704	54588	0.53%	0.058%
40	18.075	2561	2565	2573	rBV	212358	319304	3.07%	0.338%
41	18.145	2574	2577	2585	rVB4	35662	63873	0.61%	0.068%
42	19.104	2736	2740	2745	rBV2	92472	121123	1.17%	0.128%
43	19.175	2748	2752	2757	rBV	91327	159859	1.54%	0.169%
44	19.310	2772	2775	2783	rBV	142752	214734	2.07%	0.228%
45	19.451	2793	2799	2806	rBV	8695833	10392192	100.00%	11.016%
46	19.533	2807	2813	2829	rVB	6789326	9664645	93.00%	10.245%
47	21.286	3106	3111	3120	rBV	3859175	5057788	48.67%	5.361%
48	23.510	3482	3489	3503	rVB2	4072266	8222271	79.12%	8.716%
49	23.663	3509	3515	3525	rVB2	2207856	4462622	42.94%	4.731%




Sum of corrected areas: 94335511

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110822\
Data File : BP012560.D
Acq On : 08 Nov 2022 20:25
Operator : CG/JU
Sample : N5407-04
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EW4Y4

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

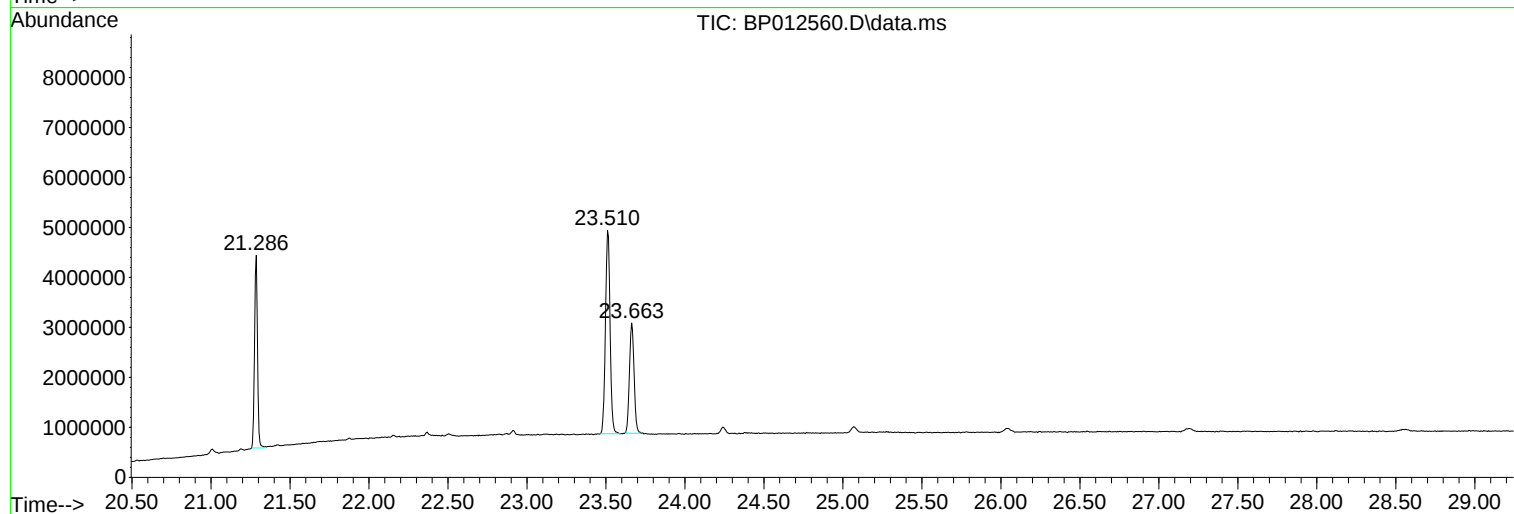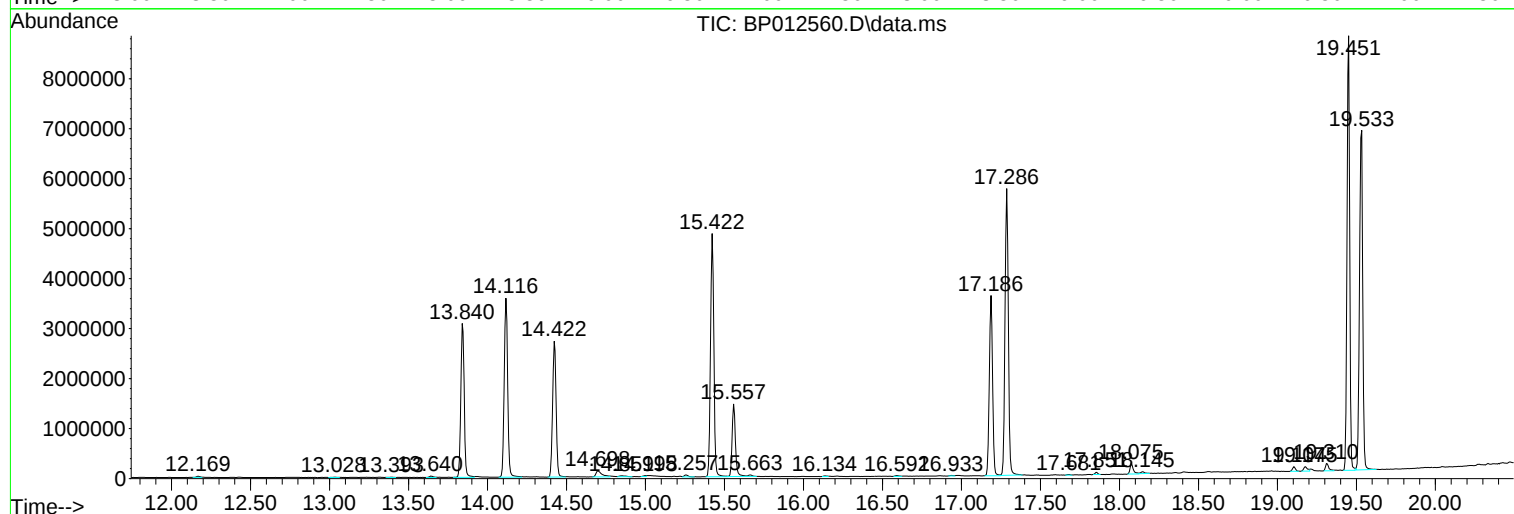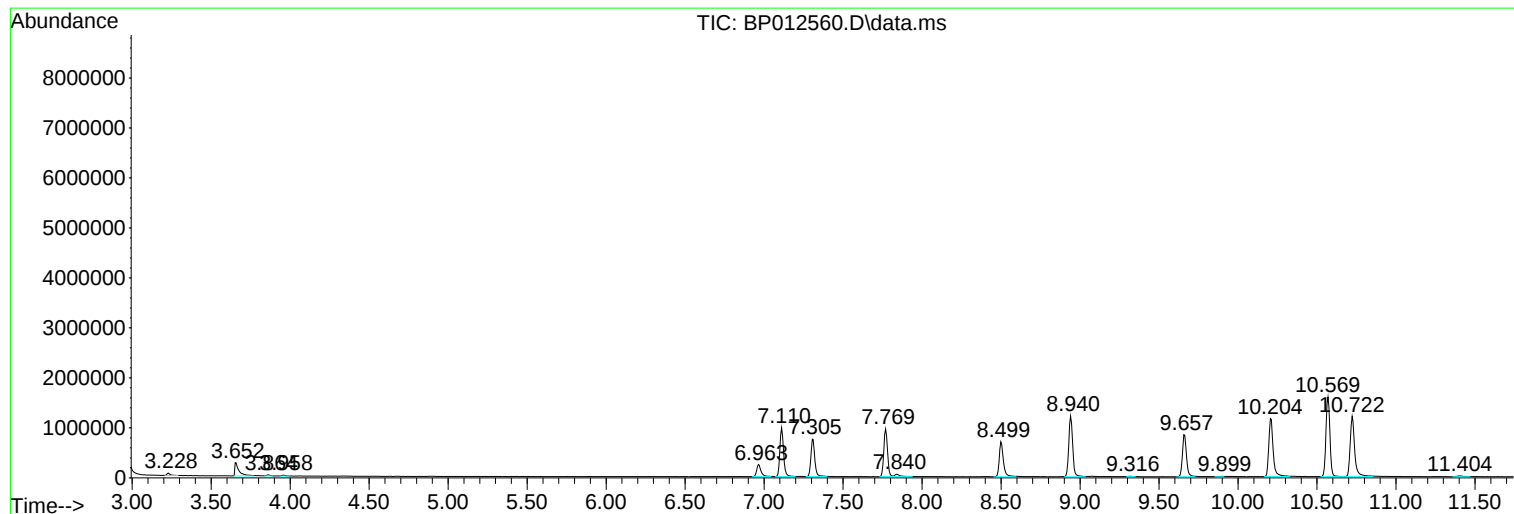

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110822\
Data File : BP012560.D
Acq On : 08 Nov 2022 20:25
Operator : CG/JU
Sample : N5407-04
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EW4Y4










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Butyl citrate Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
19.451	41.09 ng/ul	10392200	Chrysene-d12	21.286

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Butyl citrate	360	C18H32O7	000077-94-1	94
2			Butyl citrate	360	C18H32O7	000077-94-1	78
3			Adipic acid, butyl 2-methylpent-...	286	C16H30O4	1010353-55-8	72
4			O-Methyl-DL-serine, N-dimethylam...	230	C11H22N2O3	1000375-99-5	50
5			Adipic acid, butyl 2-hexyl ester	286	C16H30O4	1000353-71-0	38

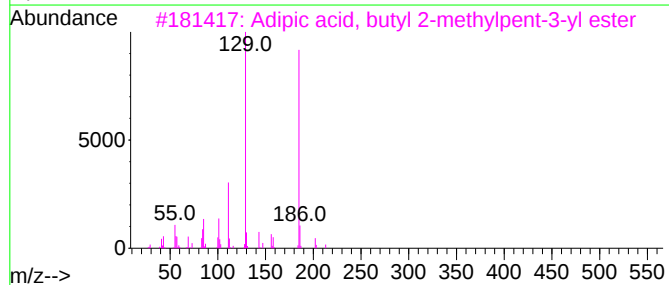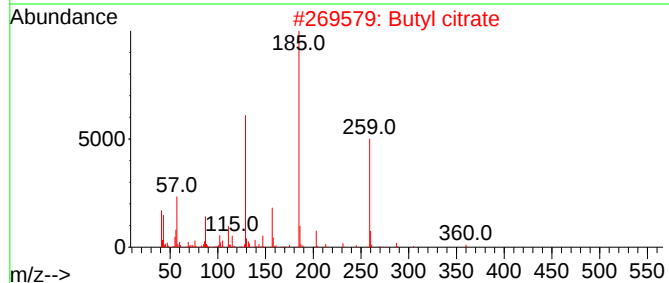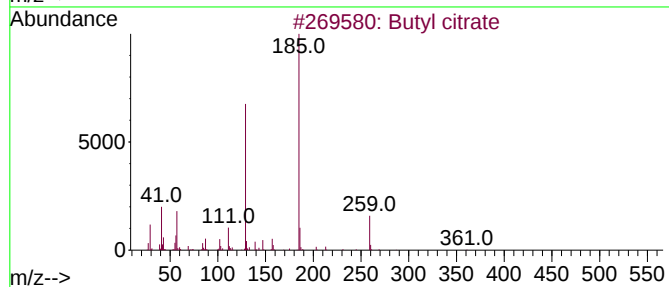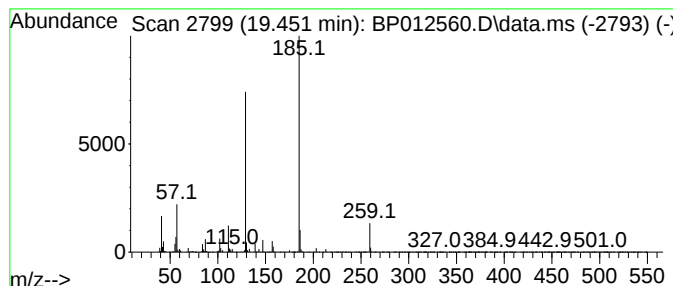

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110822\
Data File : BP012560.D
Acq On : 08 Nov 2022 20:25
Operator : CG/JU
Sample : N5407-04
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EW4Y4

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Butyl citrate	19.451	41.1	ng/ul	10392200	5	21.286	5057790	20.0