

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110822\
 Data File : BP012561.D
 Acq On : 08 Nov 2022 20:59
 Operator : CG/JU
 Sample : N5407-05
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EW4Y5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
 Title : SVOA CALIBRATION

Signal : TIC: BP012561.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.228	37	41	46	rBV	49512	62118	0.60%	0.064%
2	3.664	112	115	128	rBV	112847	226164	2.20%	0.232%
3	3.858	144	148	155	rVB	19065	30926	0.30%	0.032%
4	3.958	161	165	175	rVB	20411	30872	0.30%	0.032%
5	6.964	669	676	688	rBV	285021	521152	5.07%	0.535%
6	7.111	694	701	713	rBV	1041024	1679108	16.33%	1.724%
7	7.305	728	734	756	rBV	898494	1524422	14.83%	1.565%
8	7.769	806	813	821	rBV	940972	1538316	14.96%	1.579%
9	7.840	821	825	838	rVB	42137	87883	0.85%	0.090%
10	8.499	929	937	954	rBV	819850	1475076	14.35%	1.514%
11	8.940	1004	1012	1026	rBV	1347875	2281272	22.19%	2.342%
12	9.316	1070	1076	1083	rVB5	9851	19266	0.19%	0.020%
13	9.658	1127	1134	1152	rBV	1066010	1845080	17.95%	1.894%
14	10.205	1218	1227	1258	rBV	1427672	2726740	26.52%	2.799%
15	10.569	1281	1289	1305	rBV	1535537	2635764	25.64%	2.706%
16	10.722	1308	1315	1334	rBV	712888	1469574	14.29%	1.509%
17	11.410	1420	1432	1437	rBV	8891	24464	0.24%	0.025%
18	12.169	1555	1561	1573	rBV2	25135	59977	0.58%	0.062%
19	13.028	1702	1707	1714	rBV2	5868	16292	0.16%	0.017%
20	13.234	1735	1742	1746	rBV6	9139	16415	0.16%	0.017%
21	13.316	1751	1756	1763	rVV5	9903	20852	0.20%	0.021%
22	13.393	1763	1769	1778	rVB5	7875	17356	0.17%	0.018%
23	13.840	1838	1845	1859	rBV	3663802	5207496	50.65%	5.346%
24	14.116	1884	1892	1909	rBV	4225135	6244647	60.74%	6.411%
25	14.422	1937	1944	1958	rBV	2741539	4017600	39.08%	4.125%
26	14.698	1985	1991	2011	rBV	128516	395025	3.84%	0.406%
27	15.222	2076	2080	2082	rBV	13462	16919	0.16%	0.017%
28	15.257	2082	2086	2092	rVB2	23036	34555	0.34%	0.035%
29	15.422	2107	2114	2131	rBV	5420661	8196944	79.72%	8.416%
30	15.557	2131	2137	2150	rVV	1681514	2461083	23.94%	2.527%
31	15.663	2152	2155	2160	rVB2	29567	44392	0.43%	0.046%
32	16.592	2309	2313	2317	rBV6	12728	19737	0.19%	0.020%
33	16.975	2376	2378	2387	rVB8	9226	15968	0.16%	0.016%
34	17.187	2406	2414	2424	rBV	3487994	4984993	48.48%	5.118%
35	17.287	2424	2431	2453	rVB2	6064277	9210786	89.58%	9.456%
36	17.857	2525	2528	2533	rVB6	14608	17726	0.17%	0.018%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110822\
 Data File : BP012561.D
 Acq On : 08 Nov 2022 20:59
 Operator : CG/JU
 Sample : N5407-05
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EW4Y5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
 Title : SVOA CALIBRATION

37	17.957	2542	2545	2547	rBV3	11378	13568	0.13%	0.014%
38	18.075	2560	2565	2573	rBV	215795	333710	3.25%	0.343%
39	18.145	2574	2577	2583	rVB2	43031	65214	0.63%	0.067%
40	19.104	2736	2740	2747	rBV2	85430	116800	1.14%	0.120%
41	19.175	2748	2752	2758	rBV	95017	187799	1.83%	0.193%
42	19.310	2772	2775	2783	rBV	166009	235480	2.29%	0.242%
43	19.451	2794	2799	2806	rBV	7123830	8608601	83.73%	8.838%
44	19.533	2806	2813	2822	rVB	7213039	10281678	100.00%	10.556%
45	21.286	3106	3111	3119	rBV	3714494	4781418	46.50%	4.909%
46	23.510	3482	3489	3505	rVB2	4415392	9275773	90.22%	9.523%
47	23.663	3509	3515	3526	rVB2	2135980	4325592	42.07%	4.441%


Sum of corrected areas: 97402593

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110822\
Data File : BP012561.D
Acq On : 08 Nov 2022 20:59
Operator : CG/JU
Sample : N5407-05
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EW4Y5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

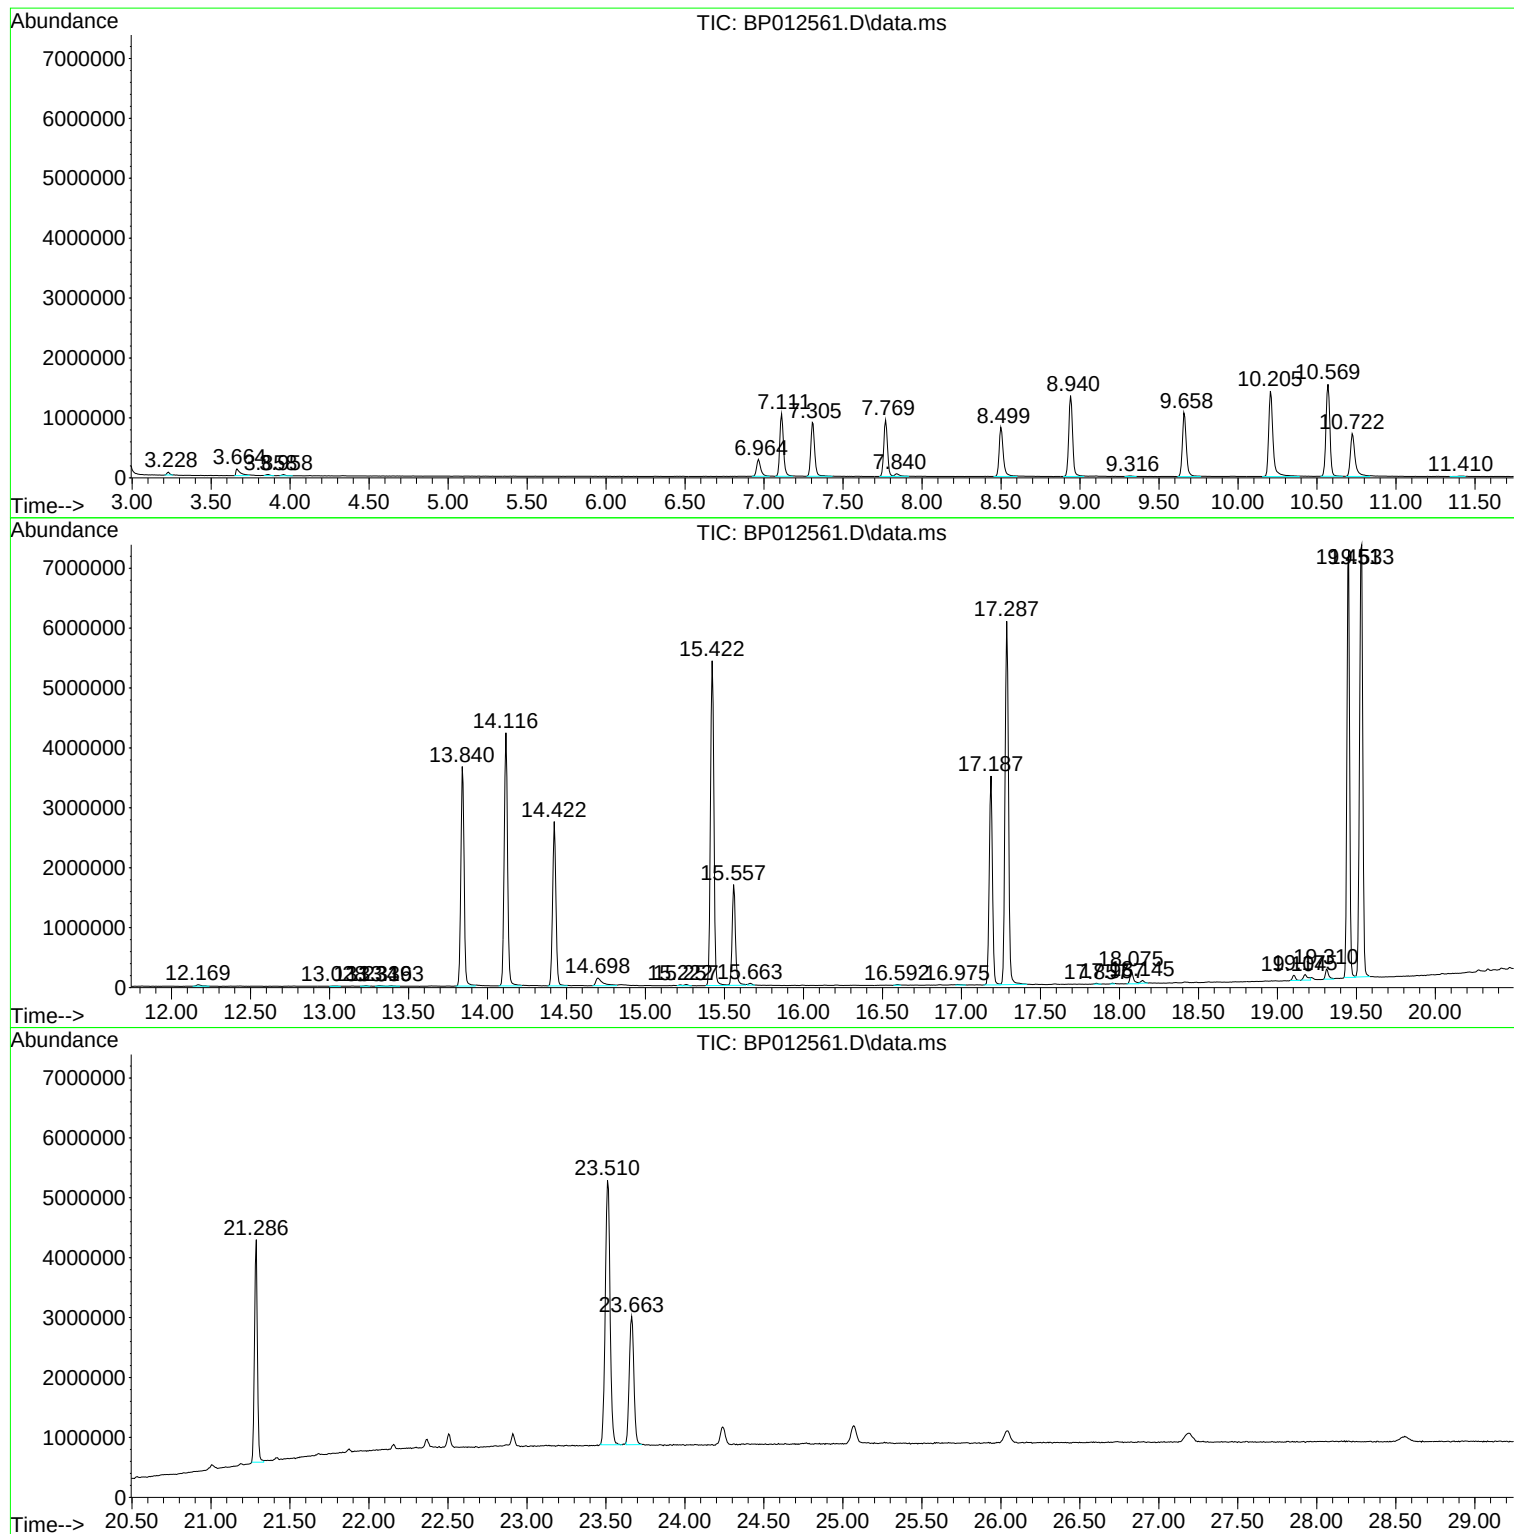

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110822\
Data File : BP012561.D
Acq On : 08 Nov 2022 20:59
Operator : CG/JU
Sample : N5407-05
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EW4Y5










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Butyl citrate Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
19.451	36.01 ng/ul	8608600	Chrysene-d12	21.286

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Butyl citrate	360	C18H32O7	000077-94-1	91
2			Adipic acid, butyl 3-pentyl ester	272	C15H28O4	1000324-60-5	72
3			Adipic acid, 2-decyl isobutyl ester	342	C20H38O4	1000353-59-6	64
4			Butyl citrate	360	C18H32O7	000077-94-1	64
5			Adipic acid, cycloheptyl isobuty...	298	C17H30O4	1000324-71-5	53

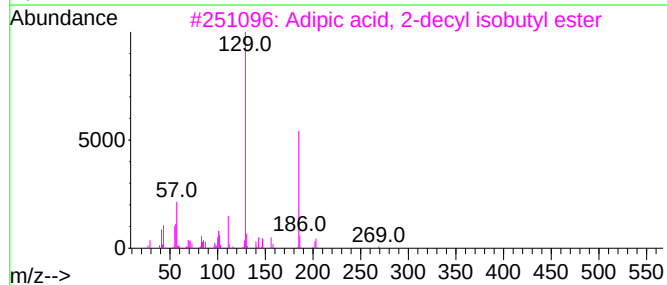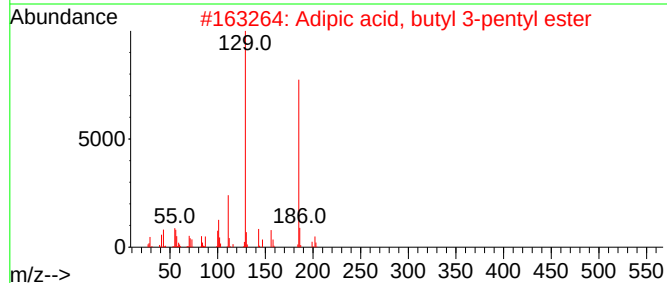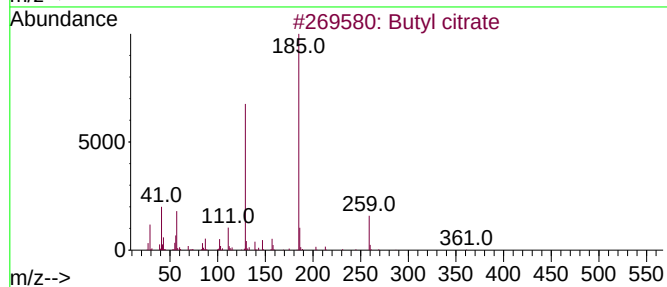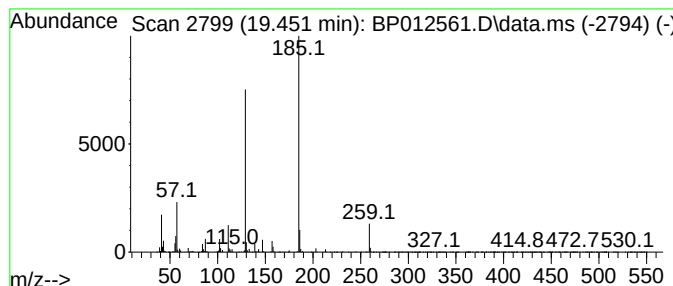

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110822\
Data File : BP012561.D
Acq On : 08 Nov 2022 20:59
Operator : CG/JU
Sample : N5407-05
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EW4Y5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Butyl citrate	19.451	36.0	ng/ul	8608600	5	21.286	4781420	20.0