

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110822\
 Data File : BP012566.D
 Acq On : 08 Nov 2022 23:49
 Operator : CG/JU
 Sample : N5407-16
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EW4Z3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
 Title : SVOA CALIBRATION

Signal : TIC: BP012566.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.228	37	41	52	rVB	43795	67173	0.72%	0.088%
2	3.658	112	114	138	rBV	165902	347109	3.74%	0.456%
3	3.858	144	148	159	rVB2	17307	35306	0.38%	0.046%
4	3.958	161	165	169	rVB	15376	18826	0.20%	0.025%
5	6.964	670	676	689	rBV	190185	346403	3.73%	0.455%
6	7.111	694	701	720	rVV	779188	1309917	14.11%	1.719%
7	7.305	727	734	749	rBV	715345	1228095	13.23%	1.612%
8	7.769	805	813	822	rBV	844074	1416303	15.25%	1.859%
9	8.499	931	937	954	rBV	624201	1150448	12.39%	1.510%
10	8.940	1004	1012	1028	rBV	989744	1733634	18.67%	2.275%
11	9.657	1126	1134	1150	rBV	785816	1356605	14.61%	1.780%
12	10.205	1220	1227	1248	rBV	1128218	2135198	23.00%	2.802%
13	10.569	1281	1289	1301	rBV	1432655	2476010	26.67%	3.249%
14	10.722	1307	1315	1342	rBV	823701	1696454	18.27%	2.226%
15	11.410	1428	1432	1435	rBV5	5839	10587	0.11%	0.014%
16	12.169	1555	1561	1570	rBV2	18300	36920	0.40%	0.048%
17	13.316	1750	1756	1761	rBV5	10708	16774	0.18%	0.022%
18	13.393	1763	1769	1773	rBV8	5809	10311	0.11%	0.014%
19	13.840	1837	1845	1863	rBV	2737799	3976873	42.83%	5.219%
20	14.116	1884	1892	1919	rBV	3125442	4744460	51.10%	6.227%
21	14.422	1937	1944	1959	rBV	2521949	3767791	40.58%	4.945%
22	14.698	1985	1991	2011	rBV2	87735	282803	3.05%	0.371%
23	14.845	2012	2016	2019	rVV5	11062	24023	0.26%	0.032%
24	14.869	2019	2020	2026	rVB5	12867	17412	0.19%	0.023%
25	15.004	2037	2043	2049	rBV5	12191	34072	0.37%	0.045%
26	15.422	2107	2114	2131	rBV	4058391	6222122	67.01%	8.166%
27	15.557	2131	2137	2151	rVV	1385024	2079926	22.40%	2.730%
28	15.663	2151	2155	2165	rVB5	24980	51472	0.55%	0.068%
29	16.592	2309	2313	2318	rBV7	13667	21557	0.23%	0.028%
30	17.186	2407	2414	2424	rBV	3221405	4705695	50.68%	6.176%
31	17.286	2424	2431	2448	rVV	5325494	7766621	83.65%	10.193%
32	17.851	2524	2527	2533	rVB7	24752	32842	0.35%	0.043%
33	17.957	2541	2545	2550	rBV8	17168	31220	0.34%	0.041%
34	18.075	2561	2565	2575	rBV	141604	236979	2.55%	0.311%
35	19.104	2736	2740	2745	rBV	79188	105123	1.13%	0.138%
36	19.175	2748	2752	2757	rBV	74744	122289	1.32%	0.160%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110822\
Data File : BP012566.D
Acq On : 08 Nov 2022 23:49
Operator : CG/JU
Sample : N5407-16
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EW4Z3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
Title : SVOA CALIBRATION

37	19.310	2772	2775	2785	rBV3	73250	113809	1.23%	0.149%
38	19.451	2796	2799	2803	rBV4	28999	38223	0.41%	0.050%
39	19.528	2806	2812	2827	rVV	6756187	9284916	100.00%	12.185%
40	21.280	3105	3110	3119	rBV	3619509	4876820	52.52%	6.400%
41	23.510	3481	3489	3500	rBV2	3874035	8013206	86.30%	10.516%
42	23.663	3508	3515	3526	rVB2	2010566	4254904	45.83%	5.584%




Sum of corrected areas: 76197231

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110822\
Data File : BP012566.D
Acq On : 08 Nov 2022 23:49
Operator : CG/JU
Sample : N5407-16
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EW4Z3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

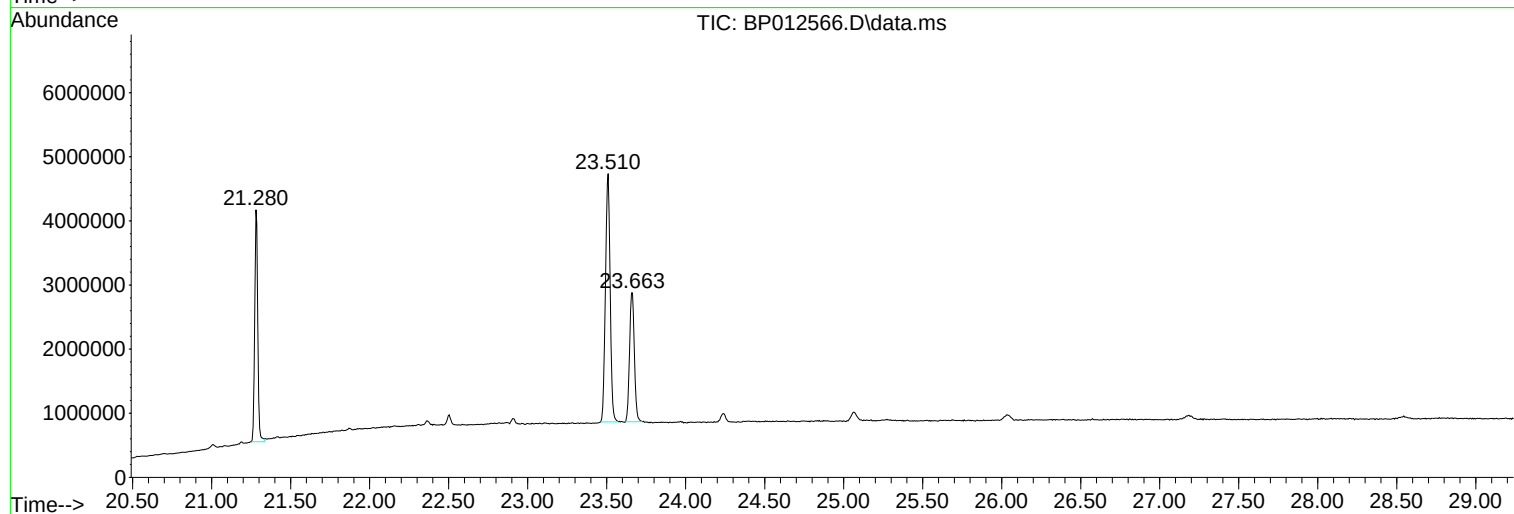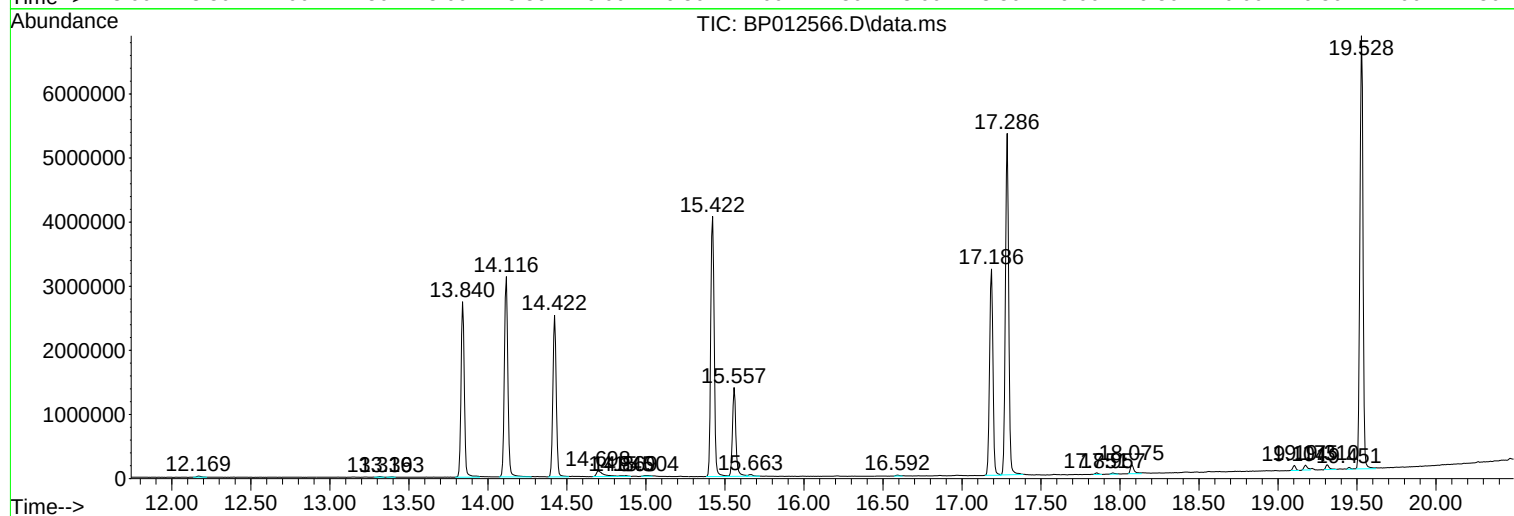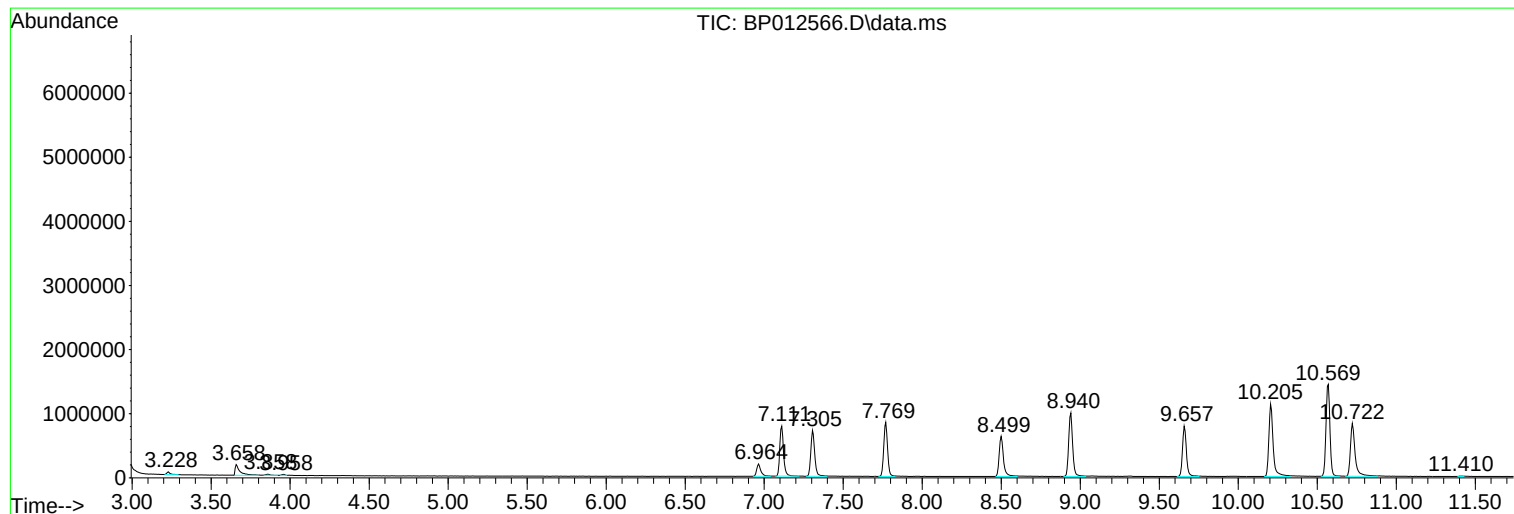

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110822\
Data File : BP012566.D
Acq On : 08 Nov 2022 23:49
Operator : CG/JU
Sample : N5407-16
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EW4Z3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110822\
Data File : BP012566.D
Acq On : 08 Nov 2022 23:49
Operator : CG/JU
Sample : N5407-16
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EW4Z3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc
