

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110822\
 Data File : BP012572.D
 Acq On : 09 Nov 2022 03:13
 Operator : CG/JU
 Sample : N5455-02
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BFZ12

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
 Title : SVOA CALIBRATION

Signal : TIC: BP012572.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.222	37	40	54	rVB2	36783	73671	0.85%	0.107%
2	3.669	115	116	128	rBV	60945	122703	1.41%	0.179%
3	3.858	144	148	156	rVB3	13929	27422	0.31%	0.040%
4	3.958	161	165	171	rVB	15350	25518	0.29%	0.037%
5	4.475	249	253	259	rVB8	6944	11634	0.13%	0.017%
6	4.899	320	325	338	rBV	13858	25481	0.29%	0.037%
7	6.963	669	676	689	rBV	316407	590738	6.78%	0.860%
8	7.110	694	701	721	rVB	737951	1268699	14.56%	1.848%
9	7.305	727	734	751	rBV	853975	1428700	16.40%	2.081%
10	7.769	805	813	824	rBV	618360	1051465	12.07%	1.531%
11	8.499	929	937	953	rBV	896598	1586575	18.21%	2.311%
12	8.940	1003	1012	1029	rBV	969350	1687461	19.37%	2.458%
13	9.075	1031	1035	1048	rVB	5223	17918	0.21%	0.026%
14	9.657	1127	1134	1150	rBV	791520	1391670	15.98%	2.027%
15	10.204	1220	1227	1256	rBV	1139164	2324943	26.69%	3.386%
16	10.563	1280	1288	1304	rBV	1069642	1853344	21.28%	2.699%
17	10.734	1310	1317	1339	rVB	120126	301200	3.46%	0.439%
18	12.175	1555	1562	1570	rBV	17286	35934	0.41%	0.052%
19	13.310	1750	1755	1760	rBV6	9797	16513	0.19%	0.024%
20	13.839	1832	1845	1858	rBV	2810447	4035887	46.33%	5.878%
21	14.110	1884	1891	1908	rBV	2929470	4613125	52.96%	6.719%
22	14.422	1937	1944	1954	rBV	1920139	2878295	33.04%	4.192%
23	14.704	1985	1992	2005	rBV2	72445	240057	2.76%	0.350%
24	14.869	2017	2020	2026	rVB8	9181	17840	0.20%	0.026%
25	15.422	2106	2114	2131	rBV	4150682	6392804	73.38%	9.311%
26	15.557	2131	2137	2151	rVV	1262522	1884126	21.63%	2.744%
27	15.663	2151	2155	2167	rVB3	27916	61400	0.70%	0.089%
28	17.180	2407	2413	2424	rBV	2426663	3656376	41.97%	5.325%
29	17.286	2424	2431	2450	rVB	4882478	7555608	86.73%	11.004%
30	18.075	2561	2565	2571	rBV2	55845	88979	1.02%	0.130%
31	19.104	2736	2740	2745	rBV	73245	95630	1.10%	0.139%
32	19.174	2748	2752	2757	rVV	60491	87164	1.00%	0.127%
33	19.310	2772	2775	2783	rBV2	61769	102551	1.18%	0.149%
34	19.527	2806	2812	2822	rBV	6443733	8711355	100.00%	12.688%
35	21.280	3106	3110	3119	rBV	2861514	3691519	42.38%	5.376%
36	23.504	3481	3488	3502	rVB2	3723227	7420797	85.19%	10.808%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110822\
Data File : BP012572.D
Acq On : 09 Nov 2022 03:13
Operator : CG/JU
Sample : N5455-02
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BFZ12

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
Title : SVOA CALIBRATION

37	23.657	3508	3514	3526	rVB2	1643367	3285201	37.71%	4.785%
----	--------	------	------	------	------	---------	---------	--------	--------




Sum of corrected areas: 68660303

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110822\
Data File : BP012572.D
Acq On : 09 Nov 2022 03:13
Operator : CG/JU
Sample : N5455-02
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BFZ12

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

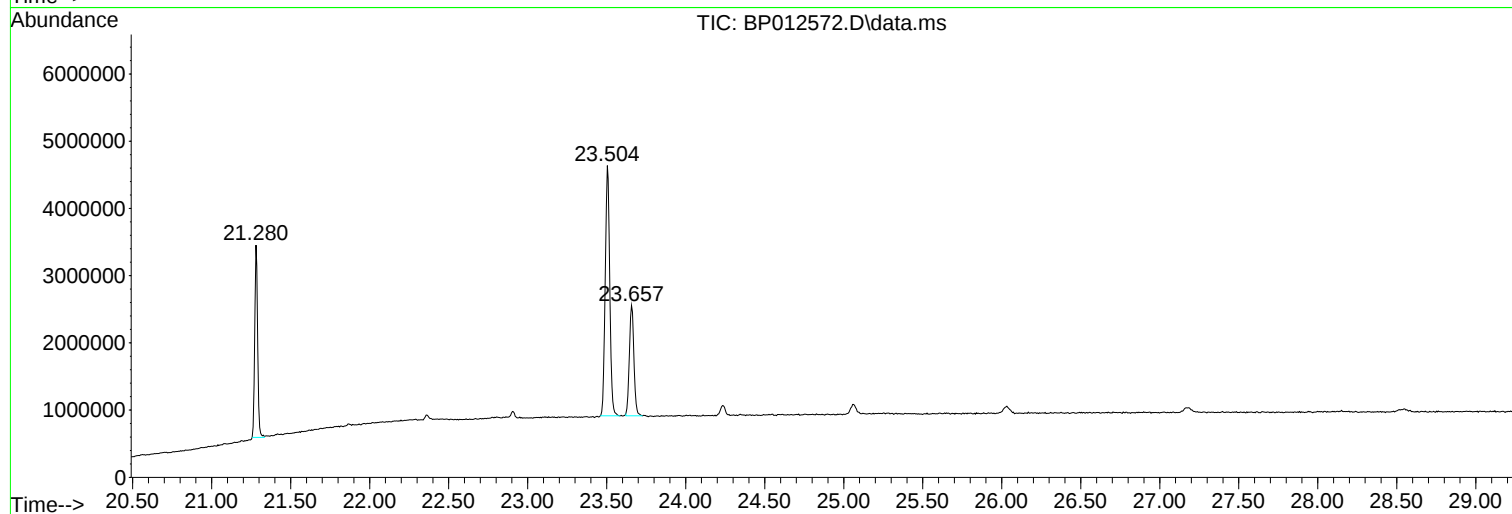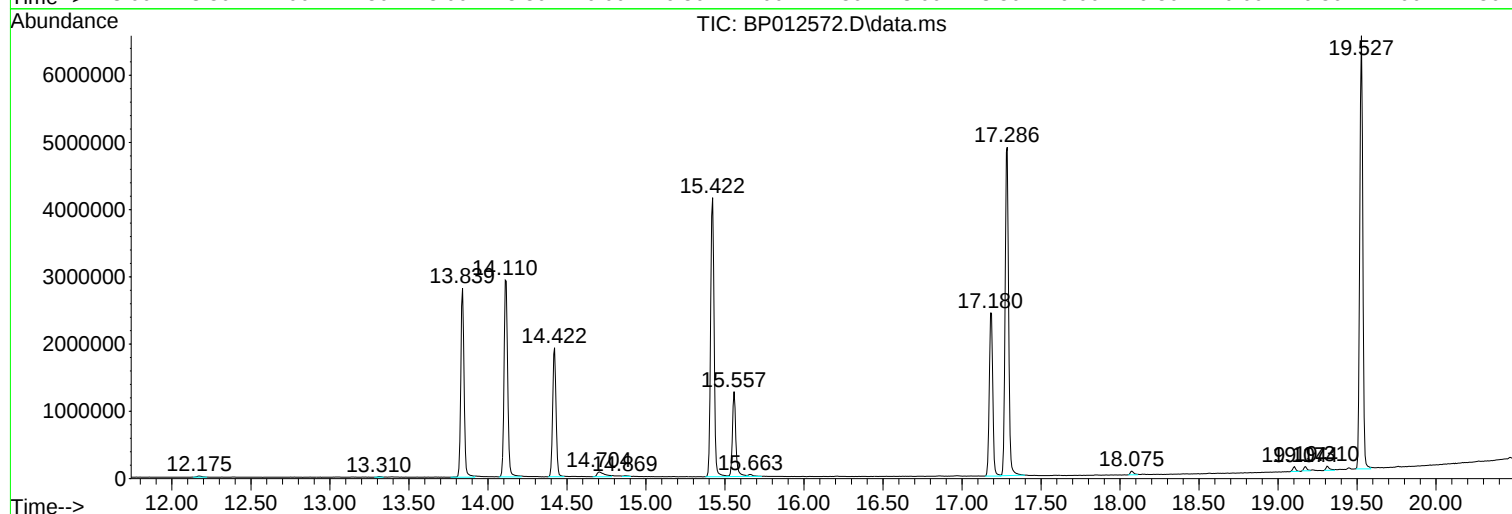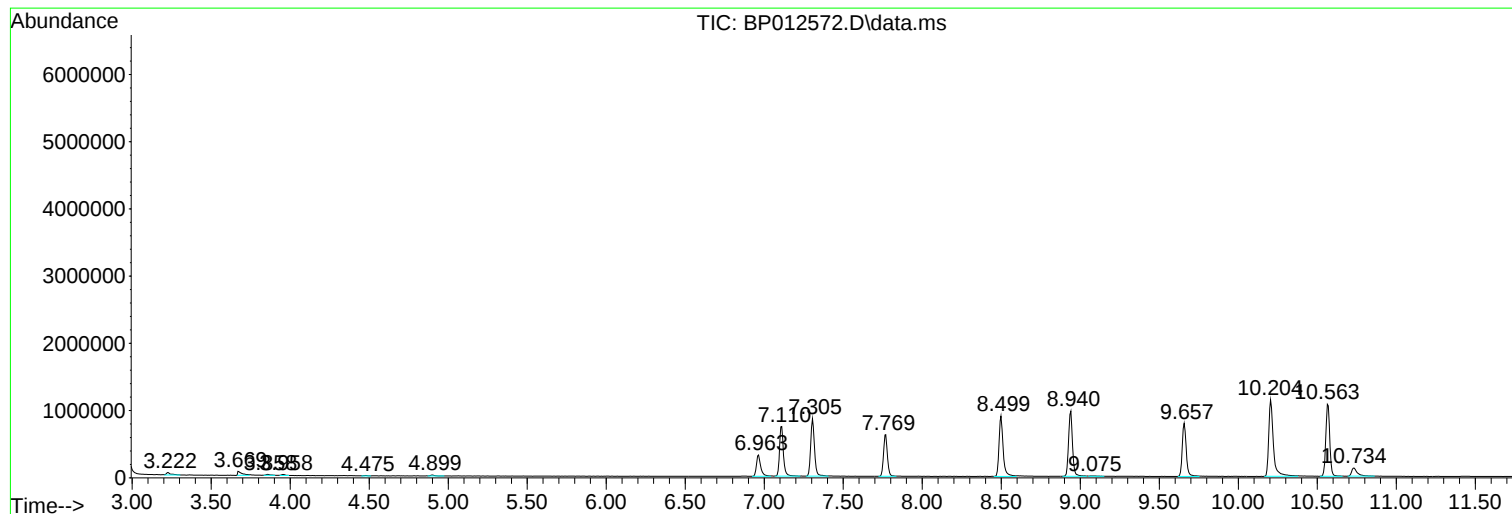

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110822\
Data File : BP012572.D
Acq On : 09 Nov 2022 03:13
Operator : CG/JU
Sample : N5455-02
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BFZ12

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110822\
Data File : BP012572.D
Acq On : 09 Nov 2022 03:13
Operator : CG/JU
Sample : N5455-02
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BFZ12

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc