

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110822\
 Data File : BP012580.D
 Acq On : 09 Nov 2022 09:05
 Operator : CG/JU
 Sample : PB148832BL
 Misc :
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK832

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
 Title : SVOA CALIBRATION

Signal : TIC: BP012580.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.228	37	41	51	rVB	52749	79493	1.00%	0.105%
2	3.652	111	113	138	rBV	318927	651268	8.23%	0.857%
3	3.958	161	165	171	rVB	14162	22122	0.28%	0.029%
4	6.963	669	676	693	rBV	967572	1702860	21.52%	2.241%
5	7.110	694	701	716	rVB	772029	1264227	15.97%	1.663%
6	7.310	728	735	753	rBV	945347	1602437	20.25%	2.108%
7	7.769	806	813	825	rBV	797722	1316988	16.64%	1.733%
8	8.499	930	937	955	rBV	1270898	2291477	28.95%	3.015%
9	8.940	1005	1012	1032	rBV	974043	1680864	21.24%	2.212%
10	9.663	1127	1135	1152	rBV	812639	1421327	17.96%	1.870%
11	10.210	1220	1228	1260	rBV	1231405	2448457	30.94%	3.222%
12	10.569	1279	1289	1305	rBV	1352244	2352684	29.73%	3.096%
13	10.728	1309	1316	1345	rVV	818415	1772639	22.40%	2.332%
14	12.175	1558	1562	1571	rBV2	17213	36600	0.46%	0.048%
15	13.398	1766	1770	1777	rVB7	4990	9404	0.12%	0.012%
16	13.845	1835	1846	1860	rBV	2600439	3749747	47.38%	4.934%
17	14.122	1885	1893	1910	rBV	2947965	4527178	57.20%	5.957%
18	14.428	1935	1945	1964	rBV	2423768	3708233	46.86%	4.879%
19	14.687	1982	1989	2012	rBV	638134	1704745	21.54%	2.243%
20	15.428	2108	2115	2132	rVV	3883044	5912115	74.70%	7.779%
21	15.563	2132	2138	2152	rVV	1205499	1790973	22.63%	2.356%
22	15.663	2152	2155	2163	rVB4	25243	45860	0.58%	0.060%
23	16.216	2244	2249	2252	rBV6	7049	9637	0.12%	0.013%
24	16.981	2374	2379	2383	rBV5	8551	15642	0.20%	0.021%
25	17.186	2408	2414	2425	rBV	3086345	4744637	59.95%	6.243%
26	17.292	2425	2432	2453	rVB	4495177	6868048	86.78%	9.037%
27	19.110	2737	2741	2747	rBV3	62480	91304	1.15%	0.120%
28	19.180	2749	2753	2757	rBV2	58116	80861	1.02%	0.106%
29	19.457	2797	2800	2806	rBV7	19351	27331	0.35%	0.036%
30	19.533	2807	2813	2827	rBV	5903026	7914025	100.00%	10.413%
31	21.286	3106	3111	3122	rBV	3712085	4894311	61.84%	6.440%
32	23.515	3483	3490	3503	rVB	3354550	6956946	87.91%	9.154%
33	23.668	3509	3516	3528	rVB2	2094308	4307710	54.43%	5.668%




Sum of corrected areas: 76002150

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110822\
Data File : BP012580.D
Acq On : 09 Nov 2022 09:05
Operator : CG/JU
Sample : PB148832BL
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK832

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

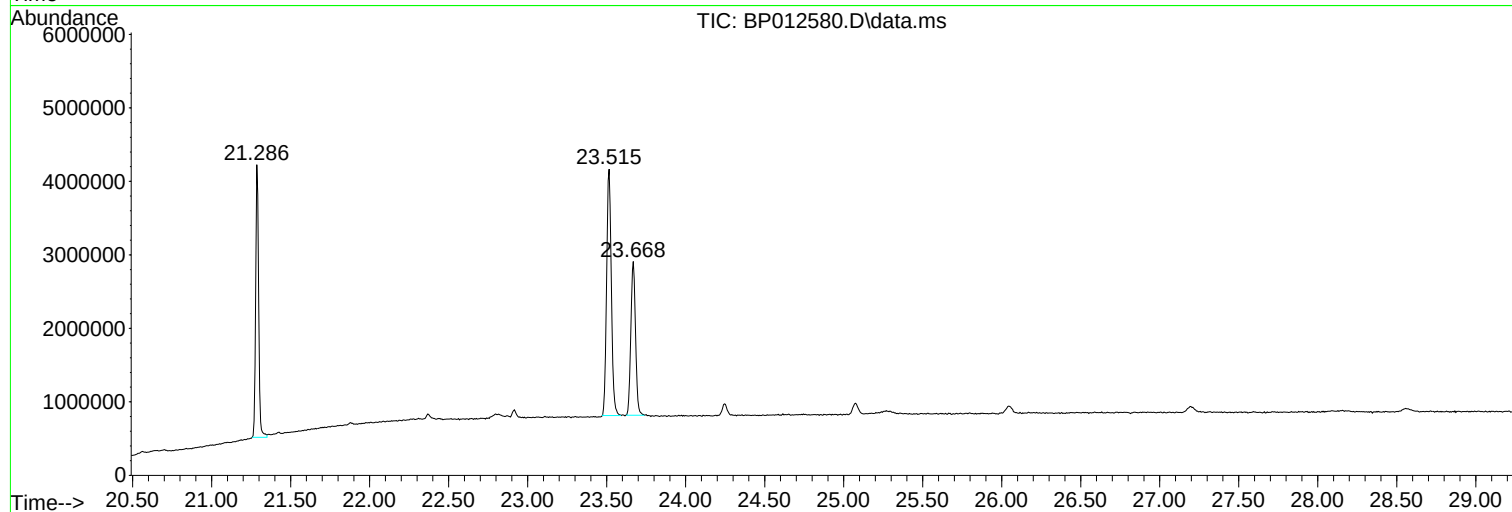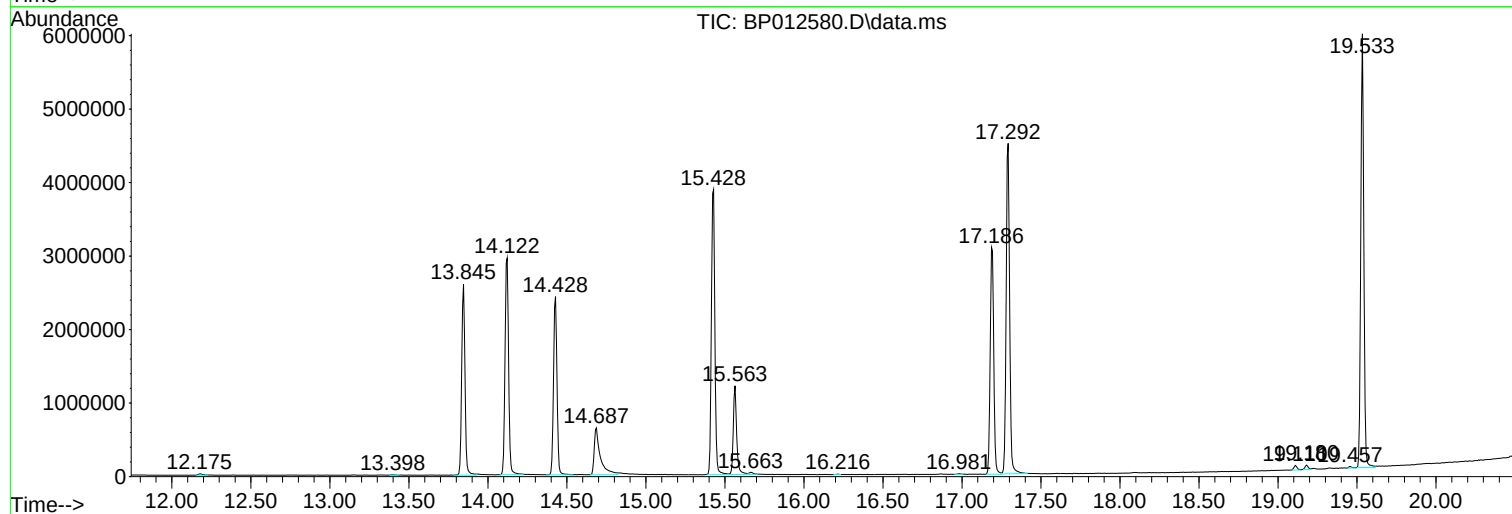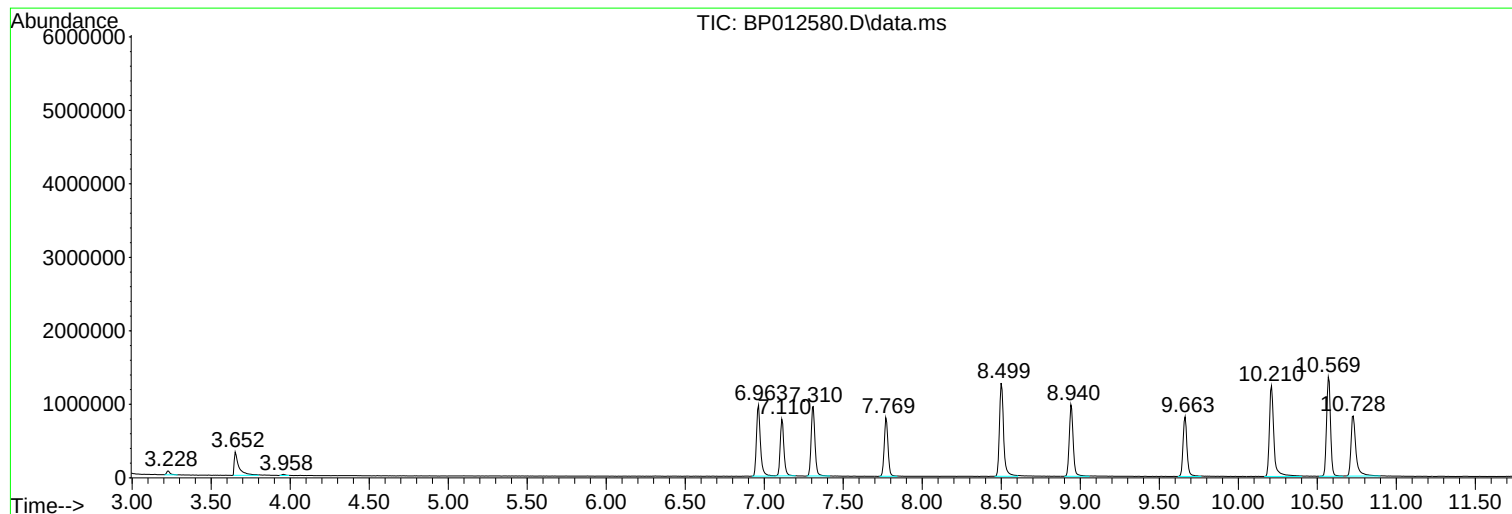

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110822\
Data File : BP012580.D
Acq On : 09 Nov 2022 09:05
Operator : CG/JU
Sample : PB148832BL
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK832

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110822\
Data File : BP012580.D
Acq On : 09 Nov 2022 09:05
Operator : CG/JU
Sample : PB148832BL
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK832

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc