

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110822\
 Data File : BP012583.D
 Acq On : 09 Nov 2022 11:01
 Operator : CG/JU
 Sample : N5407-06
 Misc :
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EW4Y6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
 Title : SVOA CALIBRATION

Signal : TIC: BP012583.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.228	38	41	49	rVB	29206	39837	0.68%	0.067%
2	3.663	114	115	125	rBV	81847	160644	2.74%	0.269%
3	3.958	162	165	170	rVB2	11299	14938	0.25%	0.025%
4	6.963	669	676	695	rBV	661700	1179368	20.12%	1.976%
5	7.110	695	701	716	rVB	552263	939762	16.03%	1.575%
6	7.310	728	735	749	rBV	681476	1166984	19.90%	1.955%
7	7.769	806	813	825	rBV	752778	1281323	21.85%	2.147%
8	8.499	930	937	956	rBV	886048	1631055	27.82%	2.733%
9	8.940	1004	1012	1026	rBV	698354	1241125	21.17%	2.080%
10	9.310	1065	1075	1076	rBV9	2827	6138	0.10%	0.010%
11	9.663	1126	1135	1153	rBV	573221	1018301	17.37%	1.706%
12	10.210	1221	1228	1249	rBV	890967	1770972	30.21%	2.967%
13	10.569	1281	1289	1306	rBV	1324679	2266263	38.65%	3.797%
14	10.728	1309	1316	1345	rVV	836698	1808120	30.84%	3.030%
15	11.945	1516	1523	1531	rBV7	7685	18785	0.32%	0.031%
16	13.398	1764	1770	1777	rVB7	3437	7055	0.12%	0.012%
17	13.845	1835	1846	1859	rBV	1867789	2808269	47.90%	4.706%
18	14.116	1885	1892	1907	rBV	2186187	3390202	57.82%	5.681%
19	14.428	1938	1945	1964	rBV	2315392	3546808	60.50%	5.943%
20	14.692	1984	1990	2007	rBV	308314	932159	15.90%	1.562%
21	15.422	2108	2114	2128	rBV	2874403	4406889	75.17%	7.384%
22	15.563	2132	2138	2152	rVV	779232	1169677	19.95%	1.960%
23	15.669	2152	2156	2170	rVB2	35344	64699	1.10%	0.108%
24	16.216	2245	2249	2254	rVB6	9116	13652	0.23%	0.023%
25	16.869	2356	2360	2363	rBV6	6194	8962	0.15%	0.015%
26	16.980	2376	2379	2385	rVB	6318	9661	0.16%	0.016%
27	17.186	2408	2414	2425	rBV	3034876	4498273	76.72%	7.537%
28	17.286	2425	2431	2452	rVB2	3151199	4956942	84.55%	8.306%
29	17.857	2525	2528	2534	rVB7	7637	11060	0.19%	0.019%
30	18.080	2562	2566	2574	rBV3	39132	71840	1.23%	0.120%
31	19.451	2795	2799	2806	rVB	176780	207125	3.53%	0.347%
32	19.533	2807	2813	2823	rBV	4304472	5862916	100.00%	9.824%
33	21.286	3106	3111	3123	rBV	3358152	4477087	76.36%	7.502%
34	23.515	3483	3490	3506	rVB	2255742	4889161	83.39%	8.192%
35	23.668	3510	3516	3526	rVB2	1872570	3803900	64.88%	6.374%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110822\
Data File : BP012583.D
Acq On : 09 Nov 2022 11:01
Operator : CG/JU
Sample : N5407-06
Misc :
ALS Vial : 42 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EW4Y6

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
Title : SVOA CALIBRATION




Sum of corrected areas: 59679952

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110822\
Data File : BP012583.D
Acq On : 09 Nov 2022 11:01
Operator : CG/JU
Sample : N5407-06
Misc :
ALS Vial : 42 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EW4Y6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

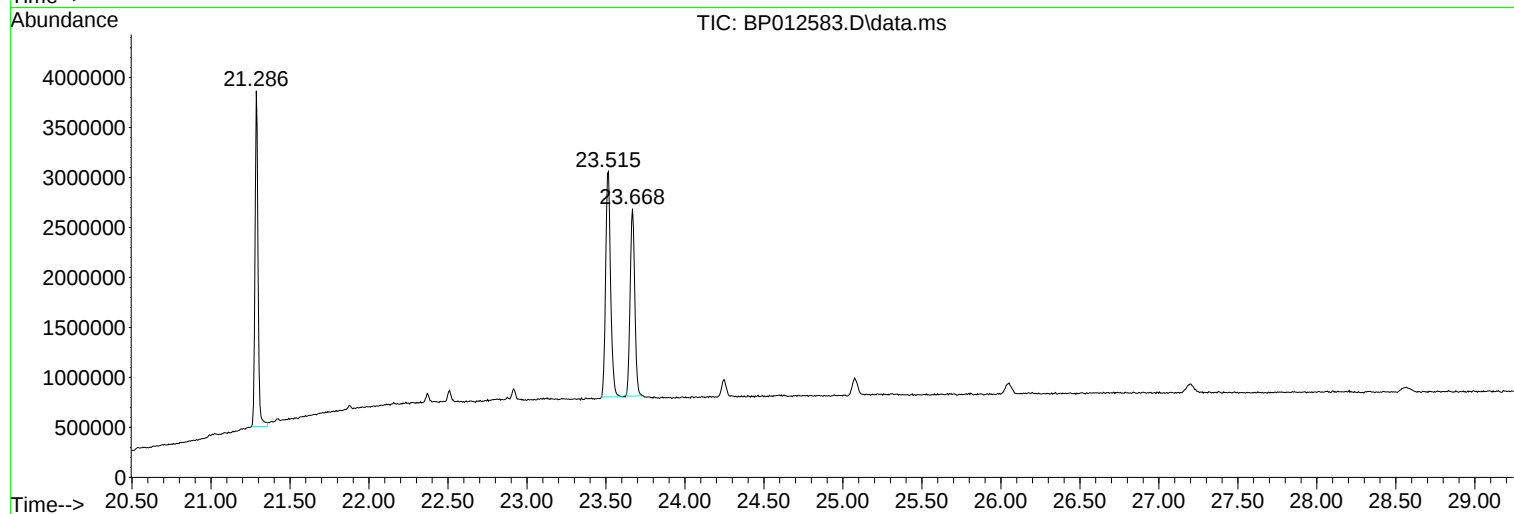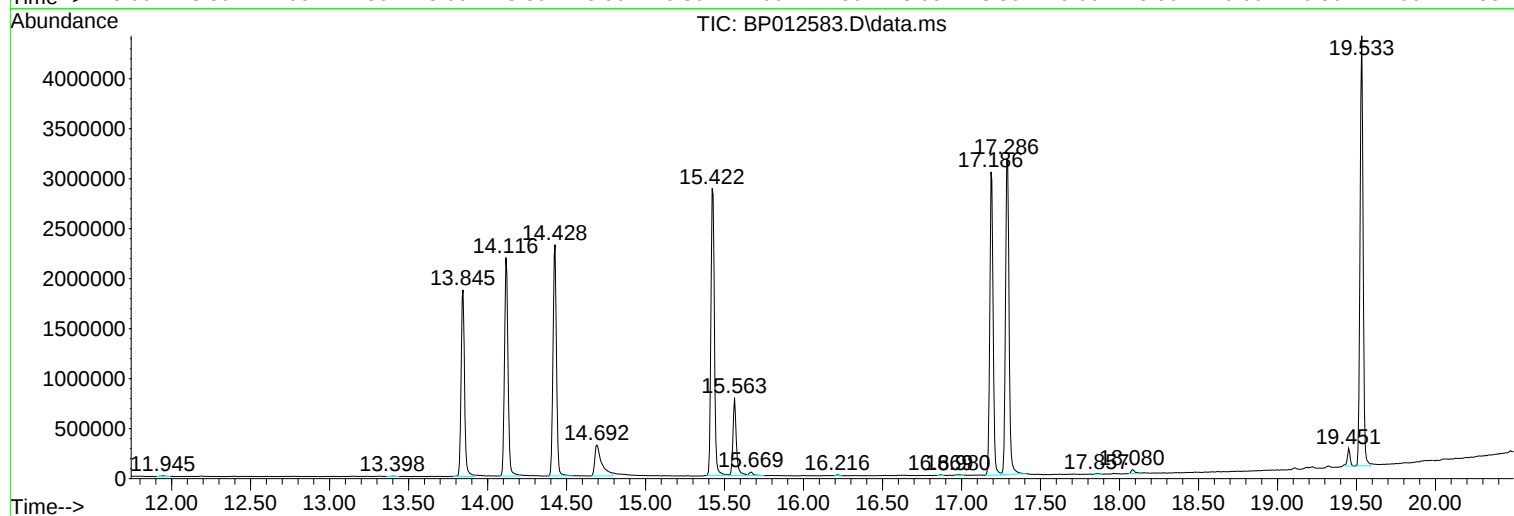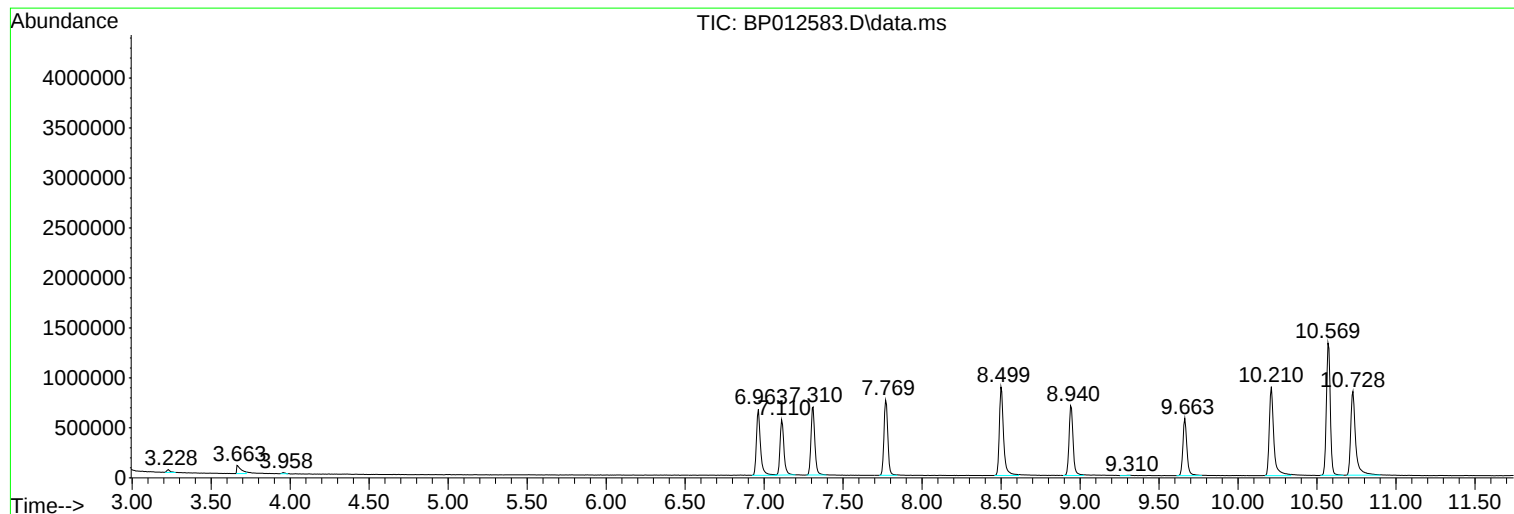

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110822\
Data File : BP012583.D
Acq On : 09 Nov 2022 11:01
Operator : CG/JU
Sample : N5407-06
Misc :
ALS Vial : 42 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EW4Y6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110822\
Data File : BP012583.D
Acq On : 09 Nov 2022 11:01
Operator : CG/JU
Sample : N5407-06
Misc :
ALS Vial : 42 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EW4Y6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc