
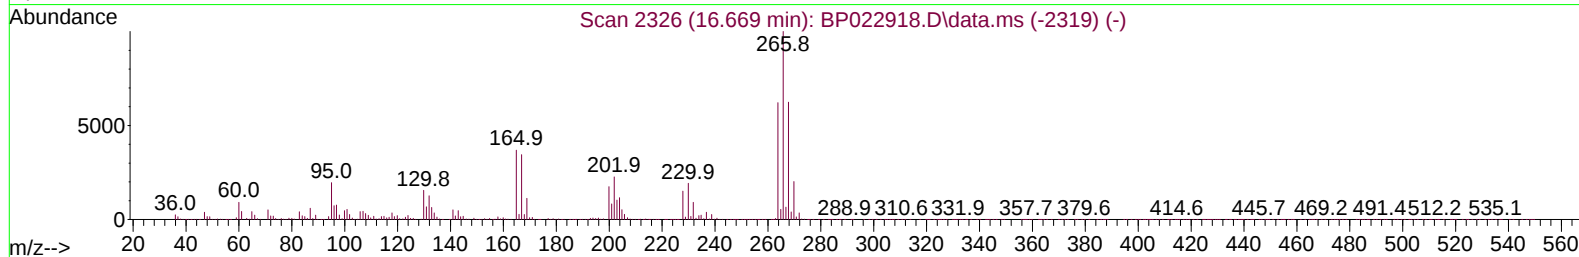
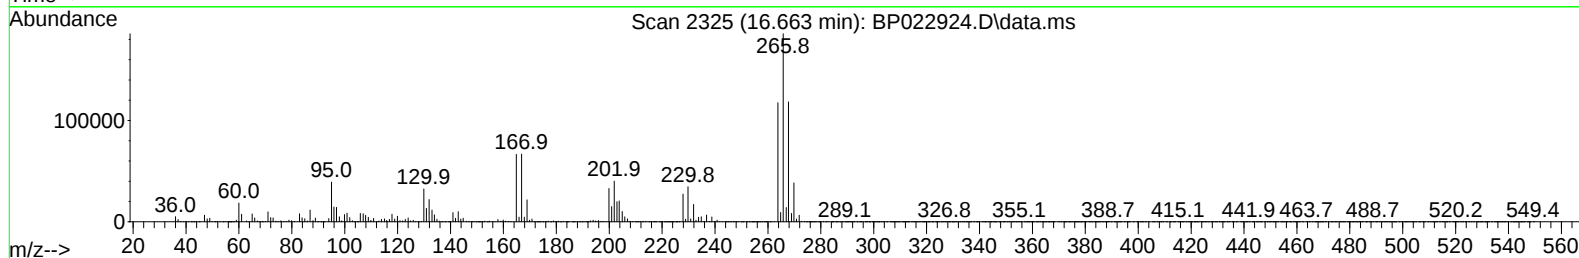


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110824\
Data File : BP022924.D
Acq On : 08 Nov 2024 07:13
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 09 04:03:48 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP110724.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 07 23:36:11 2024
Response via : Initial Calibration

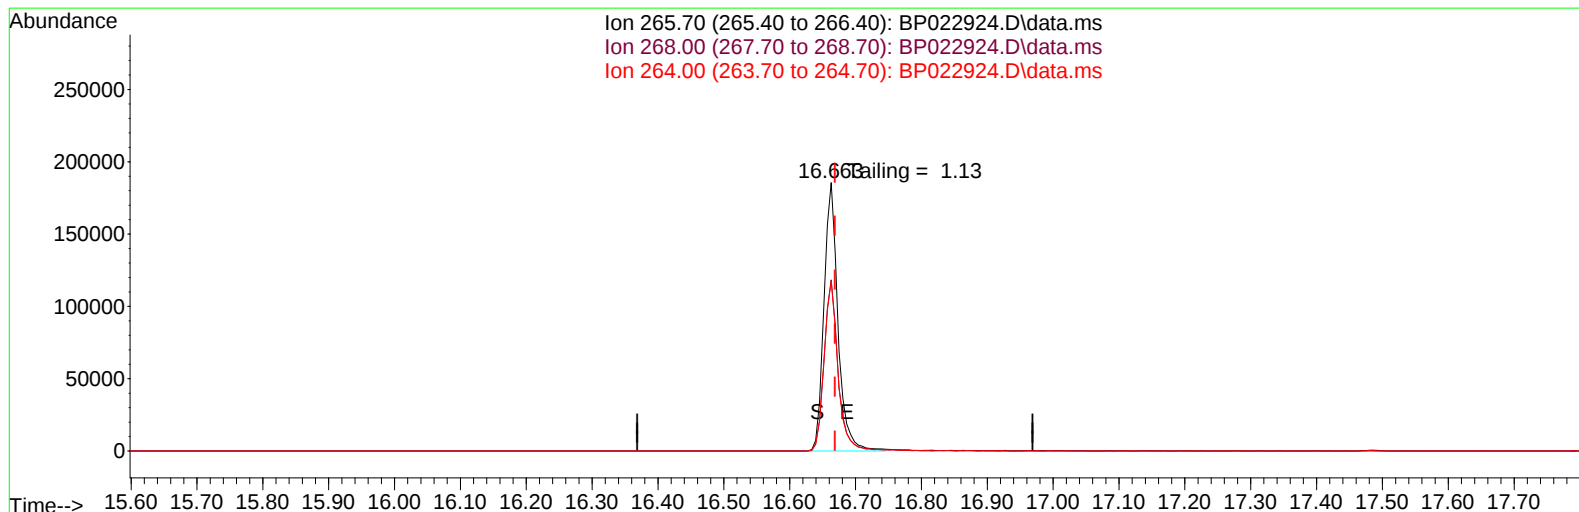

TIC: BP022924.D\data.ms

(70) Pentachlorophenol (C)




16.663min (-0.006) 2009783.57 ng

response 276055

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.40	63.75
264.00	62.10	63.36
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110824\
Data File : BP022924.D
Acq On : 08 Nov 2024 07:13
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 09 04:03:48 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP110724.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 07 23:36:11 2024
Response via : Initial Calibration

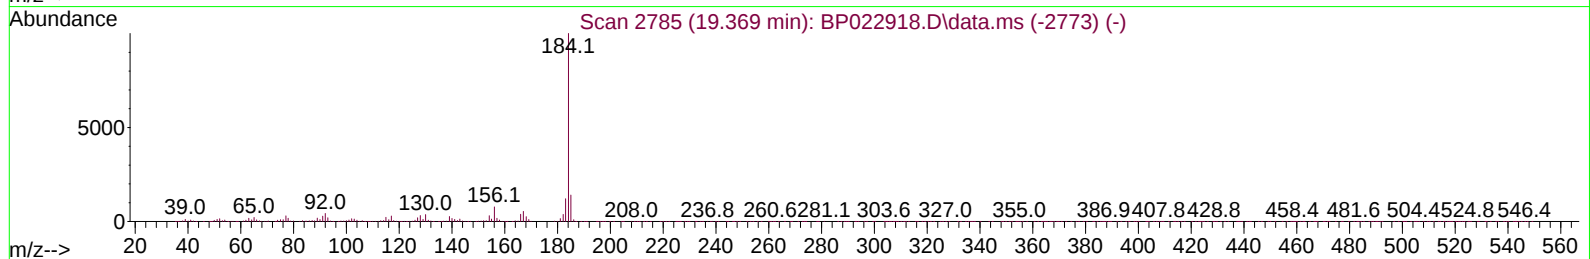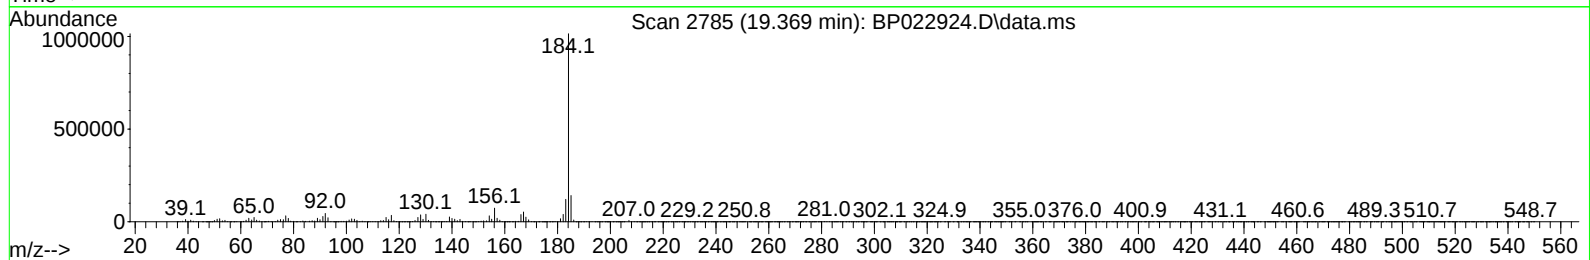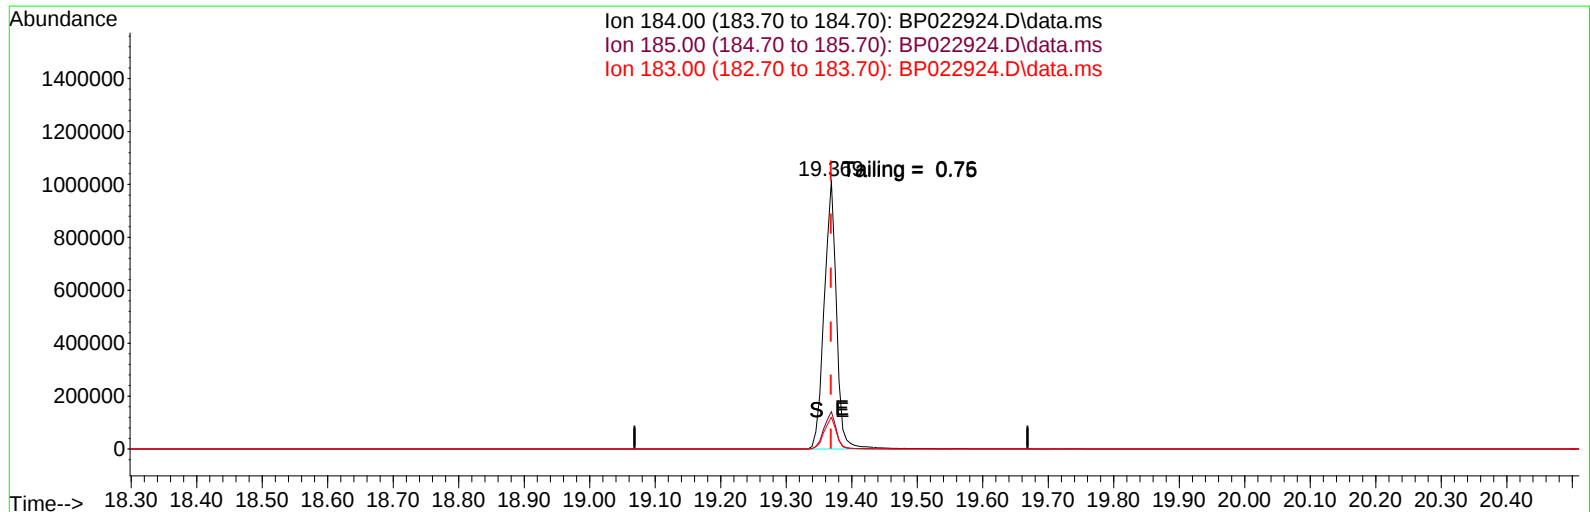

TIC: BP022924.D\data.ms

(77) Benzidine**19.369min (+ 0.000) 215863.04 ng****response 1326442**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.10	13.96
183.00	12.10	11.90
0.00	0.00	0.00