
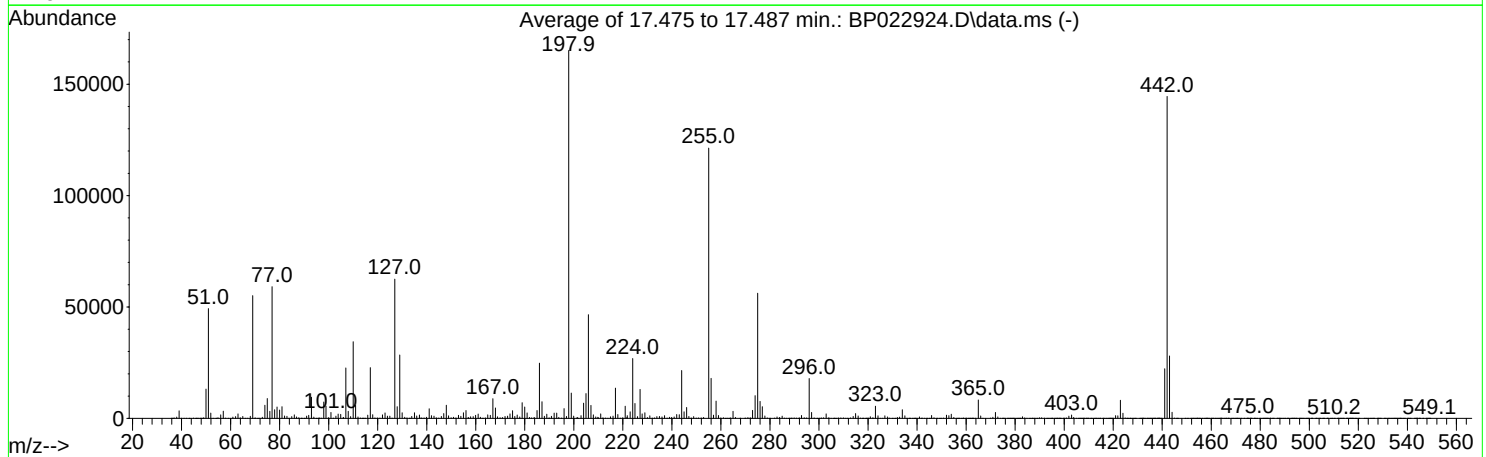


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110824\
Data File : BP022924.D
Acq On : 08 Nov 2024 07:13
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP110724.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Nov 07 23:36:11 2024

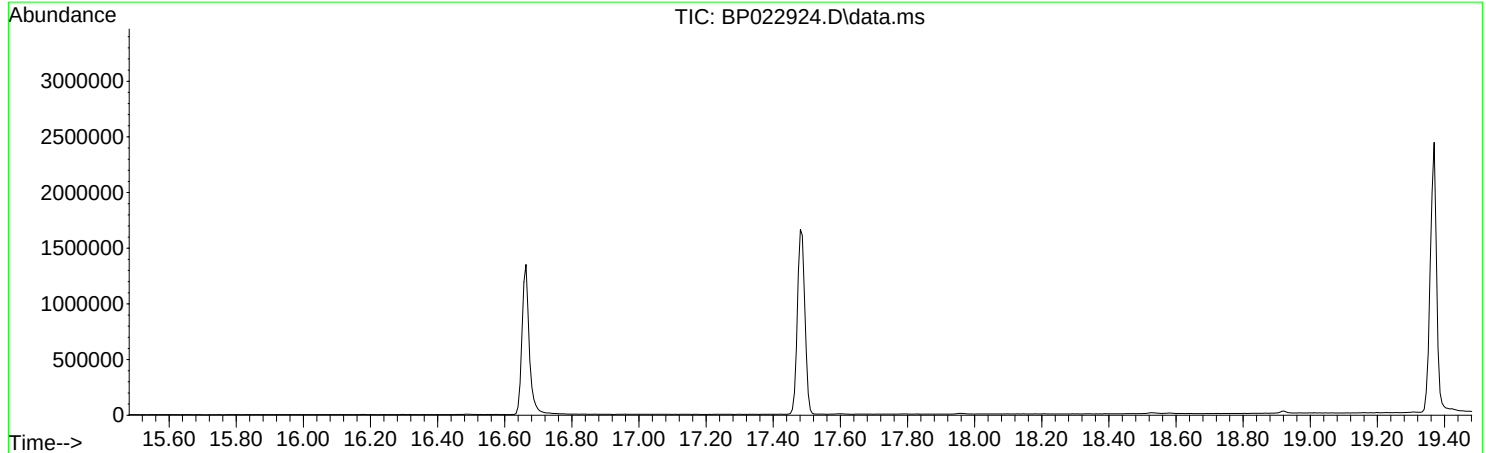

AutoFind: Scans 2463, 2464, 2465; Background Corrected with Scan 2454

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	29.8	49287	PASS
68	69	0.00	2	1.8	973	PASS
69	198	0.00	100	33.4	55133	PASS
70	69	0.00	2	0.5	255	PASS
127	198	10	80	37.8	62479	PASS
197	198	0.00	2	0.5	859	PASS
198	198	100	100	100.0	165139	PASS
199	198	5	9	6.9	11355	PASS
275	198	10	60	34.0	56149	PASS
365	198	1	100	5.0	8239	PASS
441	198	0.01	100	13.5	22246	PASS
442	442	100	100	100.0	144493	PASS
443	442	15	24	19.4	28043	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
11/8/2024	BNA_P	<u>BP022924.D</u>
Compound Name	Response	Retention Time
DDT	772806	20.651
DDD	10698	20.239
DDE	654	19.669
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
11352	784158	1.45

Instrument :
BNA_P
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110824\
Data File : BP022924.D
Acq On : 08 Nov 2024 07:13
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Nov 09 04:03:48 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP110724.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 07 23:36:11 2024
Response via : Initial Calibration

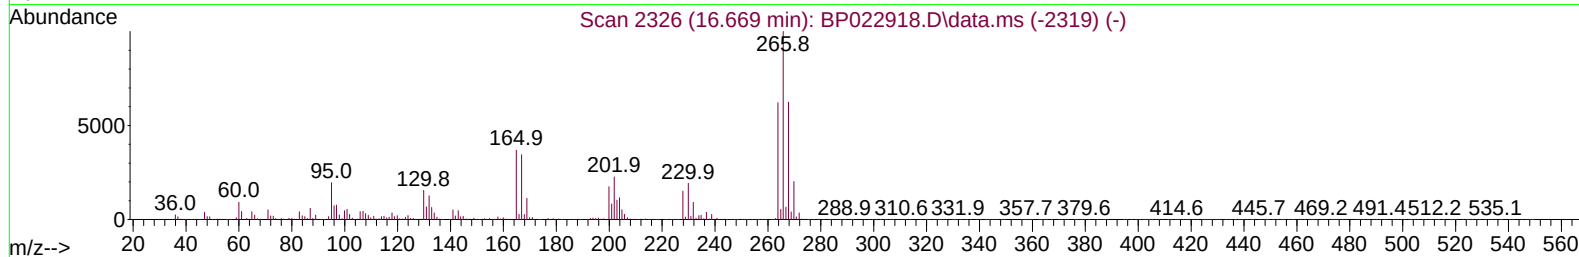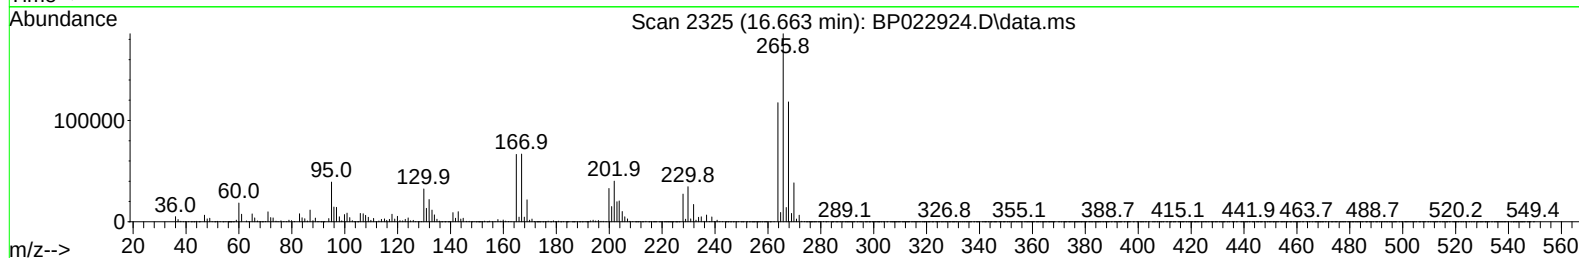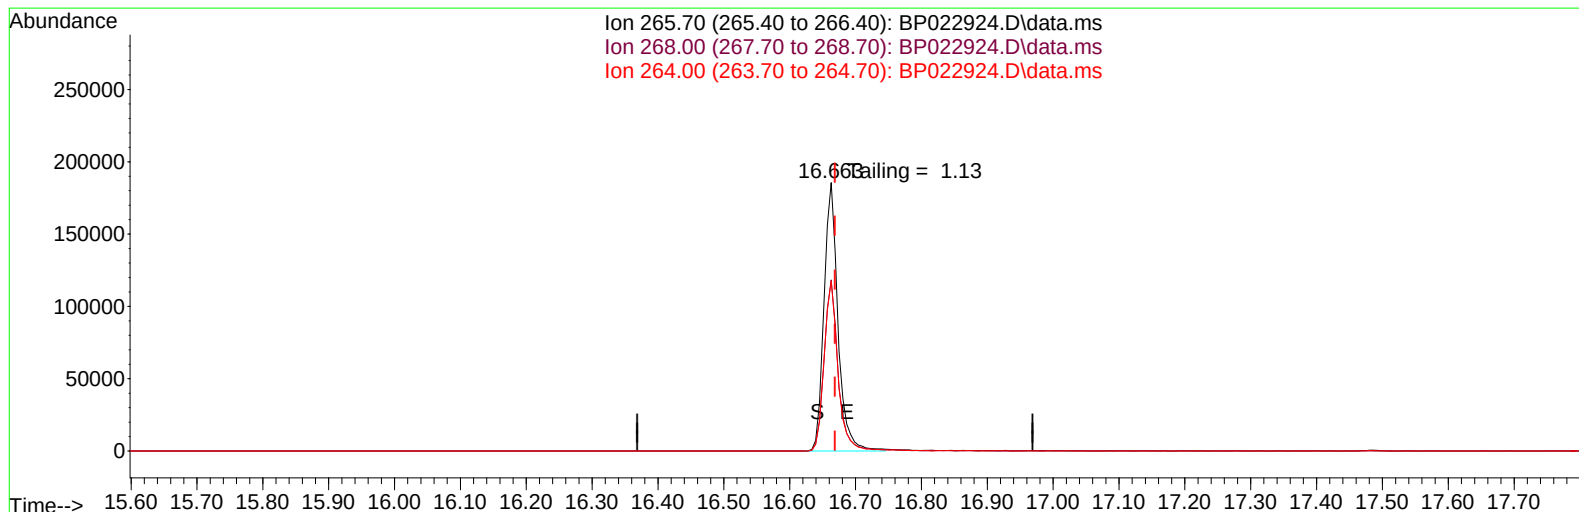

TIC: BP022924.D\data.ms

(70) Pentachlorophenol (C)

16.663min (-0.006) 2009783.57 ng




response 276055

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.40	63.75
264.00	62.10	63.36
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110824\
Data File : BP022924.D
Acq On : 08 Nov 2024 07:13
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Nov 09 04:03:48 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP110724.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 07 23:36:11 2024
Response via : Initial Calibration

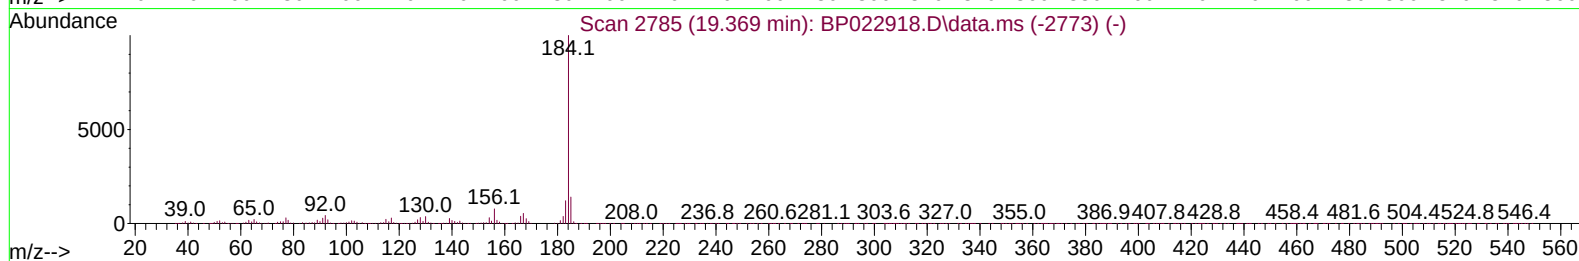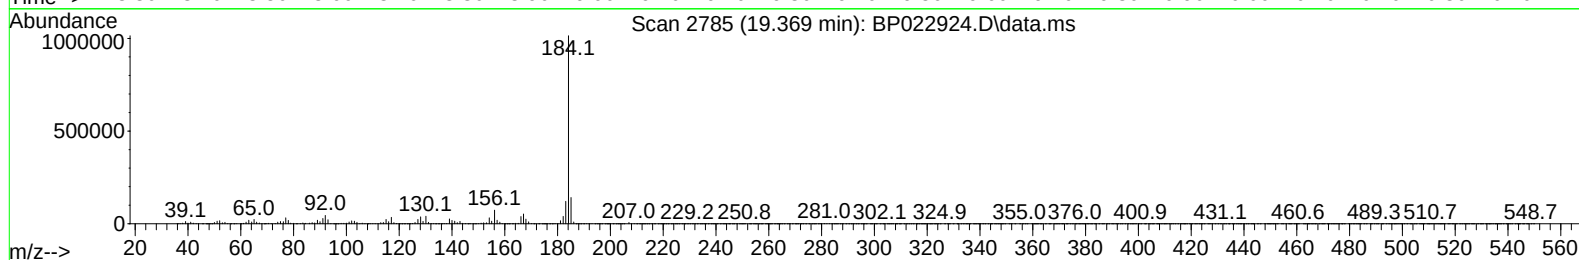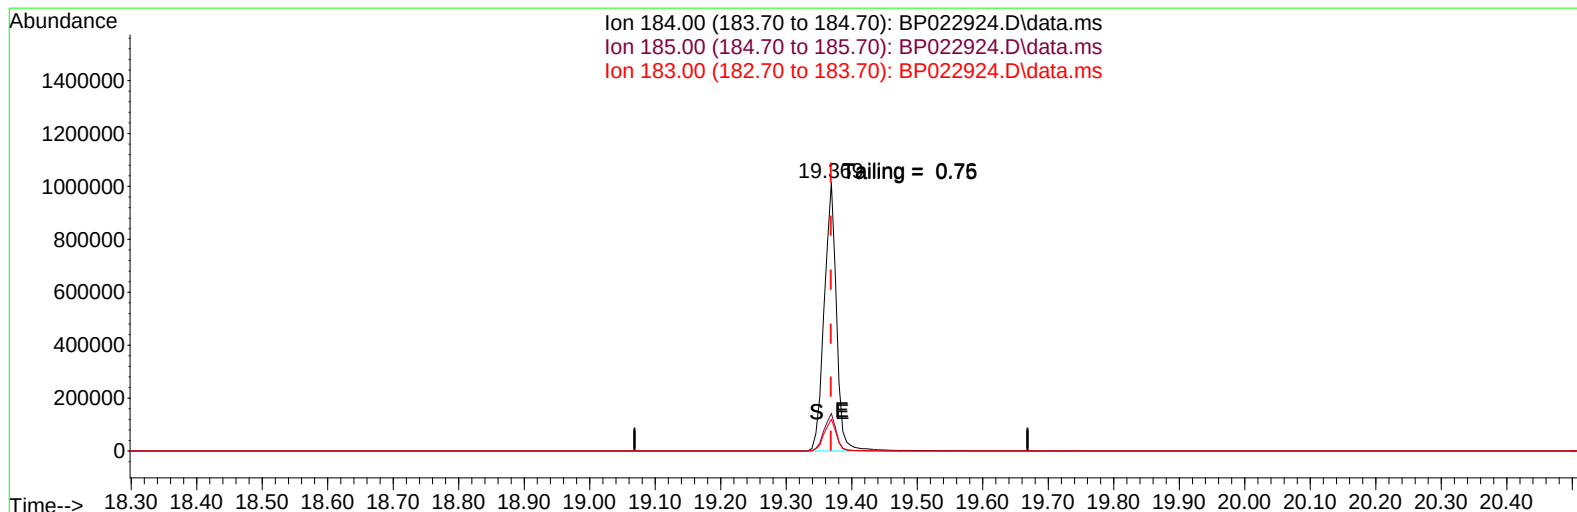

TIC: BP022924.D\data.ms

(77) Benzidine

19.369min (+ 0.000) 215863.04 ng

response 1326442

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.10	13.96
183.00	12.10	11.90
0.00	0.00	0.00