
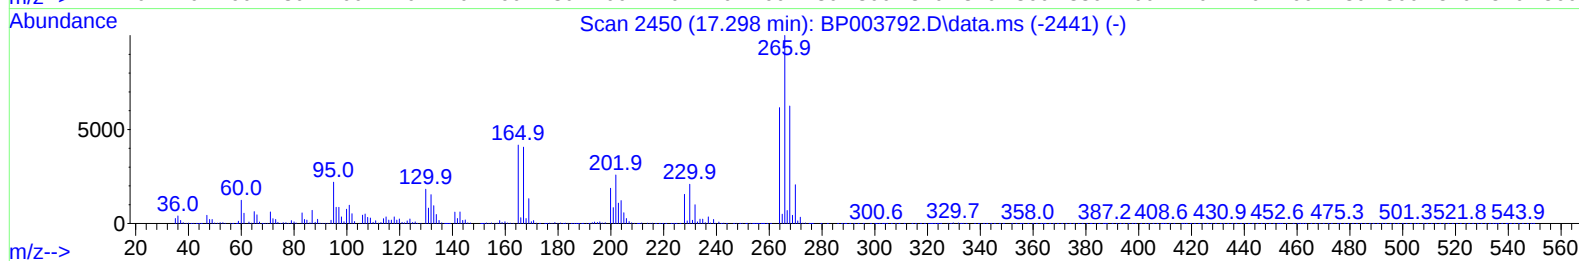
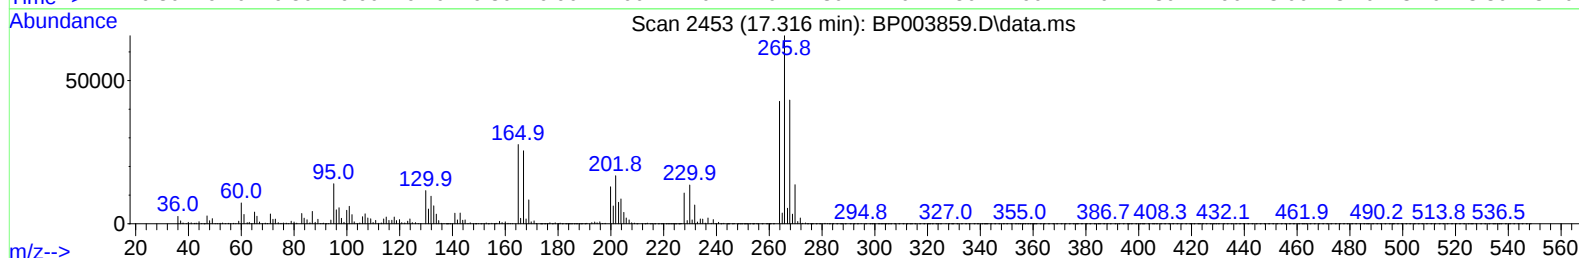


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110920\
Data File : BP003859.D
Acq On : 09 Nov 2020 09:56
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 10 06:17:32 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP110320.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 06 11:33:14 2020
Response via : Initial Calibration

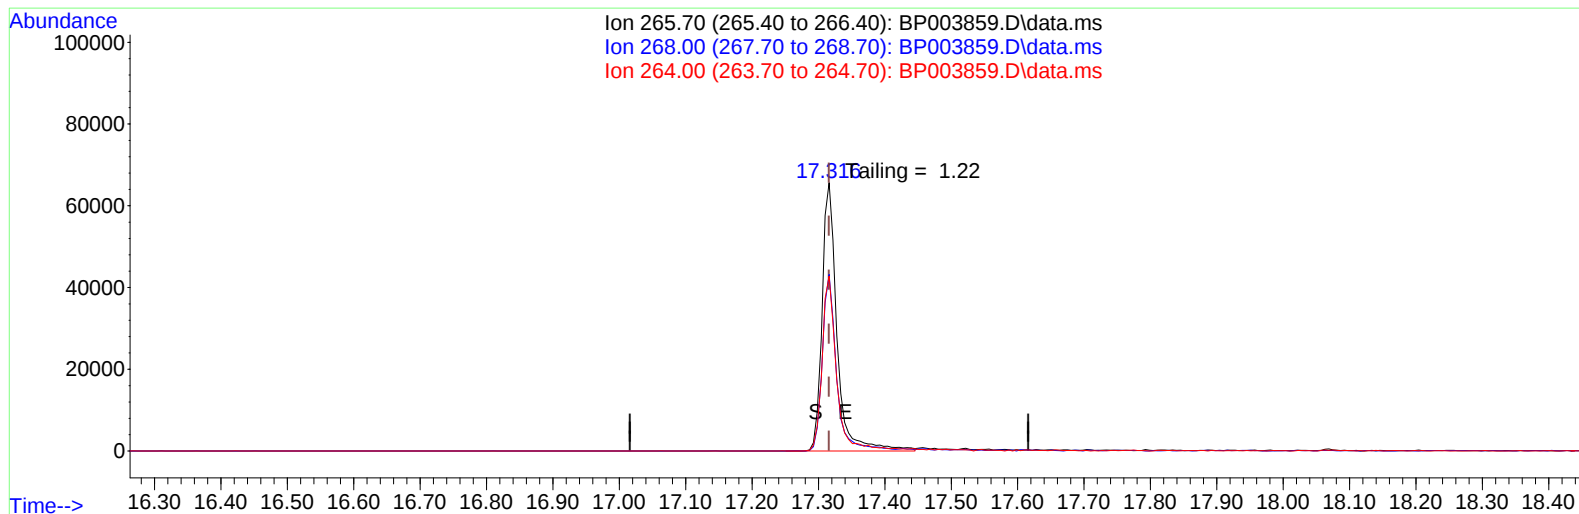

TIC: BP003859.D\data.ms

(70) Pentachlorophenol (C)




17.316min (+ 0.000) 39408.66 ng

response 103189

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.90	65.79
264.00	63.30	65.14
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110920\
Data File : BP003859.D
Acq On : 09 Nov 2020 09:56
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 10 06:17:32 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP110320.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 06 11:33:14 2020
Response via : Initial Calibration

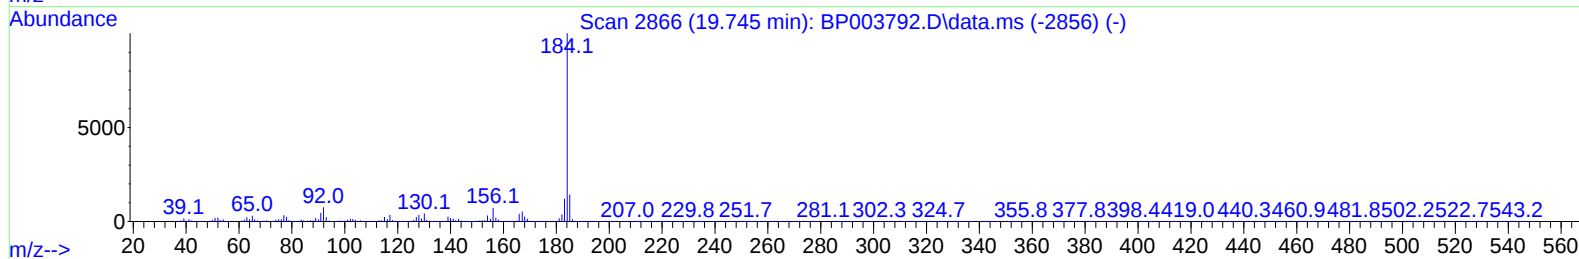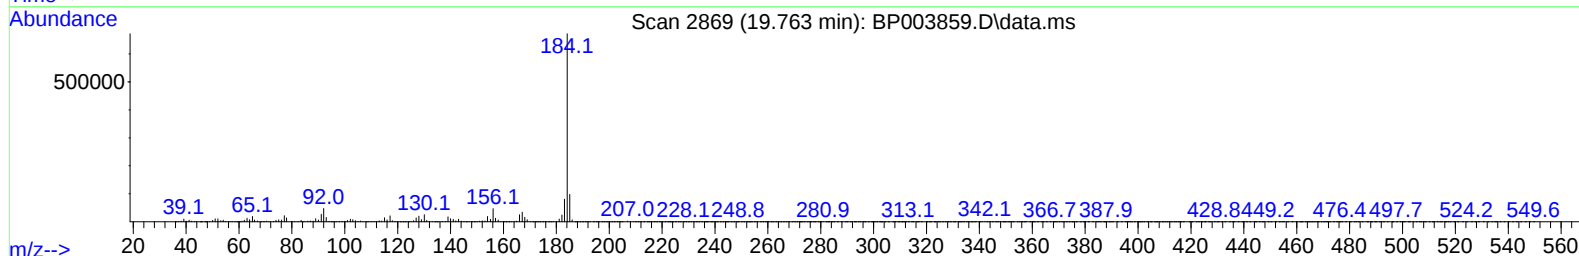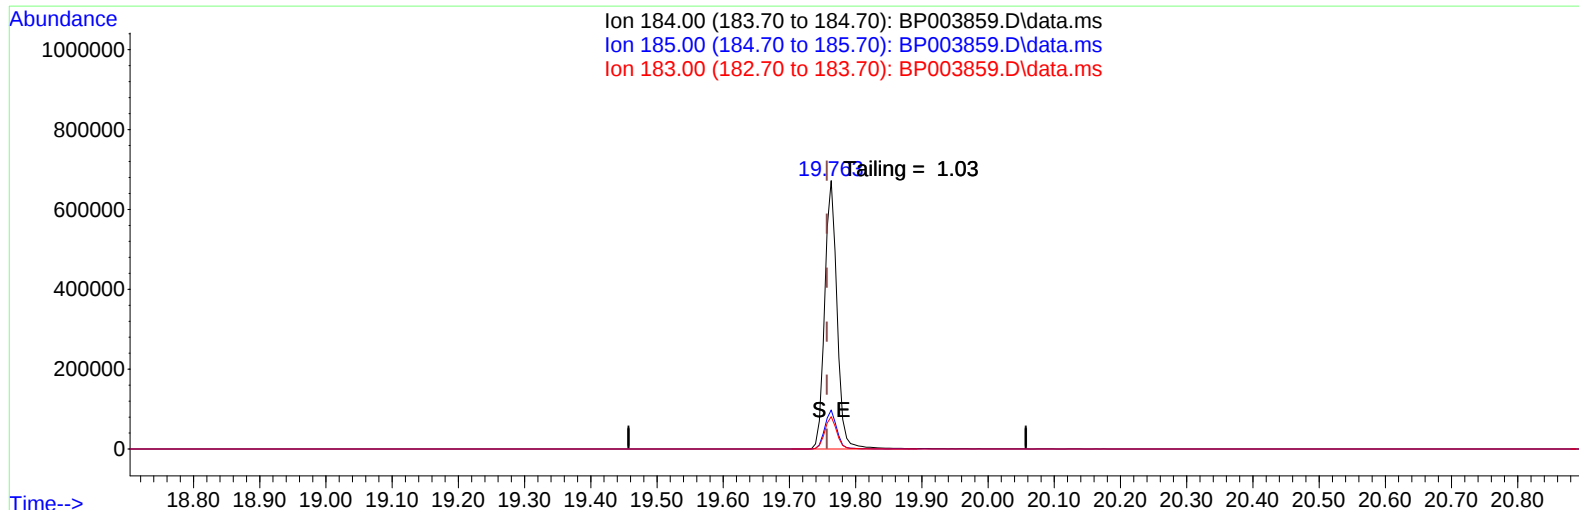

TIC: BP003859.D\data.ms

(77) Benzidine

19.763min (+ 0.006) 46177.47 ng

response 871372

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	14.55
183.00	12.00	12.04
0.00	0.00	0.00