
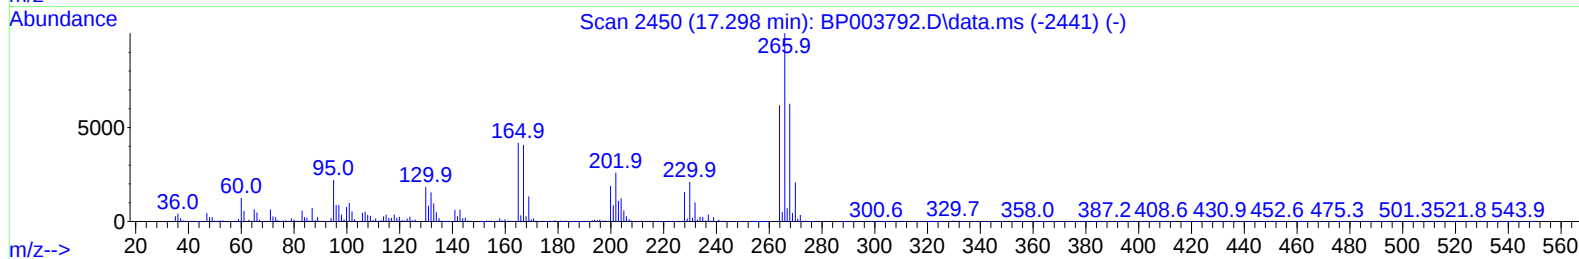
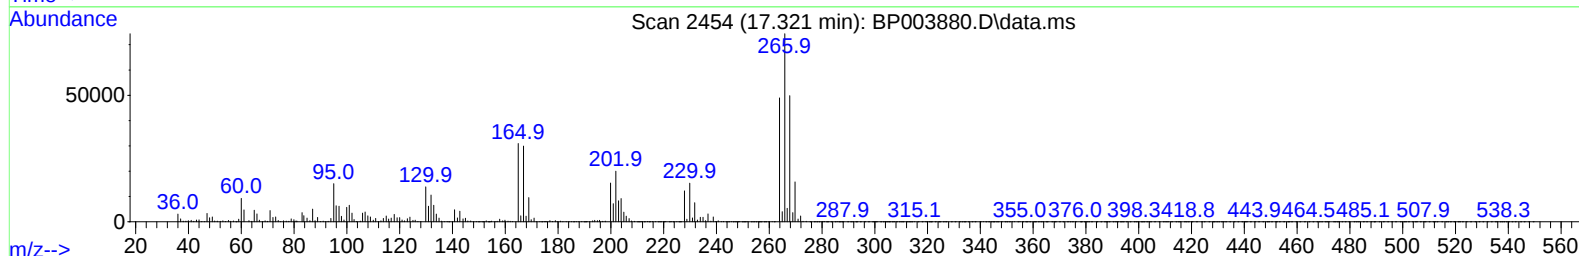


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110920\
Data File : BP003880.D
Acq On : 09 Nov 2020 23:37
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 10 06:39:13 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP110320.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 06 11:33:14 2020
Response via : Initial Calibration

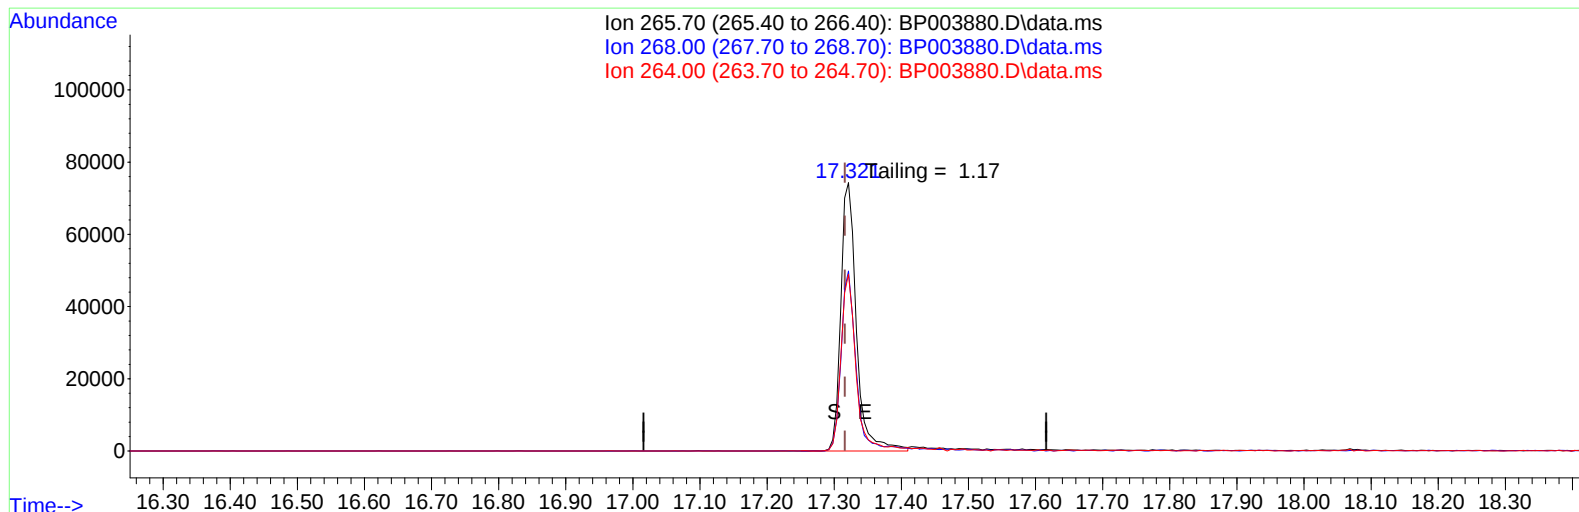

TIC: BP003880.D\data.ms

(70) Pentachlorophenol (C)




17.321min (+ 0.005) 48007.76 ng

response 120493

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.90	67.08
264.00	63.30	65.90
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110920\
 Data File : BP003880.D
 Acq On : 09 Nov 2020 23:37
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 10 06:39:13 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP110320.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Nov 06 11:33:14 2020
 Response via : Initial Calibration

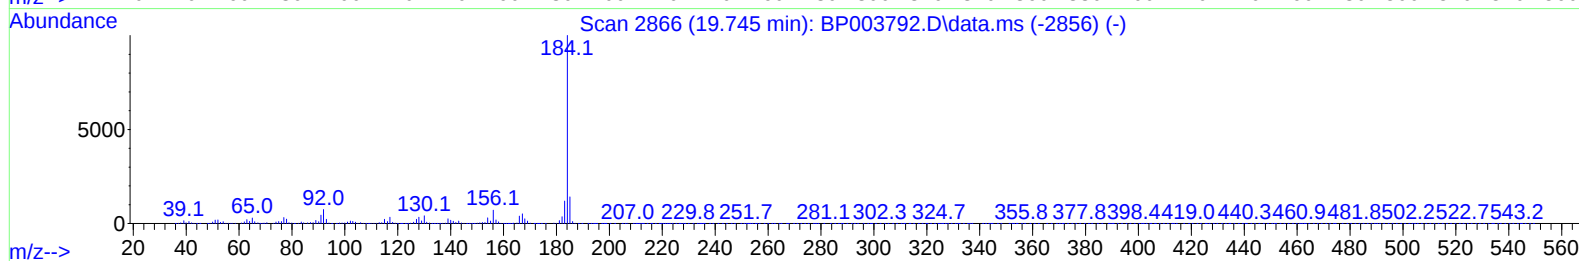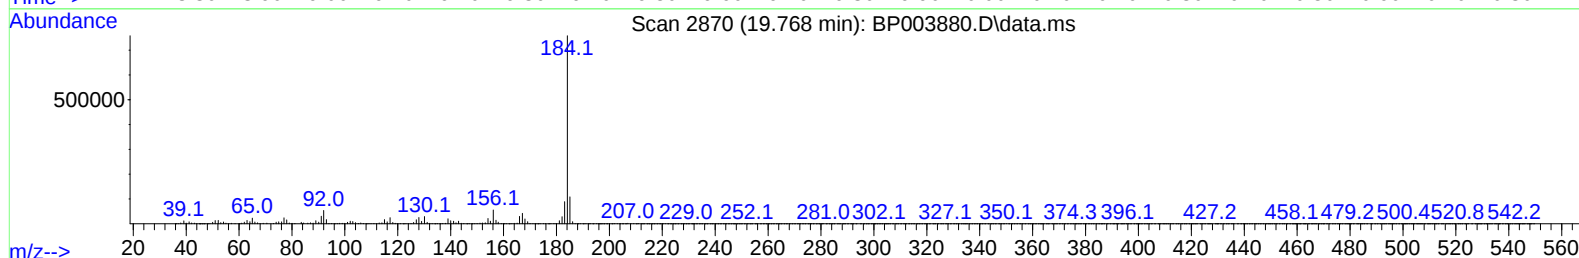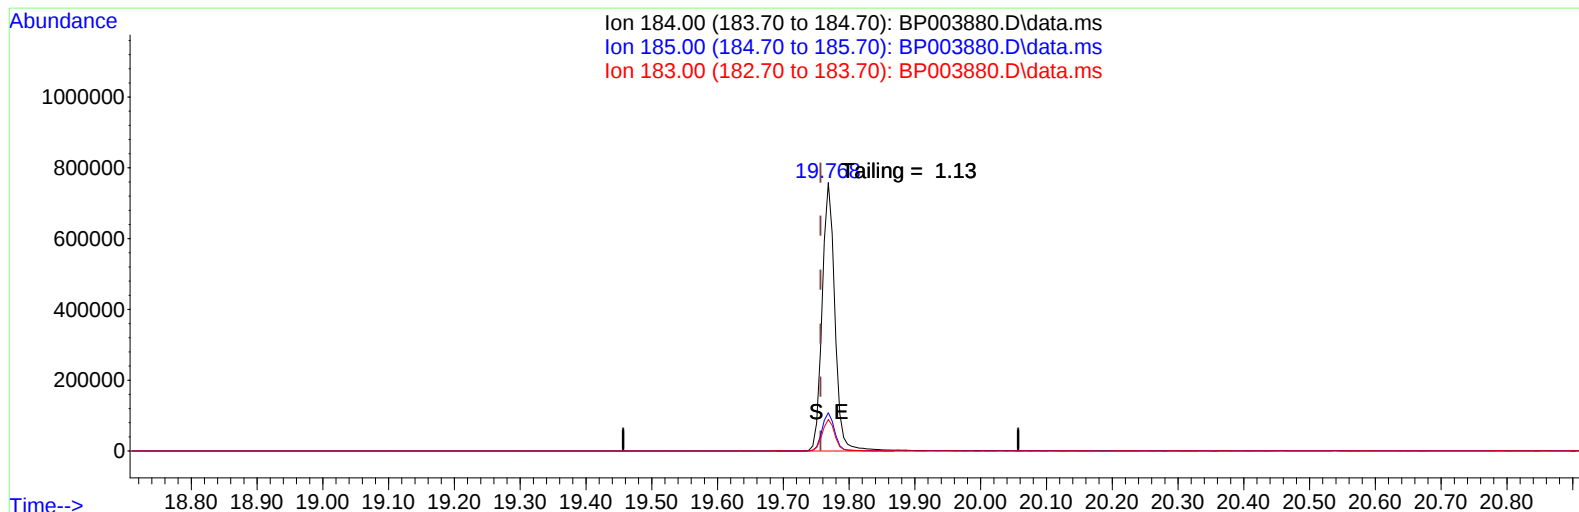

TIC: BP003880.D\data.ms

(77) Benzidine**19.768min (+ 0.011) 19200.94 ng****response 1021298**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	14.26
183.00	12.00	11.74
0.00	0.00	0.00