

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110920\
 Data File : BP003861.D
 Acq On : 09 Nov 2020 11:04
 Operator : CG/JU
 Sample : PB132870BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 PB132870BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP110320.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP003861.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.952	6	11	30	rVB	13143277	16254906	100.00%	26.946%
2	5.822	492	499	511	rBV	3661532	5301511	32.61%	8.788%
3	7.469	770	779	795	rBV	3268465	5249007	32.29%	8.701%
4	8.298	912	920	929	rBV	658028	1056751	6.50%	1.752%
5	9.463	1108	1118	1130	rBV	2073178	3452980	21.24%	5.724%
6	11.134	1393	1402	1418	rBV	810602	1361559	8.38%	2.257%
7	13.545	1804	1812	1826	rBV	4732816	6973885	42.90%	11.561%
8	14.916	2037	2045	2061	rBV	1095197	1659704	10.21%	2.751%
9	16.398	2288	2297	2321	rBV	3282842	4784510	29.43%	7.931%
10	17.645	2502	2509	2521	rBV	1321611	1817819	11.18%	3.013%
11	20.139	2927	2933	2941	rBV	7445458	8903729	54.78%	14.760%
12	21.668	3187	3193	3201	rBV	1354424	1808192	11.12%	2.997%
13	24.145	3607	3614	3628	rVB	846851	1699700	10.46%	2.818%




Sum of corrected areas: 60324253

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110920\
Data File : BP003861.D
Acq On : 09 Nov 2020 11:04
Operator : CG/JU
Sample : PB132870BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB132870BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP110320.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

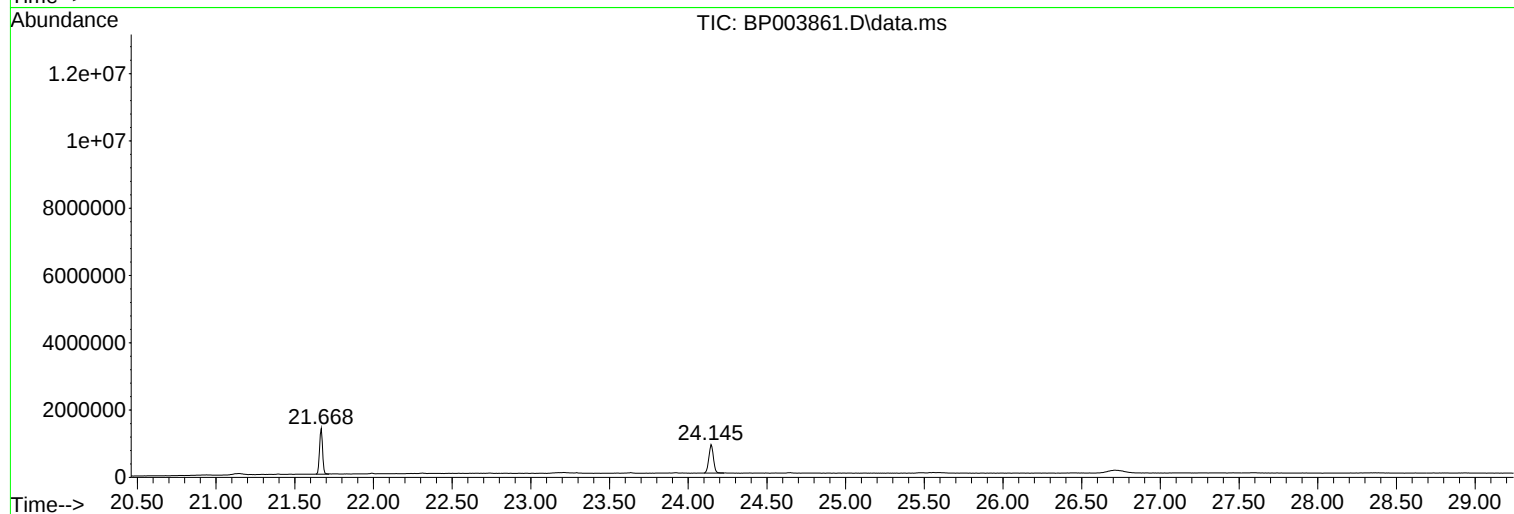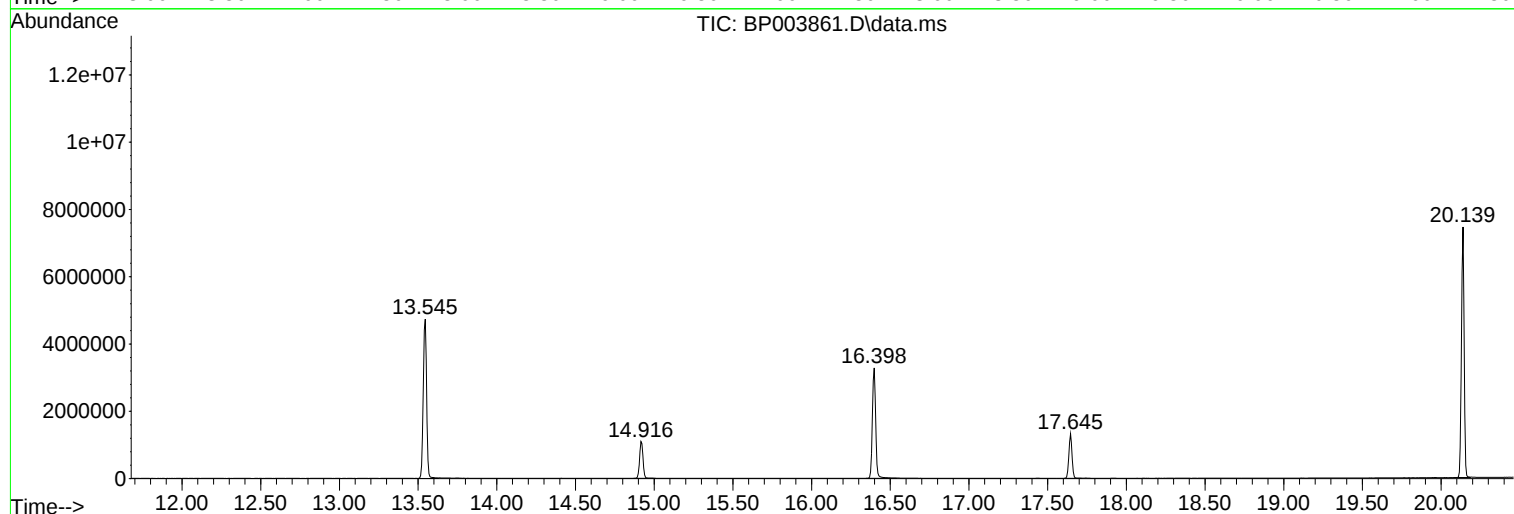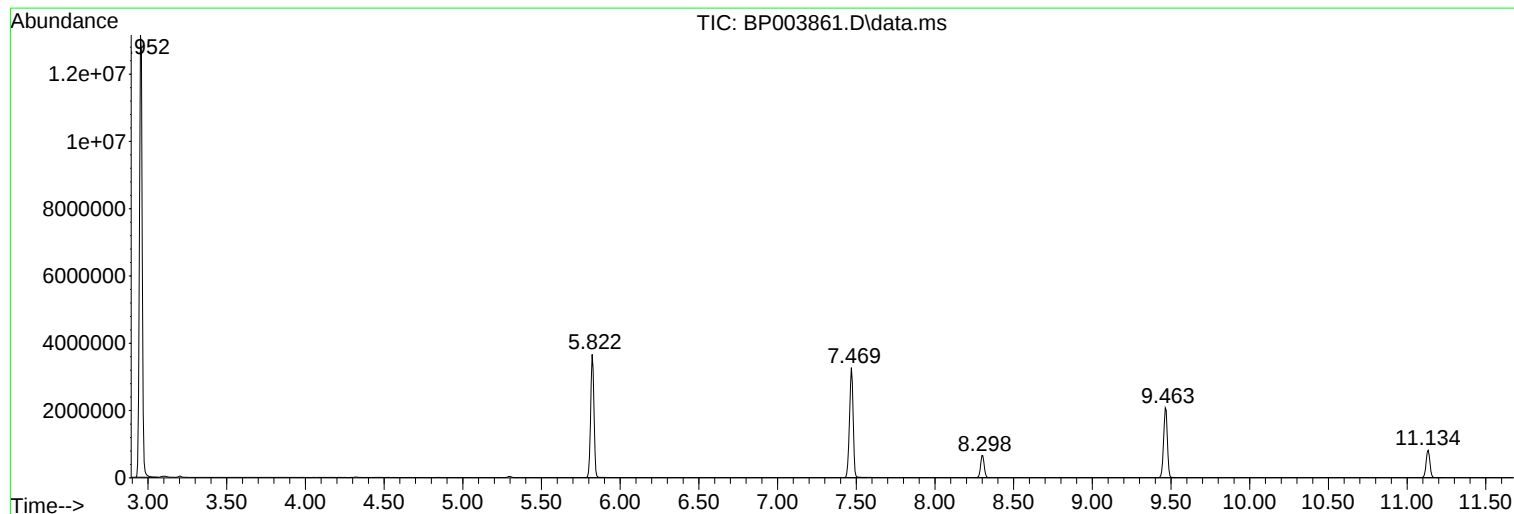

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110920\
Data File : BP003861.D
Acq On : 09 Nov 2020 11:04
Operator : CG/JU
Sample : PB132870BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB132870BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP110320.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110920\
Data File : BP003861.D
Acq On : 09 Nov 2020 11:04
Operator : CG/JU
Sample : PB132870BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB132870BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP110320.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------