

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110920\
 Data File : BP003864.D
 Acq On : 09 Nov 2020 12:47
 Operator : CG/JU
 Sample : PB132858BL
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 PB132858BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP110320.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP003864.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.952	6	11	30	rVB	12004266	14468042	100.00%	25.331%
2	5.822	492	499	513	rBV	3335752	4861852	33.60%	8.512%
3	7.469	770	779	795	rBV	2997431	4846159	33.50%	8.485%
4	8.299	913	920	929	rVB	616595	968966	6.70%	1.696%
5	9.463	1109	1118	1127	rBV	1915872	3174481	21.94%	5.558%
6	11.134	1393	1402	1415	rBV	768399	1268294	8.77%	2.221%
7	13.545	1804	1812	1833	rBV	4404875	6567448	45.39%	11.498%
8	14.916	2037	2045	2057	rBV	1044618	1577689	10.90%	2.762%
9	16.398	2289	2297	2322	rBV	3192051	4678323	32.34%	8.191%
10	17.645	2502	2509	2520	rBV	1306510	1823312	12.60%	3.192%
11	20.139	2927	2933	2946	rBV	7854910	9186782	63.50%	16.084%
12	21.669	3188	3193	3208	rVB	1424785	1891790	13.08%	3.312%
13	24.151	3607	3615	3624	rBV	862566	1803731	12.47%	3.158%




Sum of corrected areas: 57116869

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110920\
Data File : BP003864.D
Acq On : 09 Nov 2020 12:47
Operator : CG/JU
Sample : PB132858BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB132858BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP110320.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

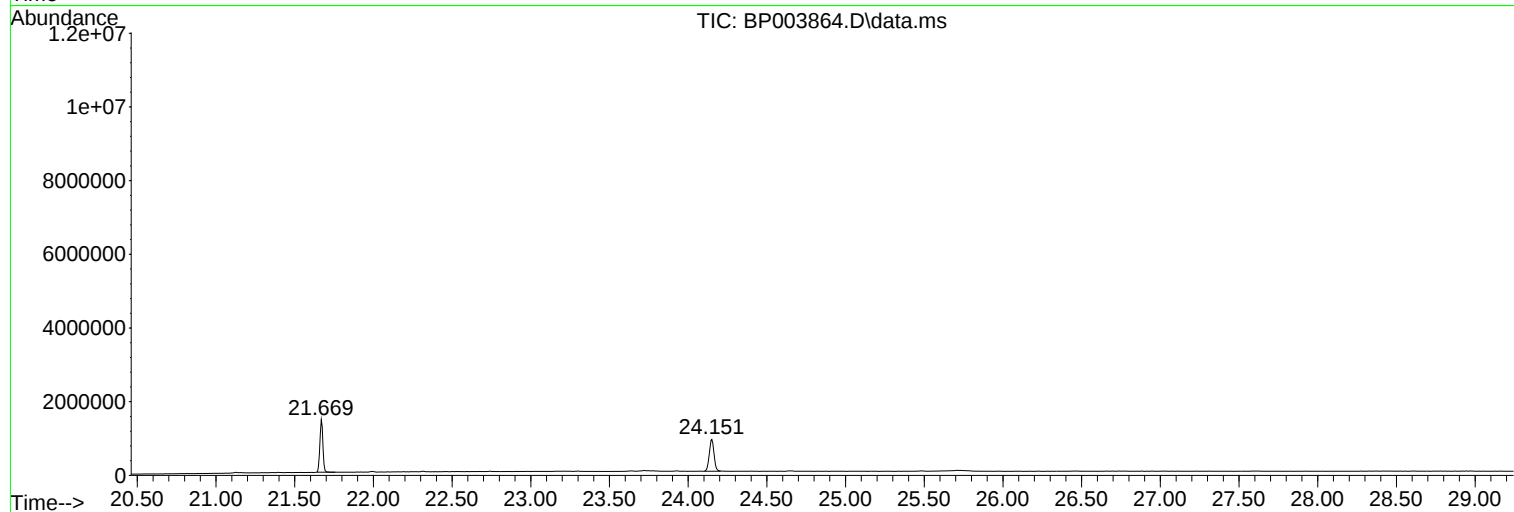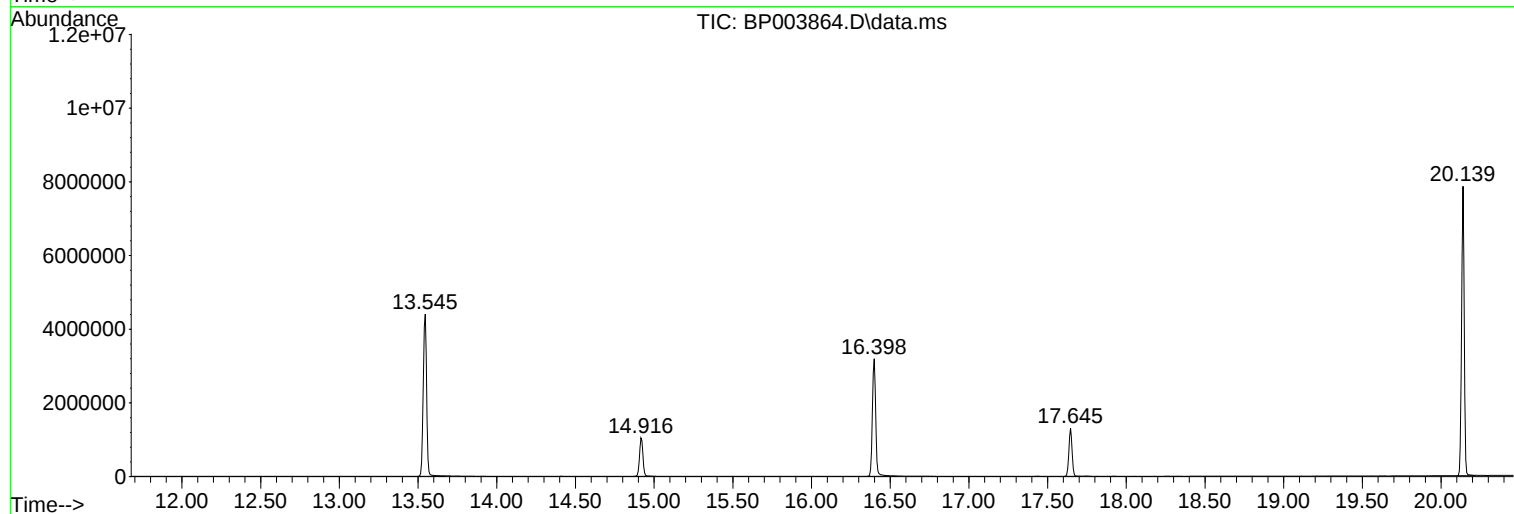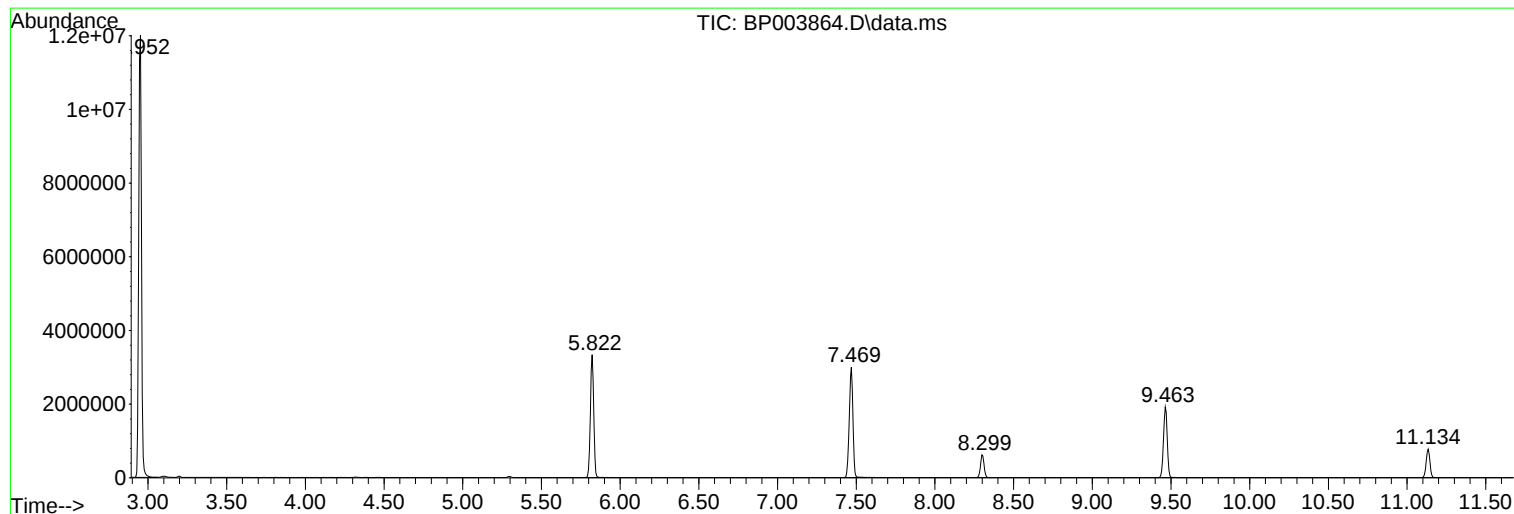

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110920\
Data File : BP003864.D
Acq On : 09 Nov 2020 12:47
Operator : CG/JU
Sample : PB132858BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB132858BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP110320.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110920\
Data File : BP003864.D
Acq On : 09 Nov 2020 12:47
Operator : CG/JU
Sample : PB132858BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB132858BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP110320.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
